



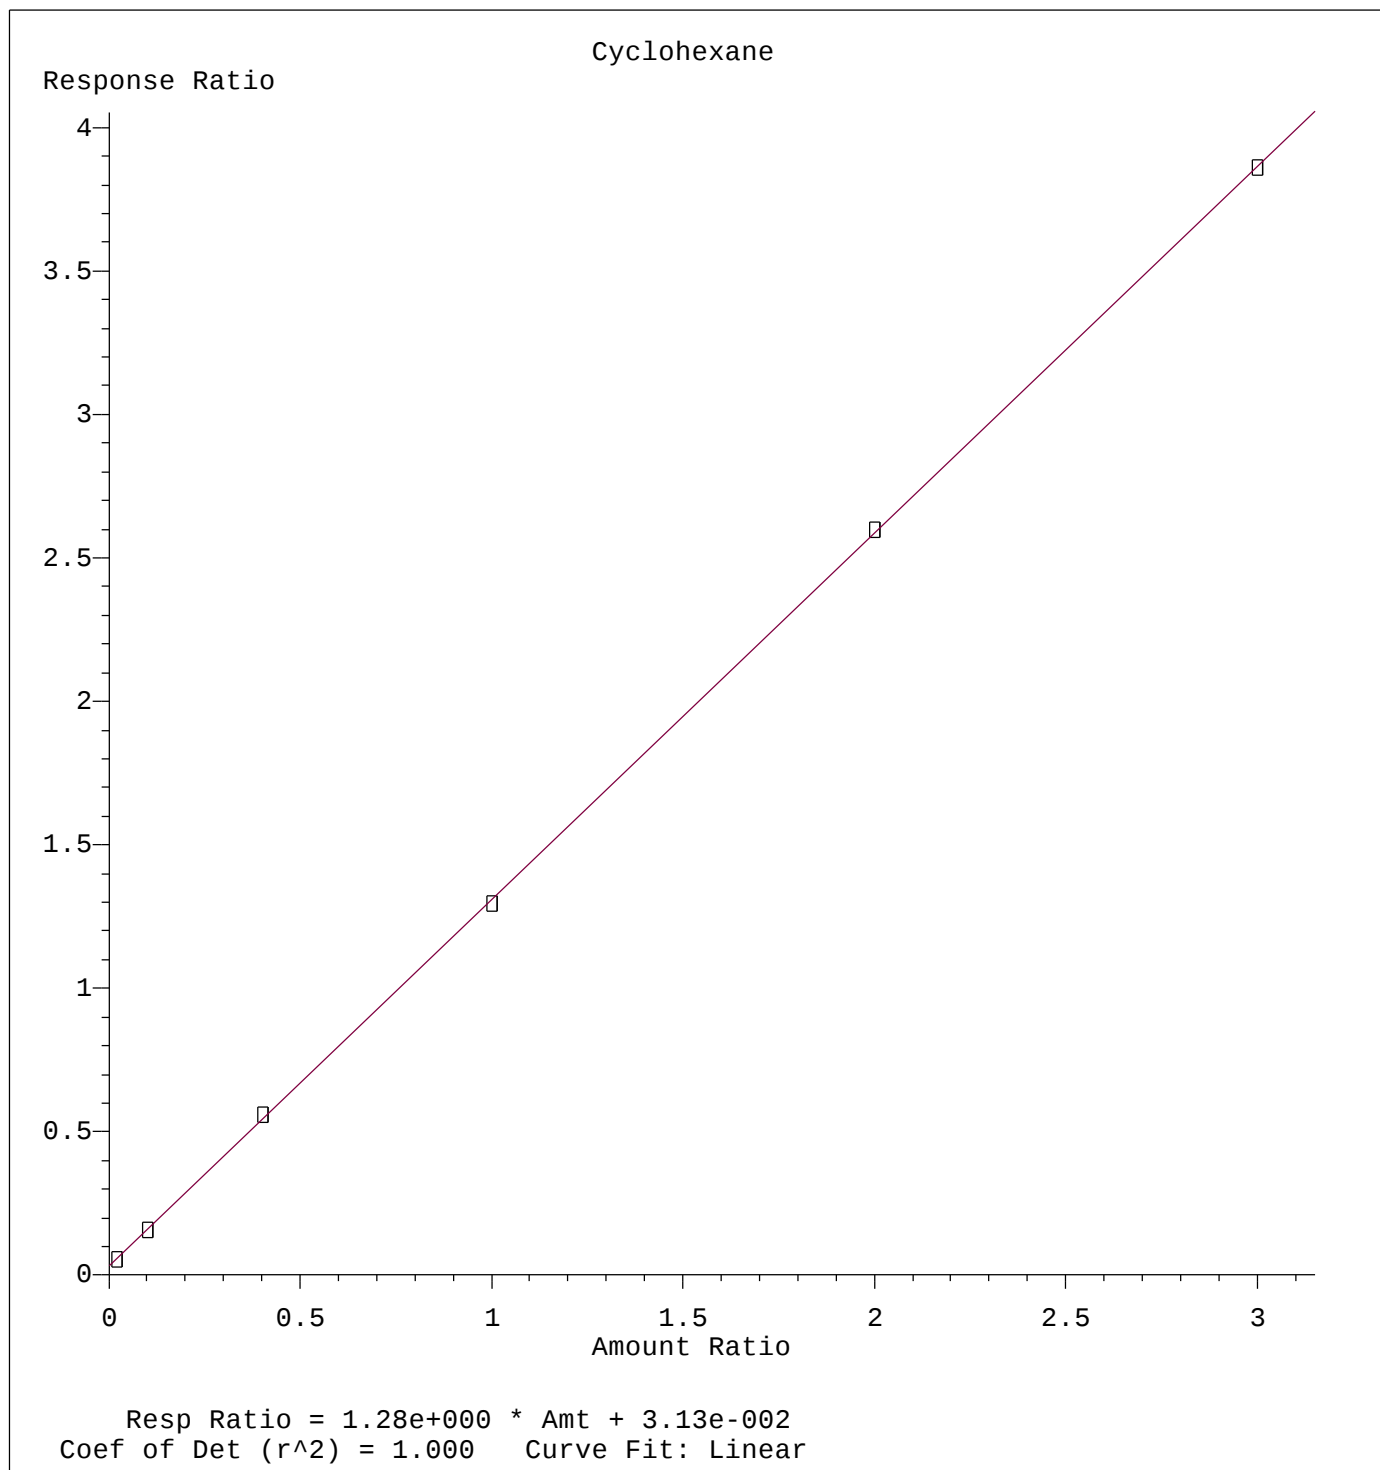

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Calibration Table Last Updated: Fri Dec 07 00:39:42 2018

trans-1,4-Dichloro-2-butene

Response Ratio

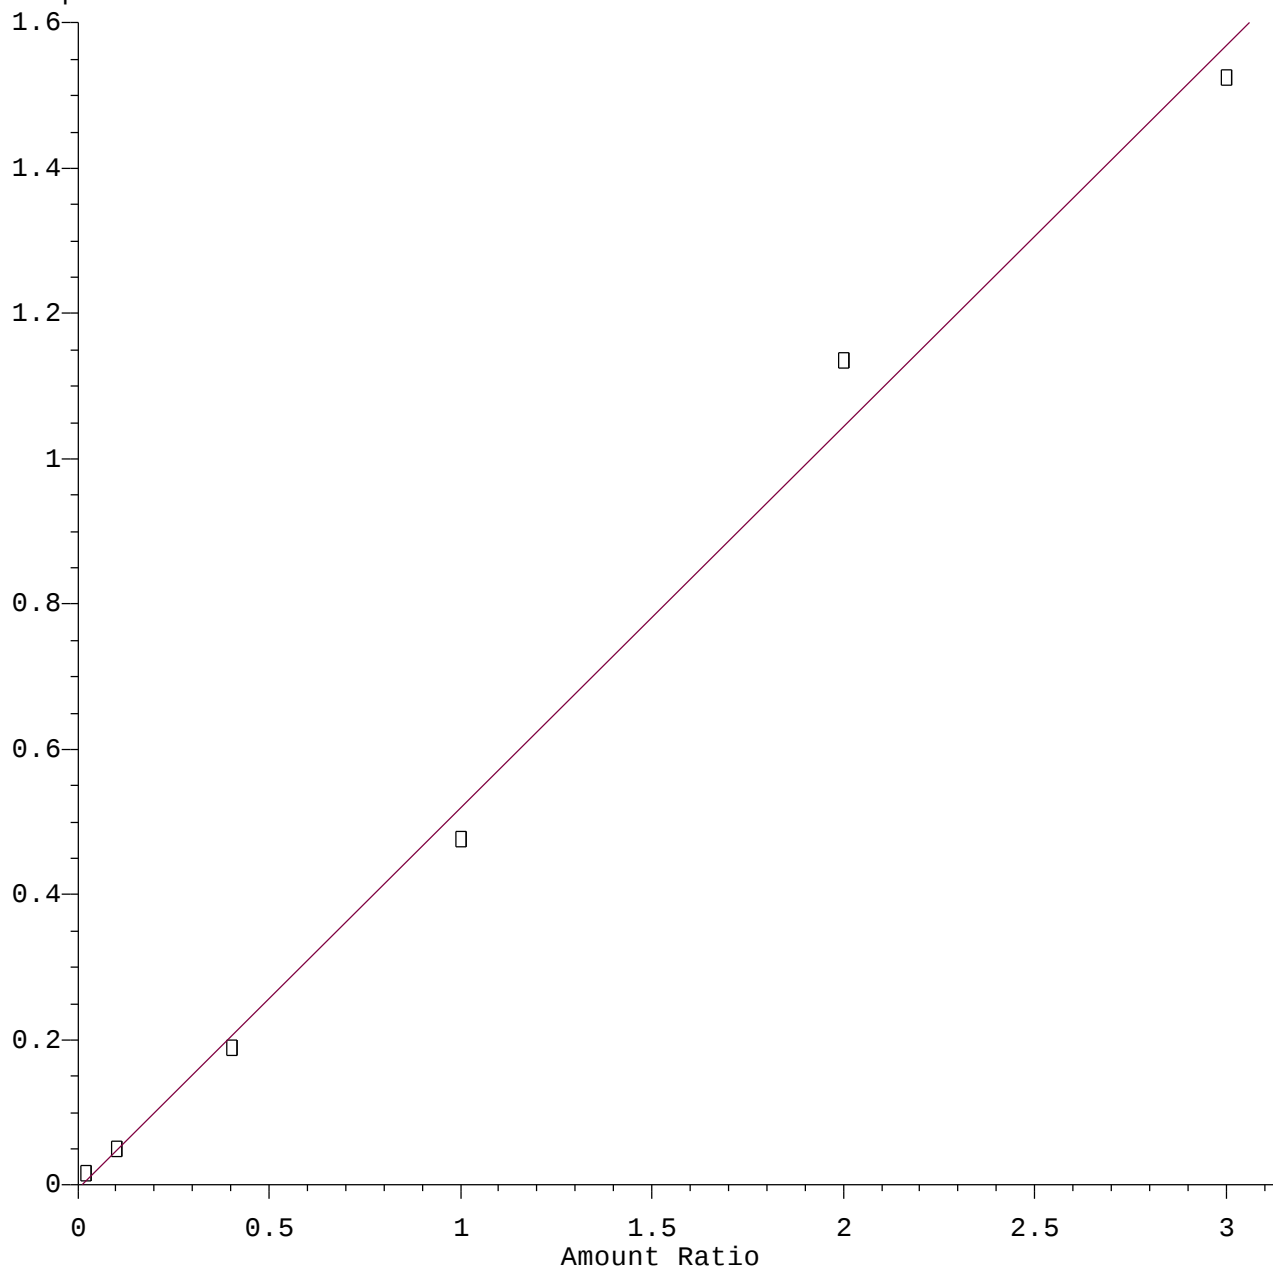


Resp Ratio = $5.25 \times 10^{-1} \times \text{Amt} - 5.50 \times 10^{-3}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Calibration Table Last Updated: Fri Dec 07 00:39:42 2018

1,2,4-Trichlorobenzene

Response Ratio

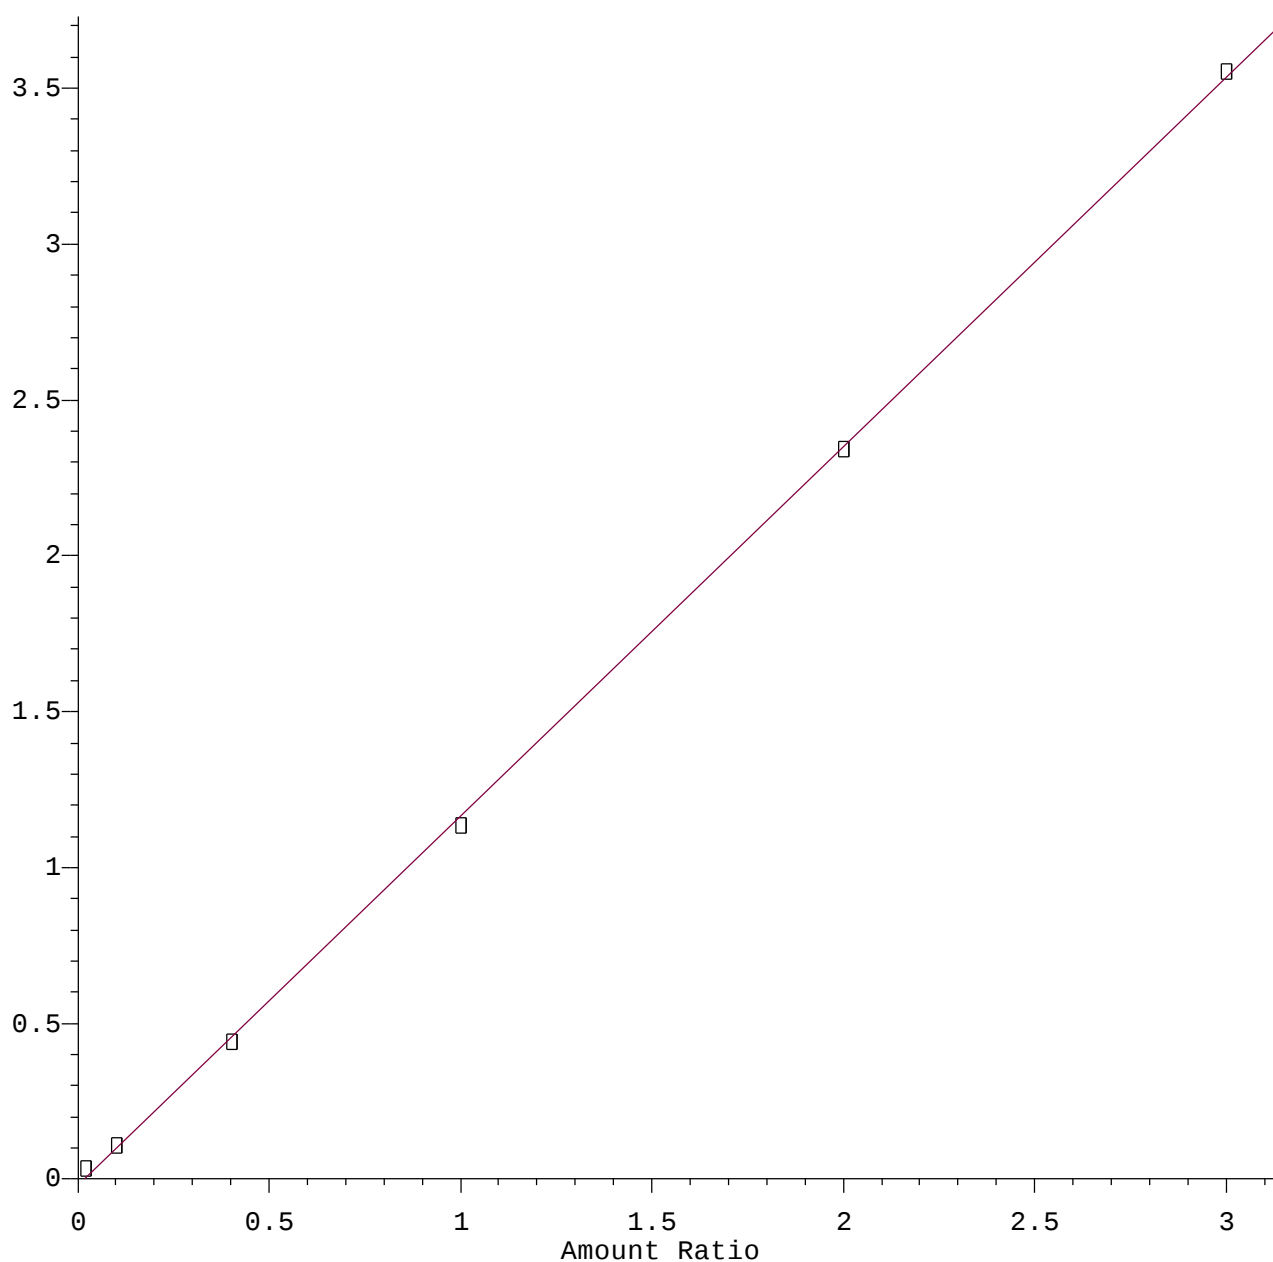


Resp Ratio = 1.18e+000 * Amt - 2.00e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Calibration Table Last Updated: Fri Dec 07 00:39:42 2018

1,2,3-Trichlorobenzene

Response Ratio

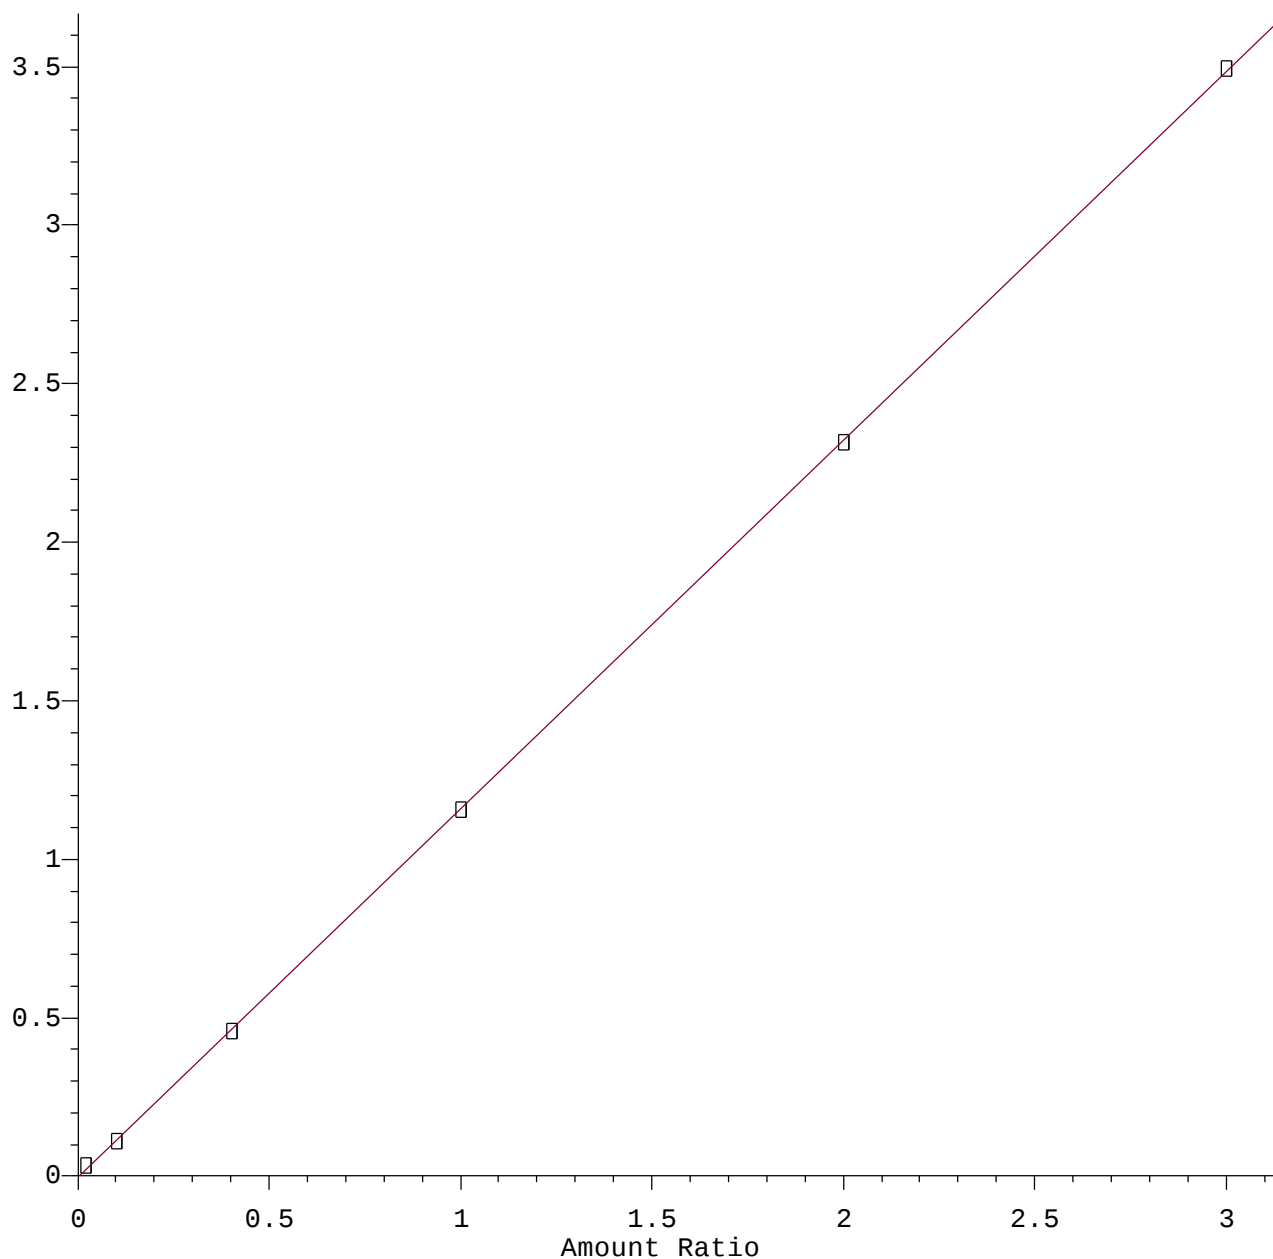

Resp Ratio = 1.16e+000 * Amt - 3.41e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Calibration Table Last Updated: Fri Dec 07 00:39:42 2018