


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120618\
Data File : VU028491.D
Acq On : 06 Dec 2018 10:54
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Title : SW846 8260
Last Update : Fri Dec 07 00:39:42 2018

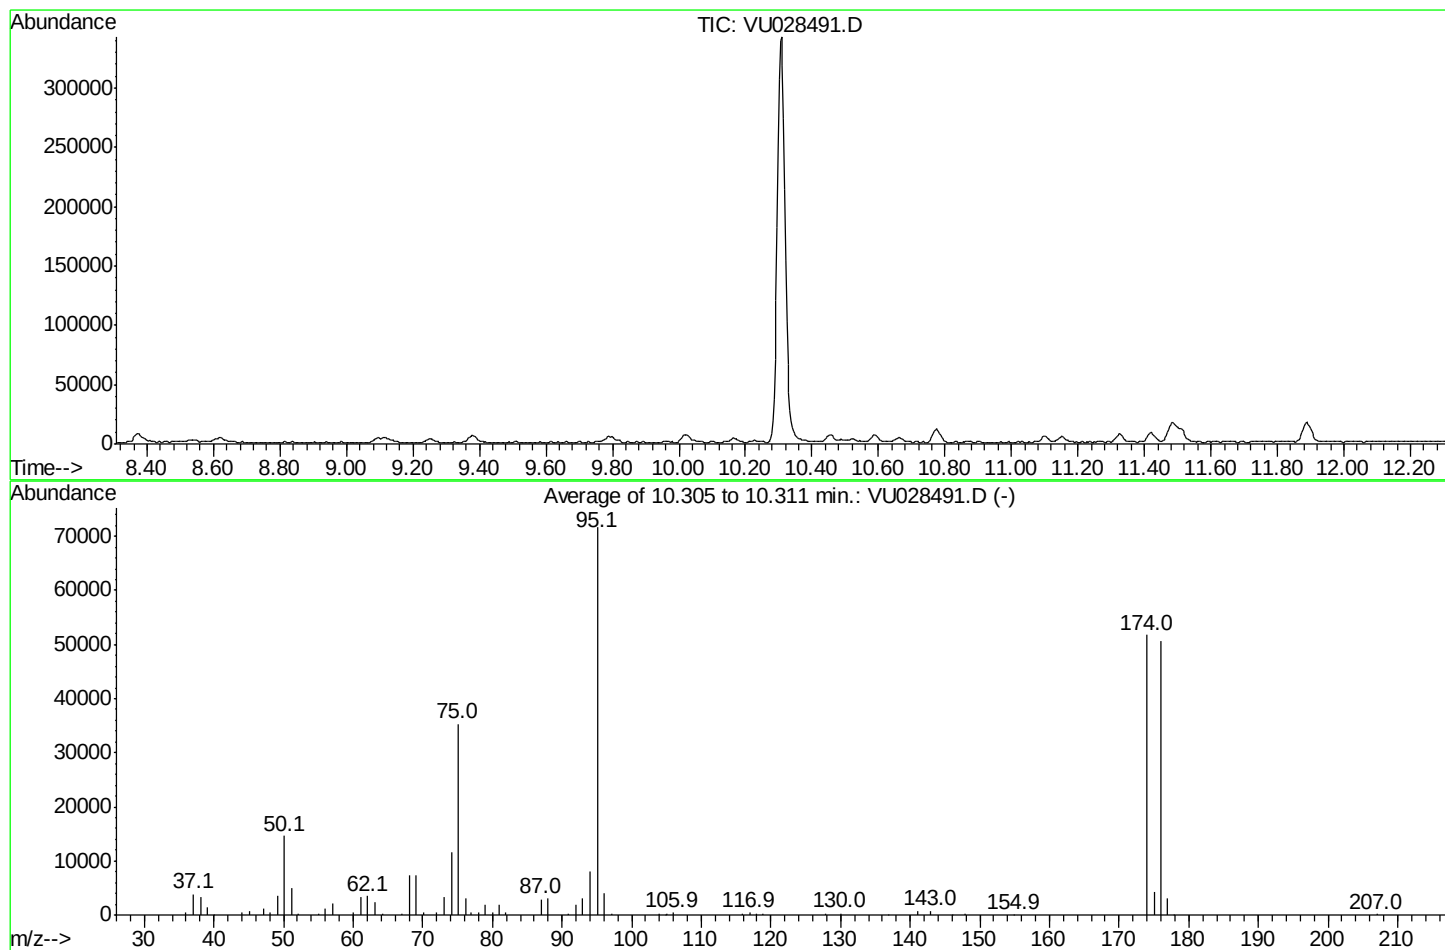

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	14616	PASS
75	95	30	60	49.4	35372	PASS
95	95	100	100	100.0	71664	PASS
96	95	5	9	5.8	4122	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.2	51722	PASS
175	174	5	9	8.1	4192	PASS
176	174	95	101	97.7	50552	PASS
177	176	5	9	5.9	2986	PASS