
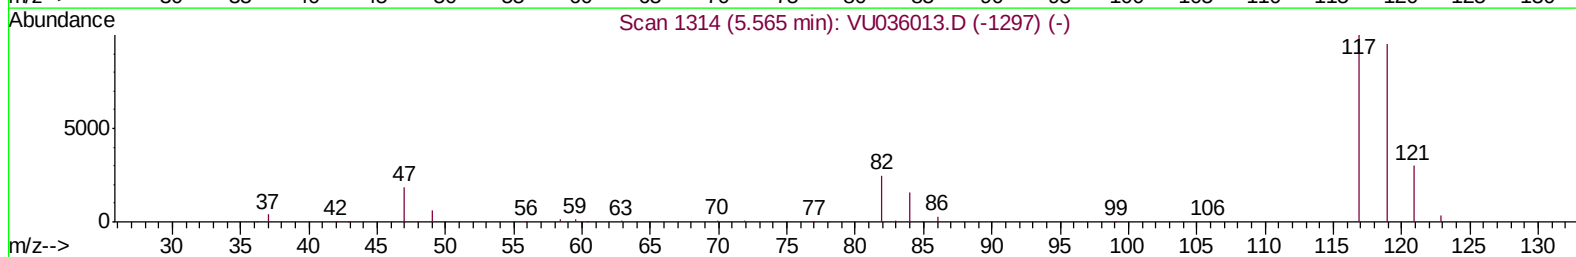
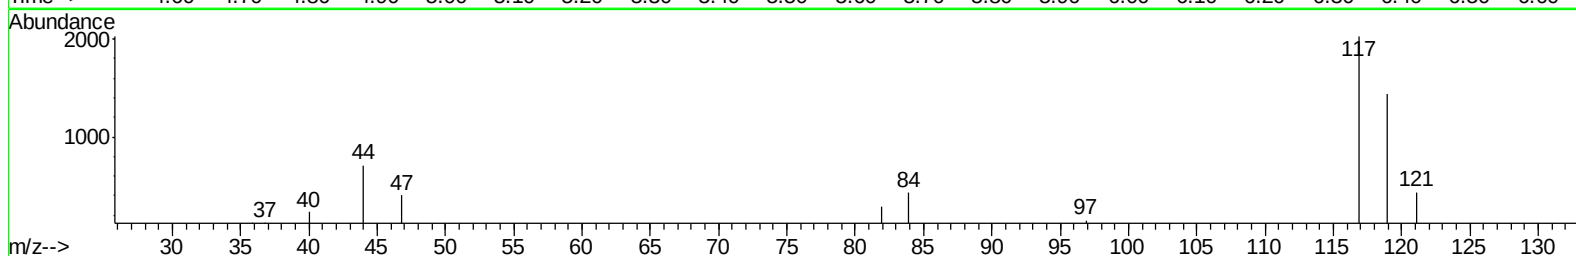


Data File : VU036031.D
Acq On : 06 Dec 2019 18:34
Operator : JC/SP
Sample : K6168-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 06 22:37:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 06 22:30:31 2019
Response via : Initial Calibration

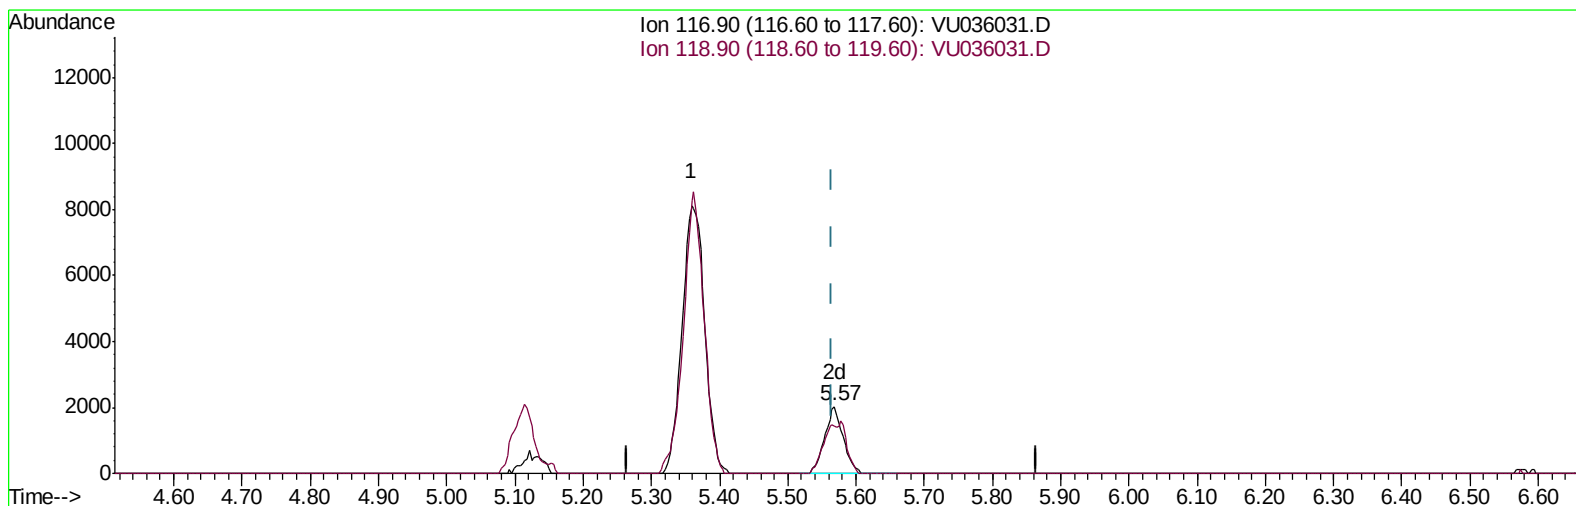

TIC: VU036031.D

(31) Carbon tetrachloride (T)

5.568min (+0.003) 0.11ug/L m

response 3762

Ion	Exp%	Act%
116.90	100	100
118.90	96.10	477.54#
0.00	0.00	0.00
0.00	0.00	0.00