
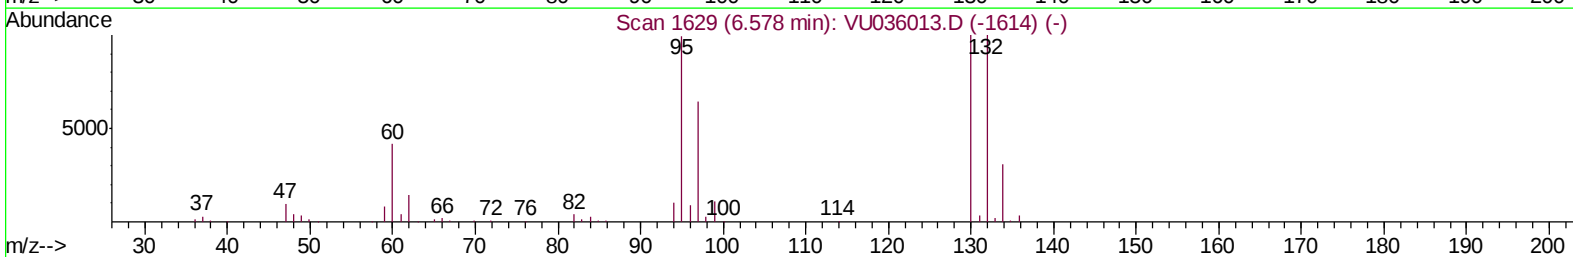
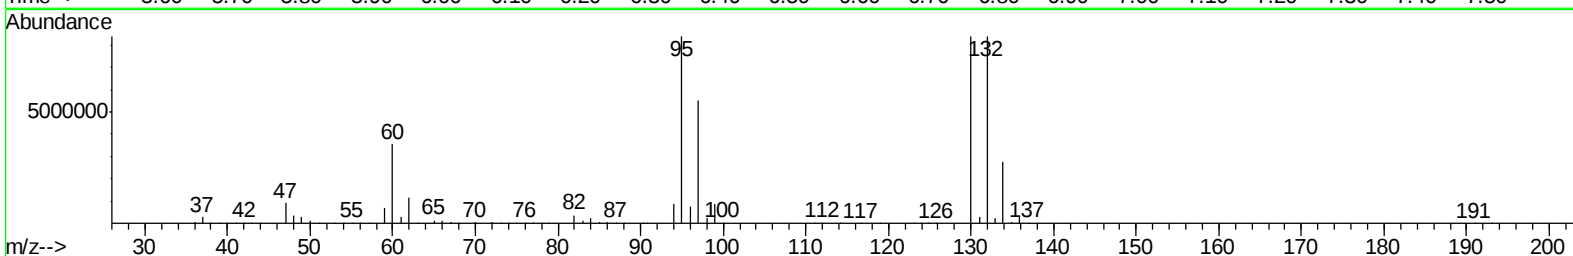


Data File : VU036032.D
Acq On : 06 Dec 2019 19:00
Operator : JC/SP
Sample : K6168-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 06 22:37:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 06 22:30:31 2019
Response via : Initial Calibration

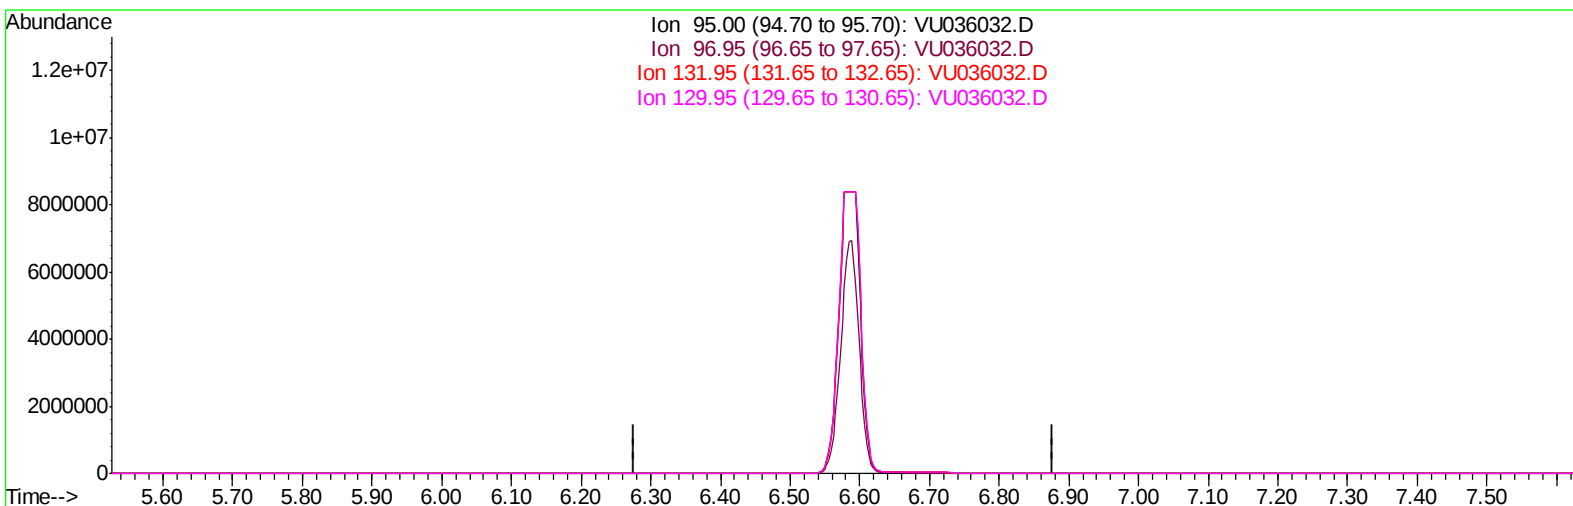

TIC: VU036032.D

(34) Trichloroethene (T)

6.578min (-6.578) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	66.10	0.00#
131.95	93.90	0.00#
129.95	98.90	0.00#