

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U120619\
 Data File : VU036019.D
 Acq On : 06 Dec 2019 13:11
 Operator : JC/SP
 Sample : K6132-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1

Quant Time: Dec 06 23:20:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 06 22:30:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	294495	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	302338	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	130229	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	115464	3.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.80%
7) Chloroethane-d5	1.93	69	120107	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.20%
11) 1,1-Dichloroethene-d2	2.59	63	143322	2.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.40%#
20) 2-Butanone-d5	4.70	46	269262	45.29	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.58%
24) Chloroform-d	5.11	84	202317	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.80%
26) 1,2-Dichloroethane-d4	5.75	65	102268	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.80%
32) Benzene-d6	5.77	84	385712	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.73	67	123069	4.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.00%
41) Toluene-d8	7.93	98	315505	3.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.60%
43) trans-1,3-Dichloropropene-	8.21	79	42236	3.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.20%
46) 2-Hexanone-d5	8.68	63	203485	44.18	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.36%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	108944	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	125707	4.67	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.40%

Target Compounds

					Ovalue
5) Vinyl chloride	1.62	62	147746	4.200	ug/L # 10
8) Chloroethane	1.95	64	79171	3.629	ug/L # 83
10) 1,1,2-Trichloro-1,2,2-trif	2.60	101	4082	0.180	ug/L # 66
13) Acetone	2.69	43	51634	9.607	ug/L 90
14) Carbon disulfide	2.82	76	5788	0.078	ug/L 99
15) Methyl Acetate	3.00	43	5601	0.581	ug/L # 78
16) Methylene chloride	3.08	84	18028	0.551	ug/L 95
18) trans-1,2-Dichloroethene	3.39	96	2574	0.115	ug/L 99
19) 1,1-Dichloroethane	3.92	63	342835	7.847	ug/L 99
21) 2-Butanone	4.78	43	107385	15.564	ug/L 98
22) cis-1,2-Dichloroethene	4.72	96	343742	14.559	ug/L 92
25) Chloroform	5.14	83	55399	1.257	ug/L 100
27) 1,2-Dichloroethane	5.84	62	4580	0.163	ug/L 97
29) 1,1,1-Trichloroethane	5.36	97	145495	3.979	ug/L 98
33) Benzene	5.82	78	170834	1.797	ug/L 100
34) Trichloroethene	6.58	95	6566	0.273	ug/L 94
38) Bromodichloromethane	7.14	83	6980	0.227	ug/L # 85

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120619\
Data File : VU036019.D
Acq On : 06 Dec 2019 13:11
Operator : JC/SP
Sample : K6132-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQW1

Quant Time: Dec 06 23:20:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 06 22:30:31 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	8.00	91	56906	0.573	ug/L	100
47) Tetrachloroethene	8.58	164	1891	0.097	ug/L #	80
51) Chlorobenzene	9.48	112	94918	1.531	ug/L	99
52) Ethylbenzene	9.60	91	18922	0.188	ug/L	89
53) m,p-Xylene	9.72	106	13957	0.368	ug/L	97
54) o-Xylene	10.13	106	9923	0.279	ug/L	95
55) Styrene	10.14	104	9385	0.157	ug/L	100
62) 1,3-Dichlorobenzene	11.77	146	5865	0.135	ug/L	94
63) 1,4-Dichlorobenzene	11.86	146	17661	0.411	ug/L	98
65) 1,2-Dichlorobenzene	12.24	146	18626	0.450	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120619\
Data File : VU036019.D
Acq On : 06 Dec 2019 13:11
Operator : JC/SP
Sample : K6132-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQW1

Quant Time: Dec 06 23:20:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 06 22:30:31 2019
Response via : Initial Calibration

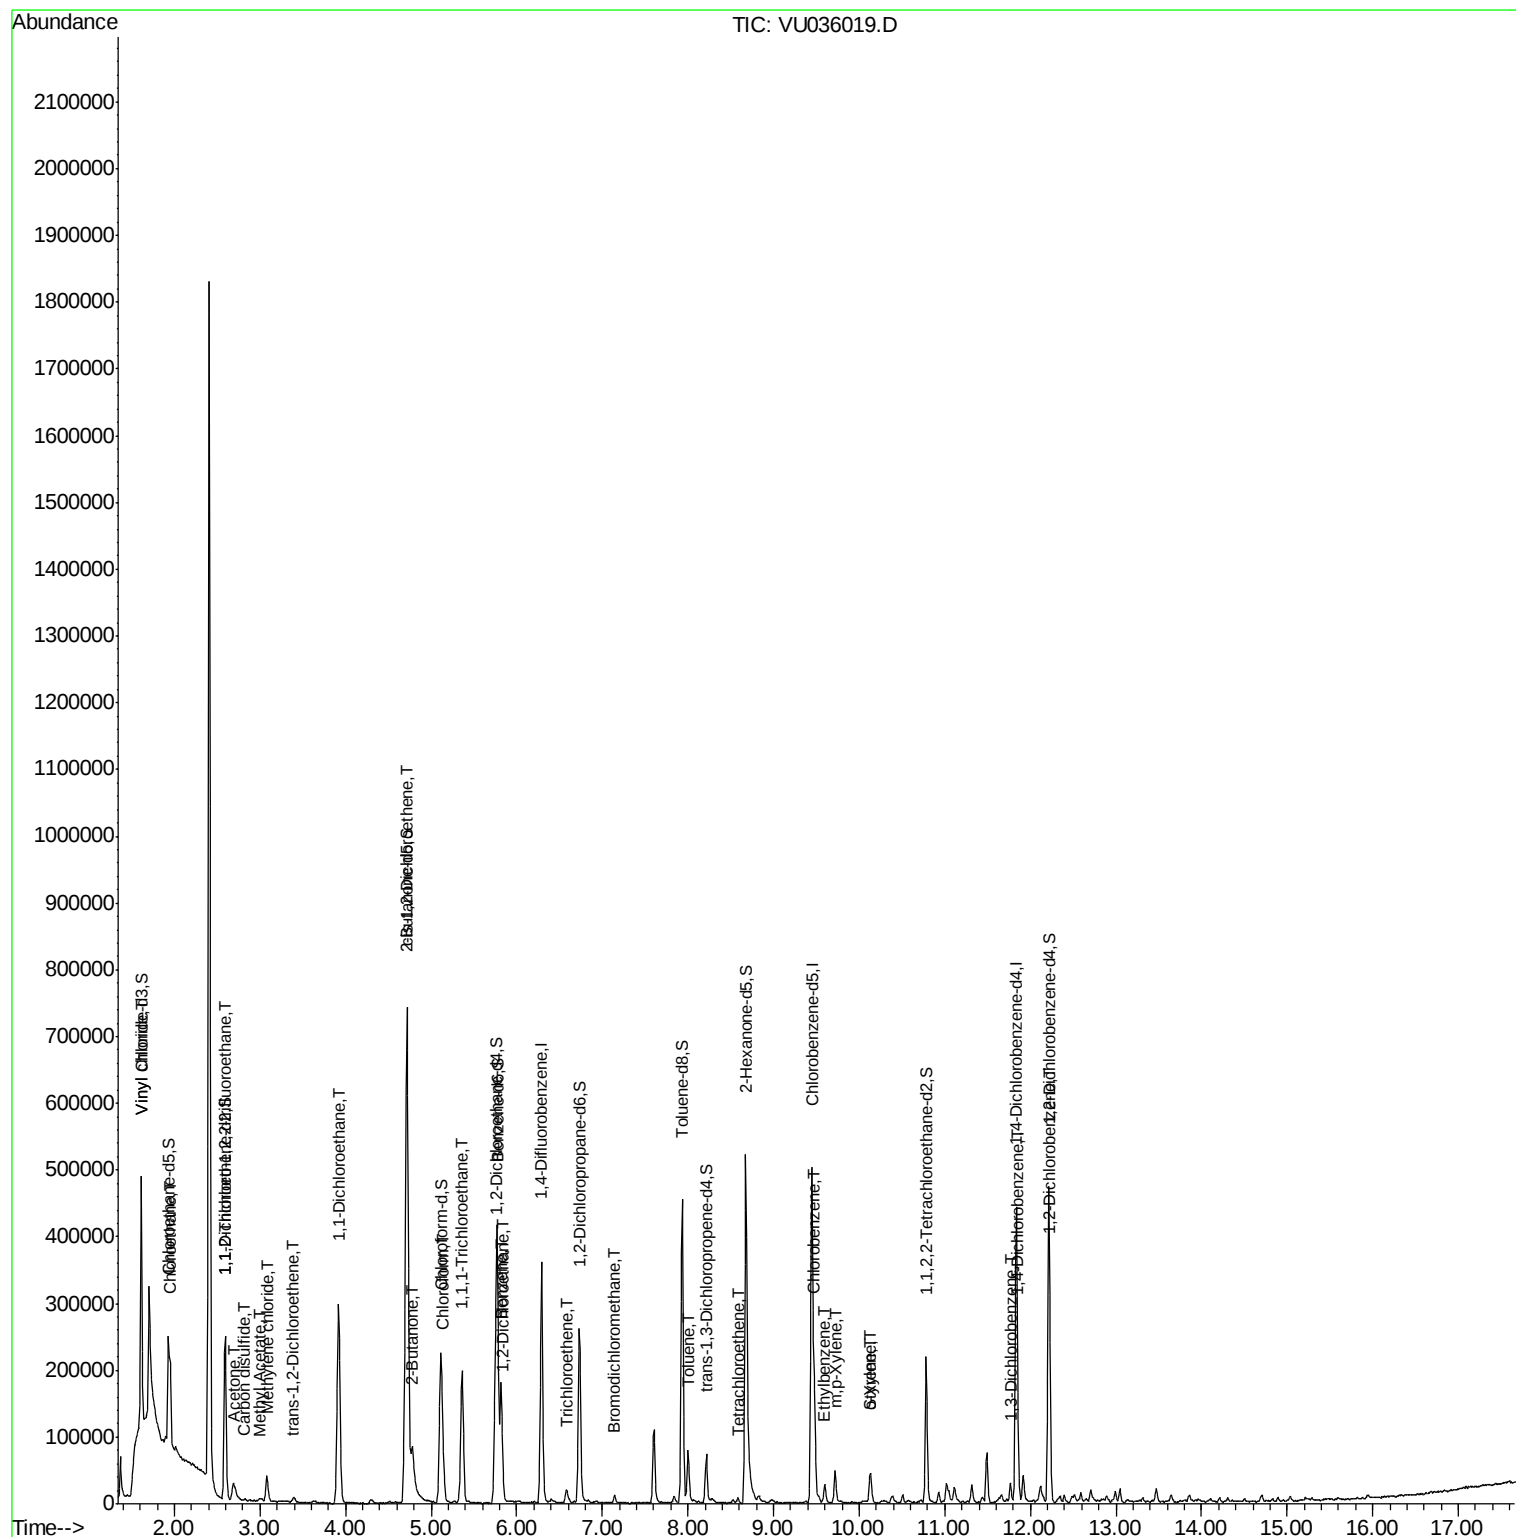

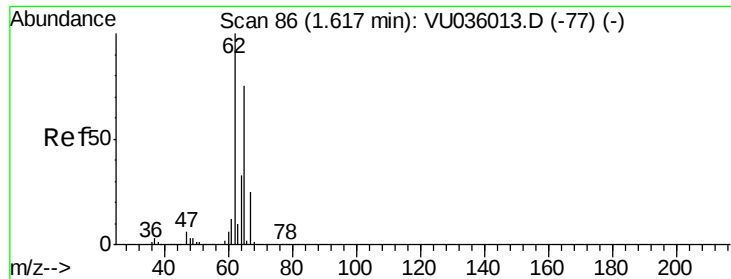

#5

Vinyl chloride

Concen: 4.200 ug/L

RT: 1.62 min Scan# 86

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampled :





BFQW1

Tot Ion: 62 Resp: 147746

Ion Ratio Lower Upper

62 100

64 83.3 23.0 42.6#

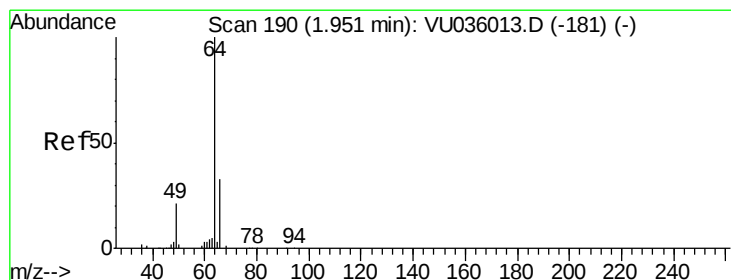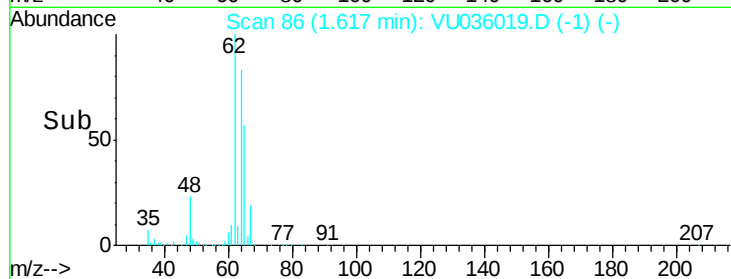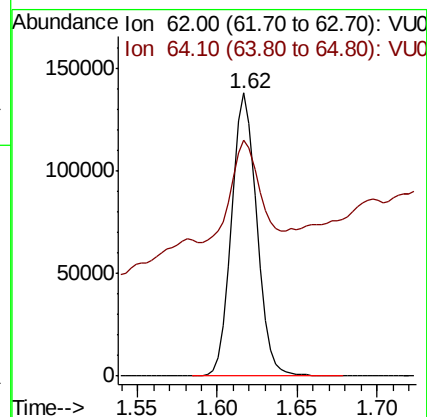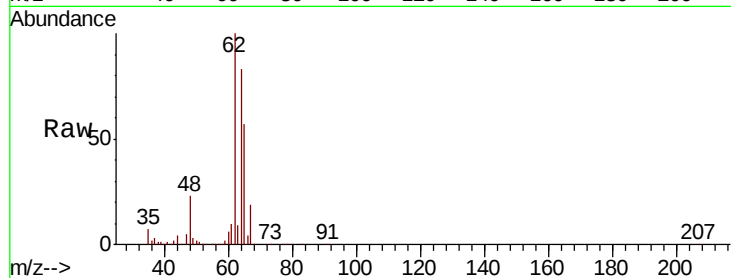

#8

Chloroethane

Concen: 3.629 ug/L

RT: 1.95 min Scan# 190

Delta R.T. 0.00 min

Lab File: VU036019.D




Acq: 06 Dec 2019 13:11


Tgt Ion: 64 Resp: 79171

Ion Ratio Lower Upper

64 100

66 21.7 22.0 40.8#

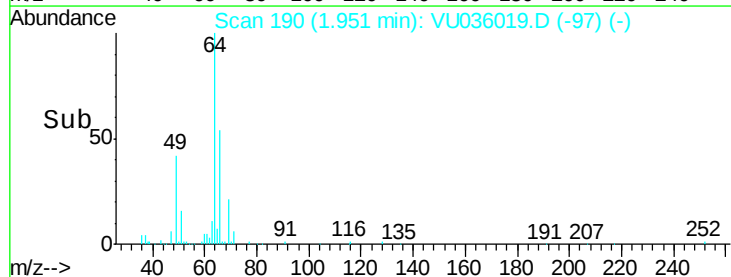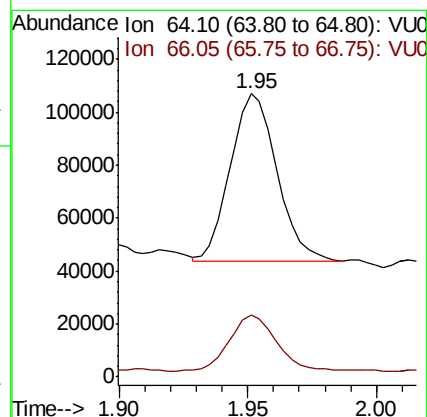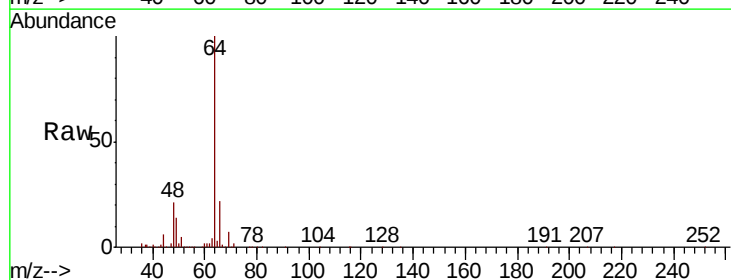

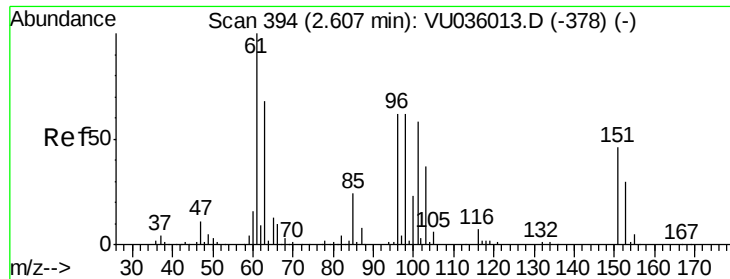

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.180 ug/L

RT: 2.60 min Scan# 391

Delta R.T. -0.01 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion:101 Resp: 4082

Ion Ratio Lower Upper

101 100

85 25.3 35.5 53.3#




151 41.2 57.5 86.3#

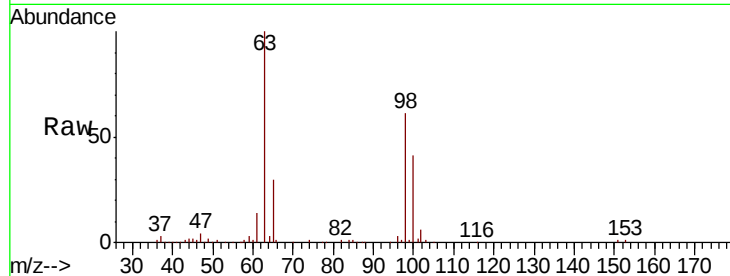

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

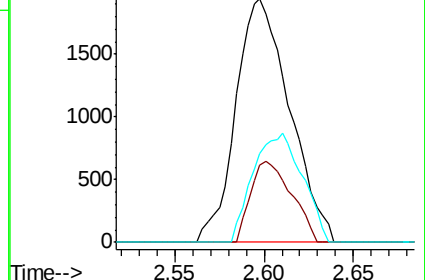

#13

Acetone

Concen: 9.607 ug/L

RT: 2.69 min Scan# 420

Delta R.T. 0.02 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion: 43 Resp: 51634

Ion Ratio Lower Upper



43 100


58 28.6 0.0 68.6



Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

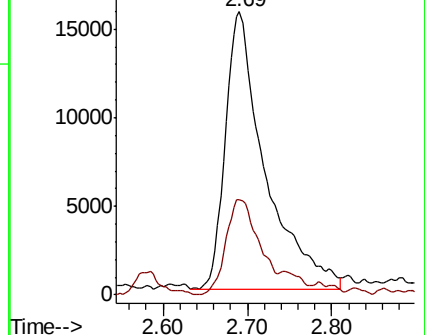



#14

Carbon disulfide

Concen: 0.078 ug/L

RT: 2.82 min Scan# 460

Delta R.T. -0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion: 76 Resp: 5788

Ion Ratio Lower Upper




76 100

78 8.1 6.9 10.3



Abundance Ion 76.05 (75.75 to 76.75): VU036019.D (-446) (-)

Ion 78.00 (77.70 to 78.70): VU036019.D (-446) (-)

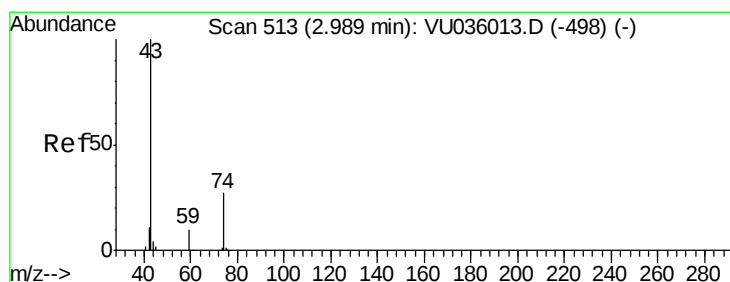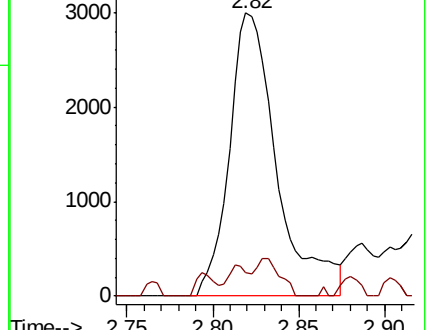

#15

Methyl Acetate

Concen: 0.581 ug/L

RT: 3.00 min Scan# 516

Delta R.T. 0.01 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion: 43 Resp: 5601

Ion Ratio Lower Upper



43 100


74 14.0 20.0 30.0#

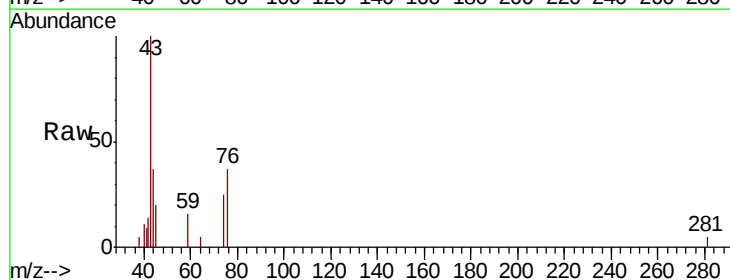

Abundance Ion 43.05 (42.75 to 43.75): VU036019.D (-498) (-)

Ion 74.05 (73.75 to 74.75): VU036019.D (-498) (-)

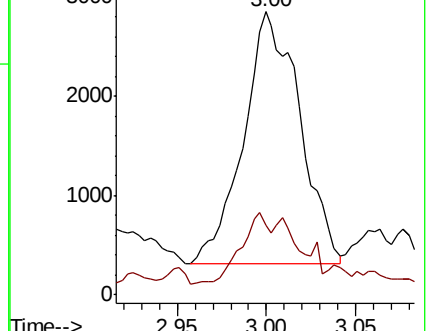







#16
Methvlene chloride
Concen: 0.551 ug/L
RT: 3.08 min Scan# 542
Delta R.T. 0.00 min
Lab File: VU036019.D
Acq: 06 Dec 2019 13:11

Instrument :
MSVOA_U
ClientSampleId :
BFQW1

Tot Ion: 84 Resp: 18028
Ion Ratio Lower Upper
84 100
86 68.3 44.7 82.9
49 118.4 86.2 160.2

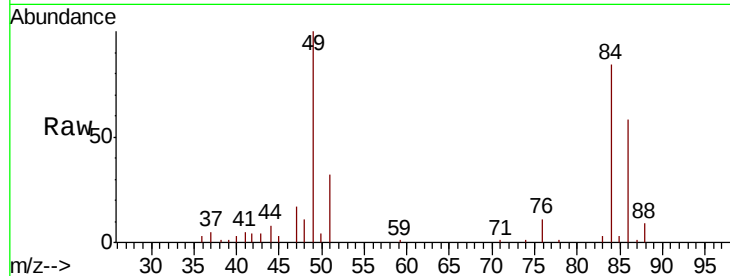


Abundance Ion 84.05 (83.75 to 84.75): VU0
15000 Ion 86.00 (85.70 to 86.70): VU0
Ion 49.10 (48.80 to 49.80): VU0

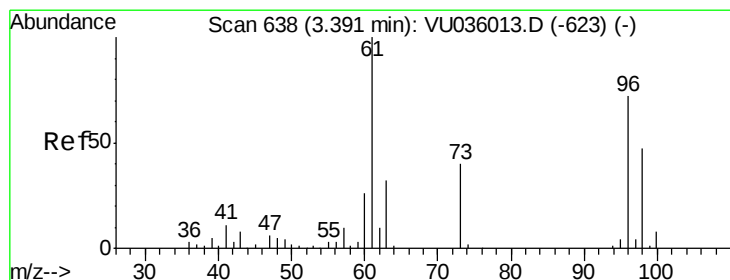
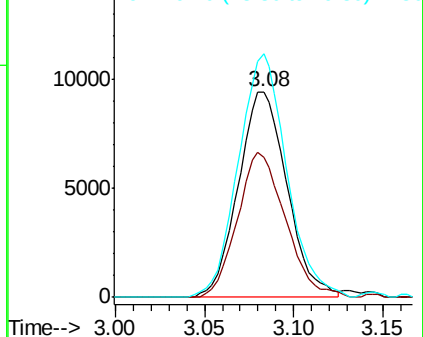



#18
trans-1,2-Dichloroethene
Concen: 0.115 ug/L
RT: 3.39 min Scan# 639
Delta R.T. 0.00 min
Lab File: VU036019.D
Acq: 06 Dec 2019 13:11

Tgt Ion: 96 Resp: 2574
Ion Ratio Lower Upper
96 100
61 143.7 101.2 187.8
98 65.1 45.0 83.6



Abundance Ion 96.00 (95.70 to 96.70): VU0
2500 Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0



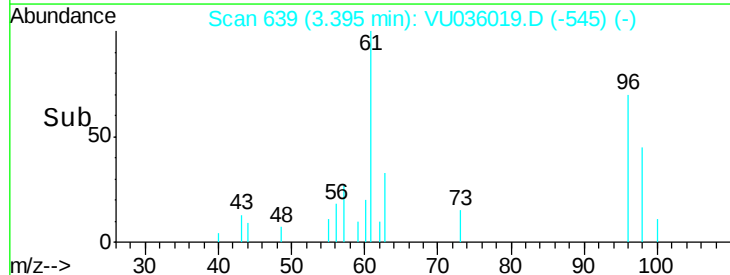
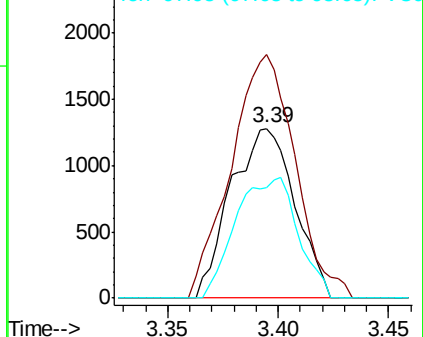




#19
 1,1-Dichloroethane
 Concen: 7.847 ug/L
 RT: 3.92 min Scan# 802
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1


Tot Ion	Ratio	Lower	Upper
63	100		
65	31.5	22.4	41.6
83	14.1	9.8	18.2

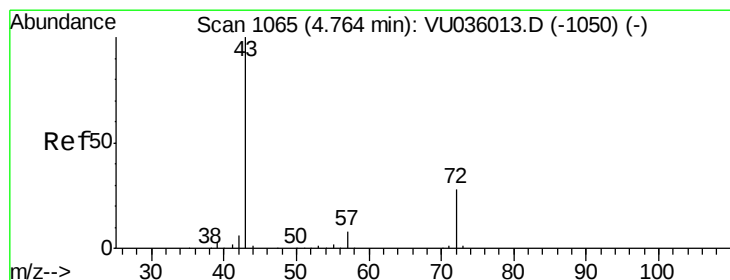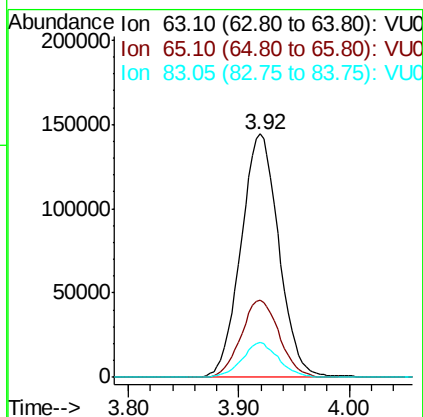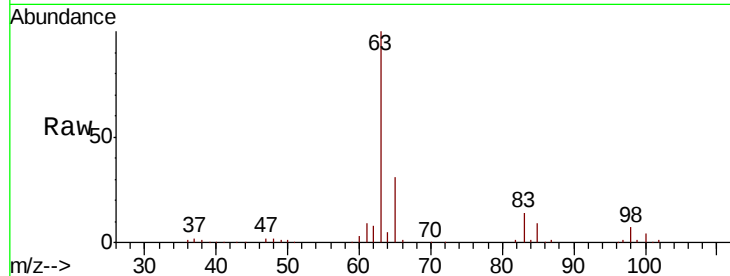

#21
 2-Butanone
 Concen: 15.564 ug/L
 RT: 4.78 min Scan# 1070
 Delta R.T. 0.02 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11

Tgt Ion	Ratio	Lower	Upper
43	100		
72	26.4	12.6	37.8

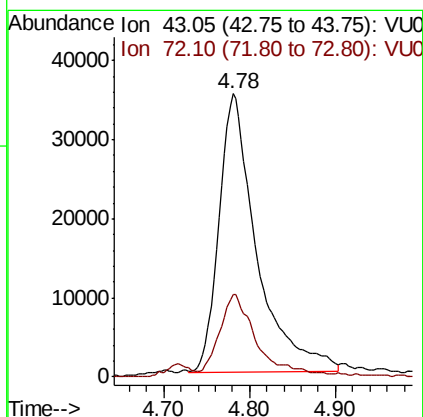



#22

cis-1,2-Dichloroethene

Concen: 14.559 ug/L

RT: 4.72 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion: 96 Resp: 343742

Ion Ratio Lower Upper

96 100

61 126.9 95.7 177.7




68 0.0 0.0 0.0



Abundance Ion 96.00 (95.70 to 96.70): VU036019.D (-957) (-)

Ion 61.05 (60.75 to 61.75): VU036019.D (-957) (-)

Ion 68.15 (67.85 to 68.85): VU036019.D (-957) (-)

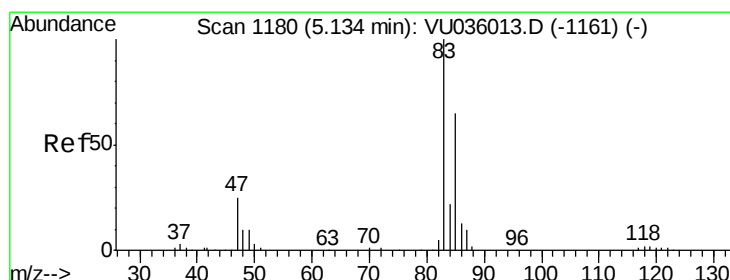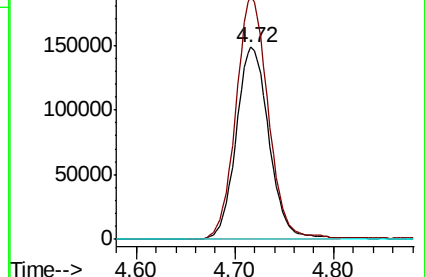

#25

Chloroform

Concen: 1.257 ug/L

RT: 5.14 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion: 83 Resp: 55399

Ion Ratio Lower Upper



83 100


85 65.1 45.4 84.2



Abundance Ion 83.05 (82.75 to 83.75): VU036019.D (-1087) (-)

Ion 85.00 (84.70 to 85.70): VU036019.D (-1087) (-)



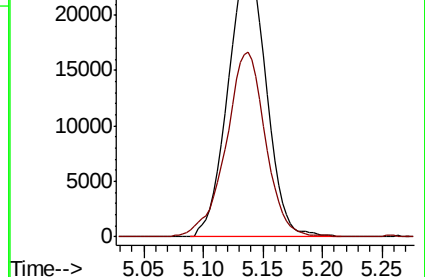



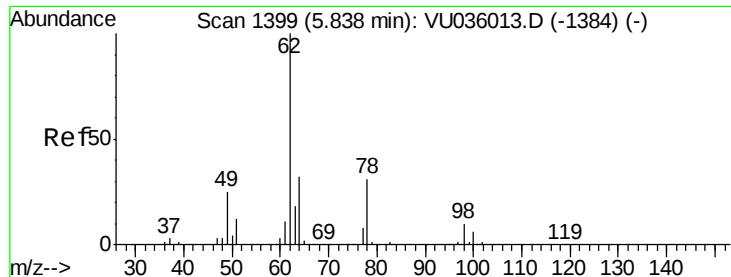

#27
 1,2-Dichloroethane
 Concen: 0.163 ug/L
 RT: 5.84 min Scan# 1400
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11




Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1


Tot Ion: 62.00 Resp: 4580
 Ion Ratio Lower Upper
 62 100
 98 8.3 7.6 11.4

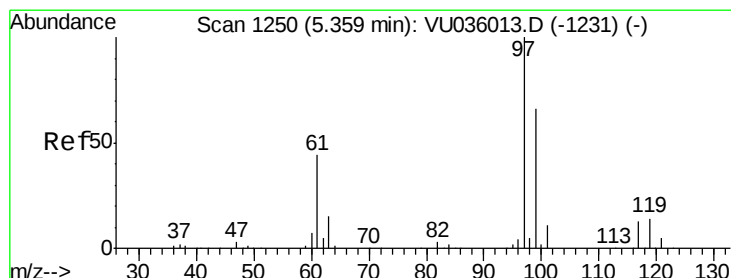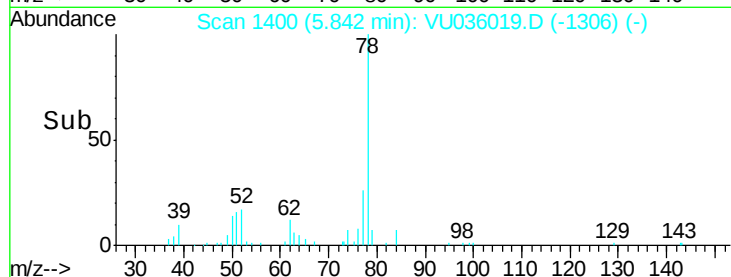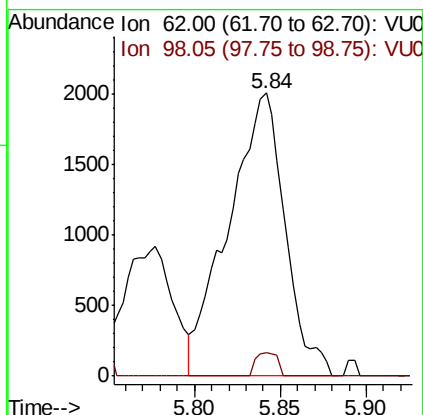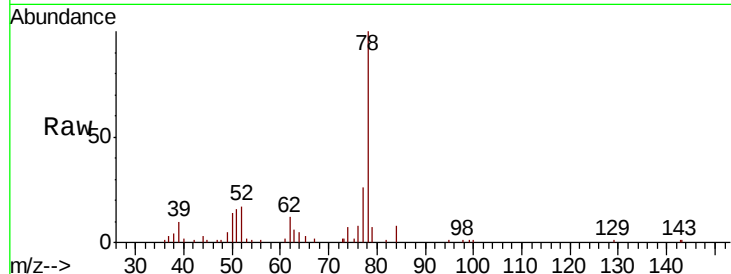

#29
 1,1,1-Trichloroethane
 Concen: 3.979 ug/L
 RT: 5.36 min Scan# 1251
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11

Tgt Ion: 97 Resp: 145495
 Ion Ratio Lower Upper
 97 100
 99 64.1 51.8 77.8
 61 44.1 37.6 56.4

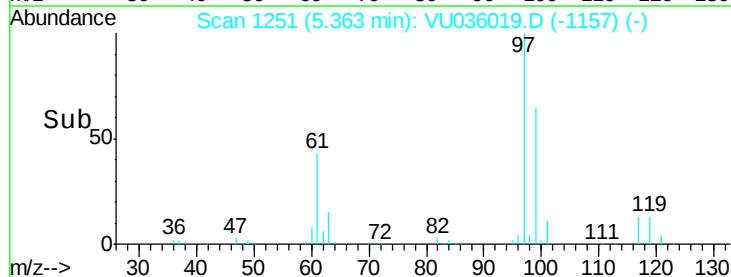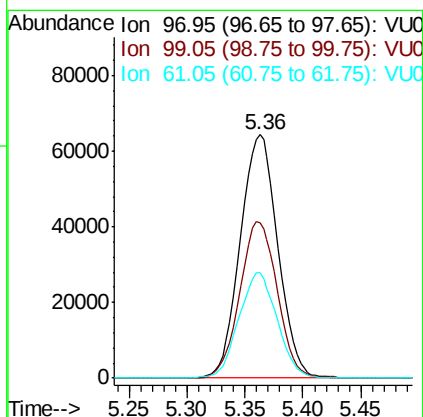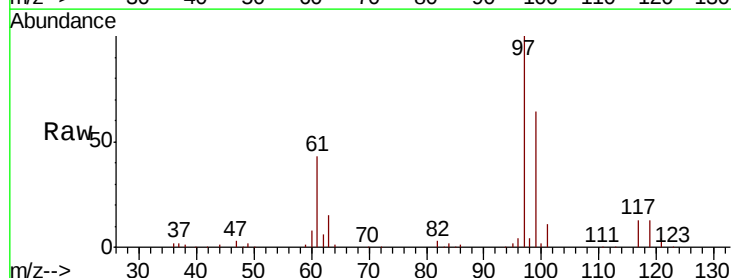

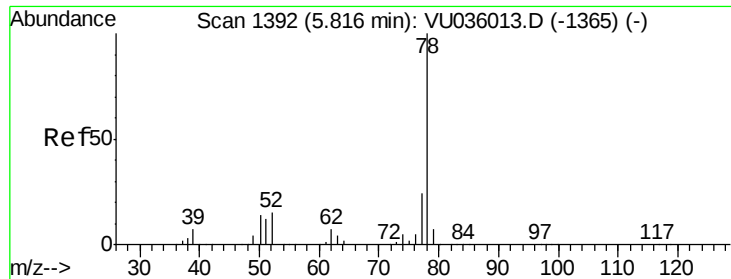

#33

Benzene

Concen: 1.797 ug/L

RT: 5.82 min Scan# 1392

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11


Instrument :

MSVOA_U




ClientSampleId :

BFQW1

Tgt Ion: 78 Resp: 170834

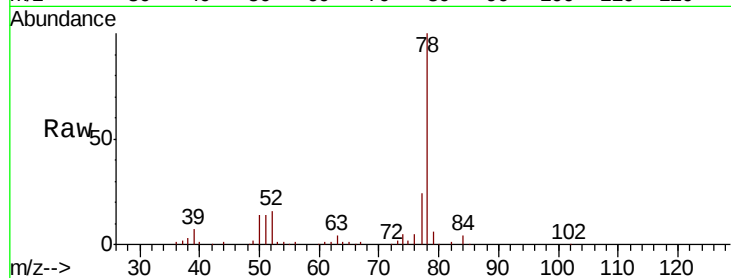

Abundance Ion 78.10 (77.80 to 78.80): VU0

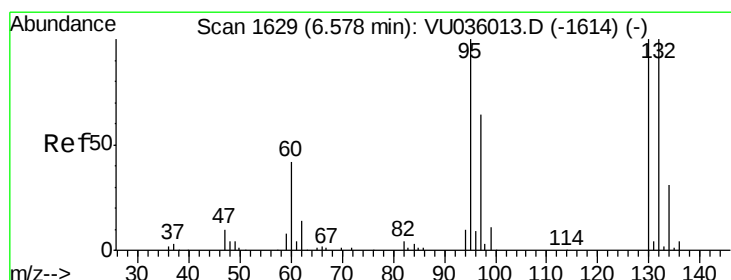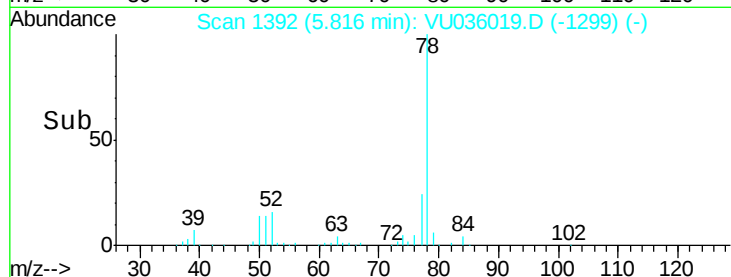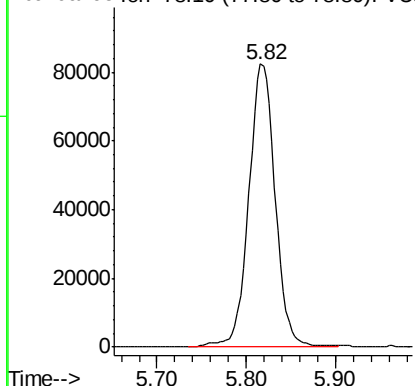

#34

Trichloroethene

Concen: 0.273 ug/L

RT: 6.58 min Scan# 1629

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Tgt Ion: 95 Resp: 6566


Ion	Ratio	Lower	Upper
95	100		
97	59.4	46.3	85.9
132	86.7	65.7	122.1
130	102.4	69.2	128.6

95 100

97 59.4 46.3 85.9

132 86.7 65.7 122.1

130 102.4 69.2 128.6


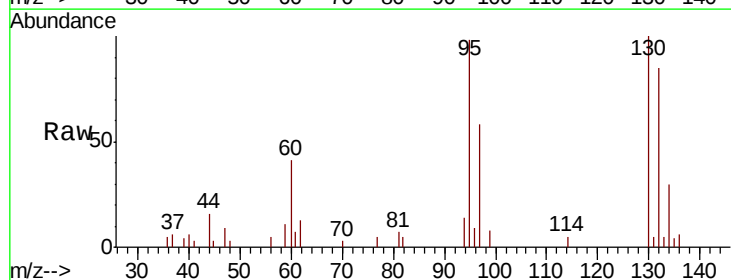



Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

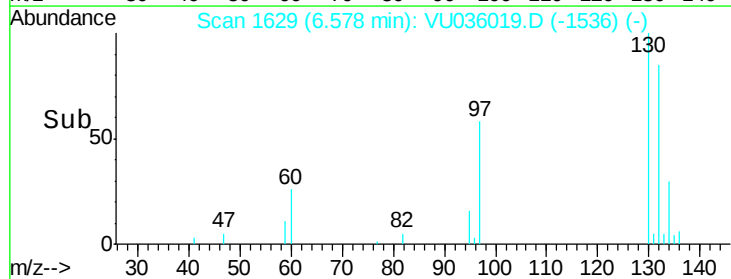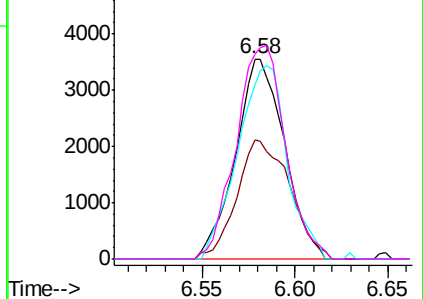



#38

Bromodichloromethane

Concen: 0.227 ug/L

RT: 7.14 min Scan# 1805

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion: 83 Resp: 6980

Ion Ratio Lower Upper

83 100

85 74.7 44.0 81.8




127 13.9 6.5 9.7#

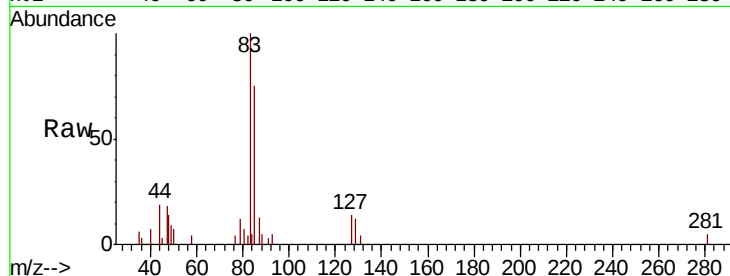

Abundance Ion 82.95 (82.65 to 83.65): VU036019.D (-1712) (-)

Ion 85.00 (84.70 to 85.70): VU036019.D (-1712) (-)

Ion 126.90 (126.60 to 127.60): VU036019.D (-1712) (-)

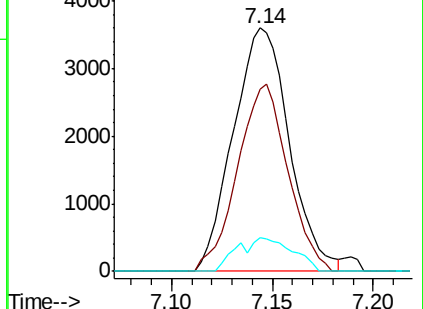

#42

Toluene

Concen: 0.573 ug/L

RT: 8.00 min Scan# 2072

Delta R.T. 0.00 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion: 91 Resp: 56906

Ion Ratio Lower Upper



91 100


92 57.0 39.8 74.0



Abundance Ion 91.15 (90.85 to 91.85): VU036019.D (-1979) (-)

Ion 92.15 (91.85 to 92.85): VU036019.D (-1979) (-)

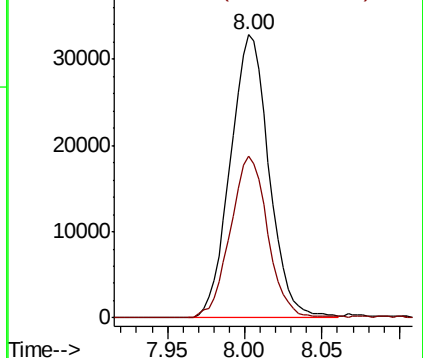



#47

Tetrachloroethene

Concen: 0.097 ug/L

RT: 8.58 min Scan# 2253

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :

BFQW1

Tot Ion:164 Resp: 1891


Ion Ratio Lower Upper

164 100

129 75.7 67.9 126.1

131 58.4 64.1 119.1#

166 122.0 92.6 172.0






Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

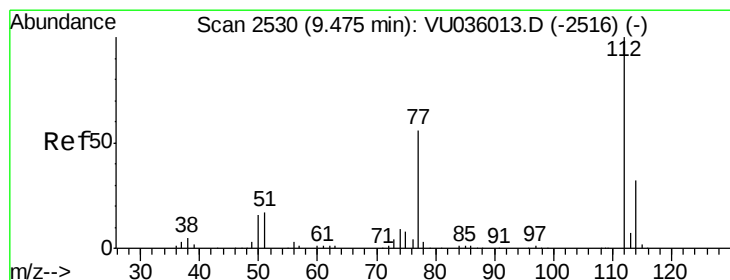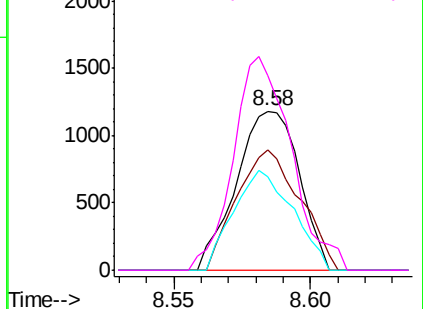

#51

Chlorobenzene

Concen: 1.531 ug/L

RT: 9.48 min Scan# 2531

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11


Tgt Ion:112 Resp: 94918

Ion Ratio Lower Upper

112 100

114 32.9 22.5 41.7



77 58.7 47.7 71.5




Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VU

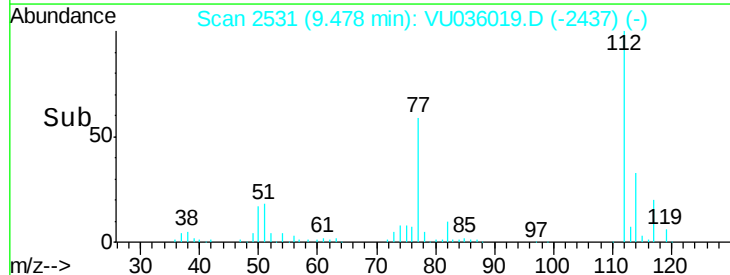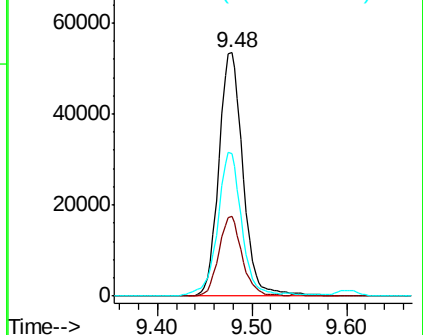

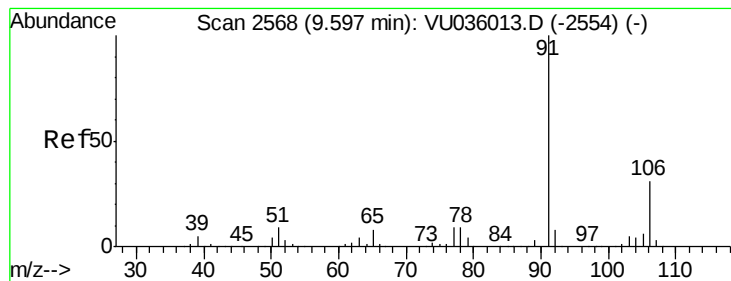

#52

Ethylbenzene

Concen: 0.188 ug/L

RT: 9.60 min Scan# 2569

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion: 91 Resp: 18922




Ion Ratio Lower Upper

91 100

106 36.0 21.1 39.3

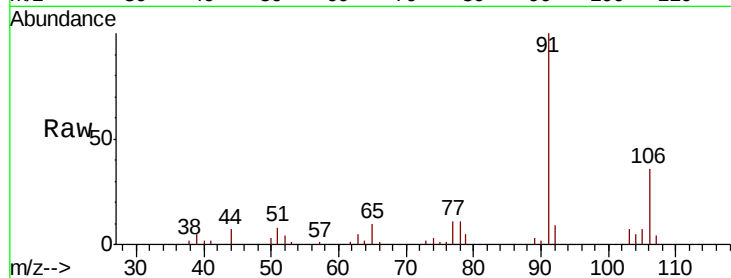

Abundance Ion 91.15 (90.85 to 91.85): VU036019.D (-2554) (-)

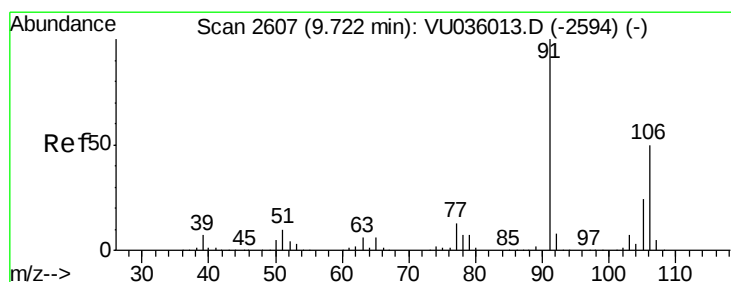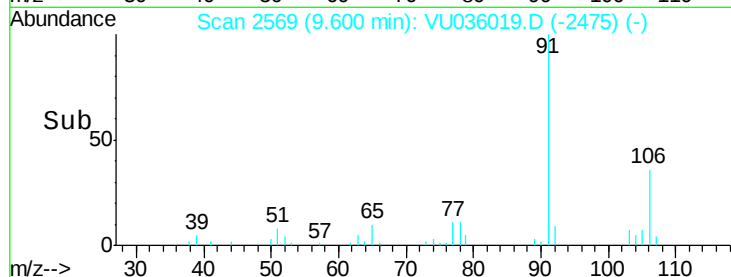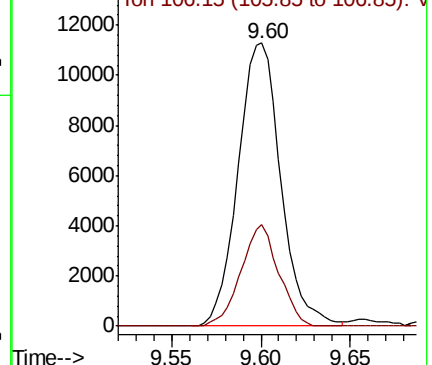

#53

m,p-Xylene

Concen: 0.368 ug/L

RT: 9.72 min Scan# 2606

Delta R.T. -0.00 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion: 106 Resp: 13957



Ion Ratio Lower Upper


106 100

91 193.4 138.9 257.9

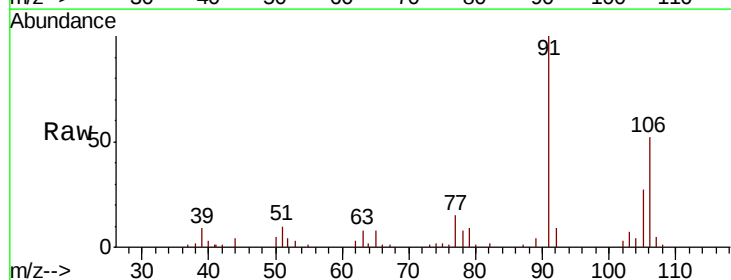

Abundance Ion 106.15 (105.85 to 106.85): VU036019.D (-2594) (-)

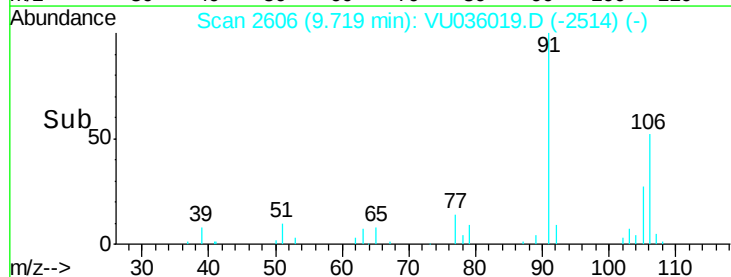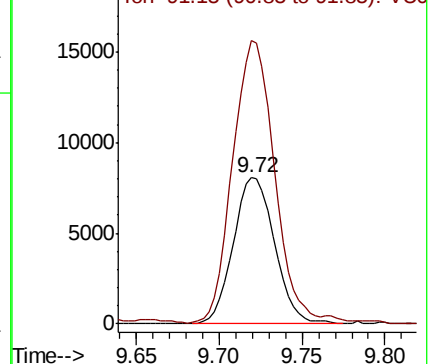



#54

o-Xylene

Concen: 0.279 ug/L

RT: 10.13 min Scan# 2733

Delta R.T. 0.00 min

Lab File: VU036019.D

Acq: 06 Dec 2019 13:11

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion:106 Resp: 9923

Ion Ratio Lower Upper




106 100

91 214.3 155.3 288.3

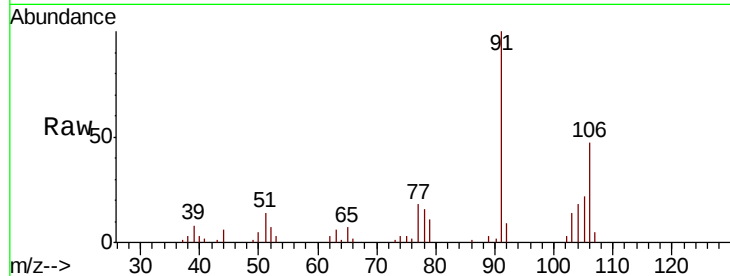

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

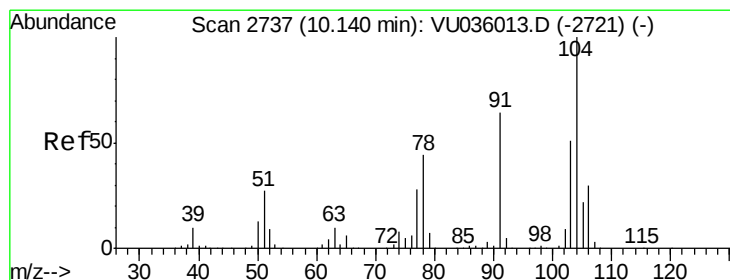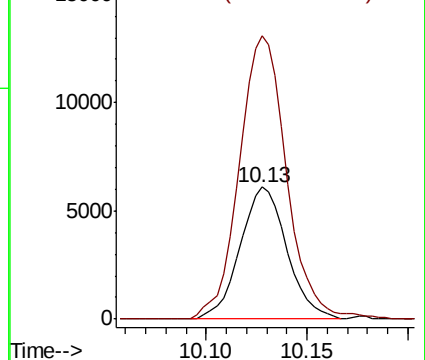

#55

Styrene

Concen: 0.157 ug/L

RT: 10.14 min Scan# 2737

Delta R.T. 0.00 min

Lab File: VU036019.D


Acq: 06 Dec 2019 13:11

Tgt Ion:104 Resp: 9385

Ion Ratio Lower Upper



104 100


78 44.4 31.2 58.0



Abundance Ion 104.10 (103.80 to 104.80): V

Ion 78.10 (77.80 to 78.80): VU0

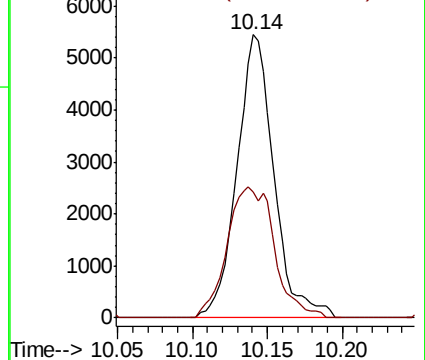


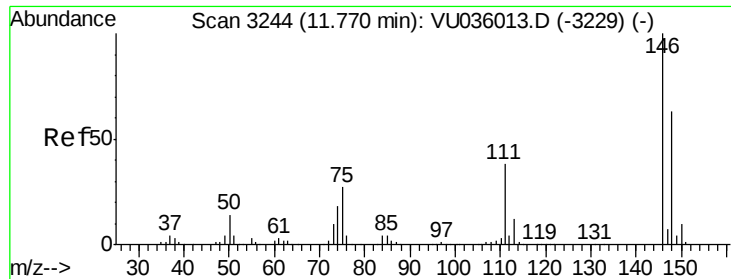




#62
 1,3-Dichlorobenzene
 Concen: 0.135 ug/L
 RT: 11.77 min Scan# 3244
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1

Tot Ion:146 Resp: 5865
 Ion Ratio Lower Upper
 146 100
 111 35.8 27.6 51.4
 148 67.2 43.4 80.6

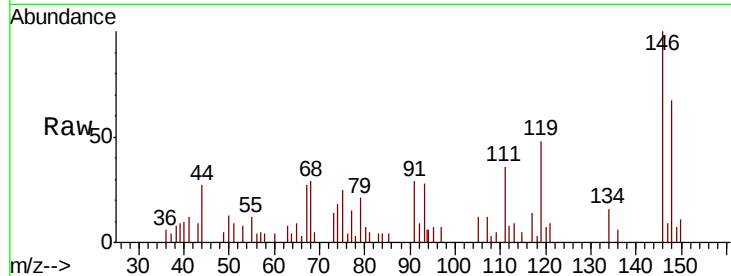


Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

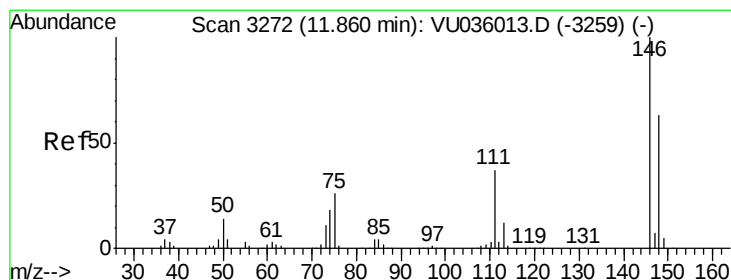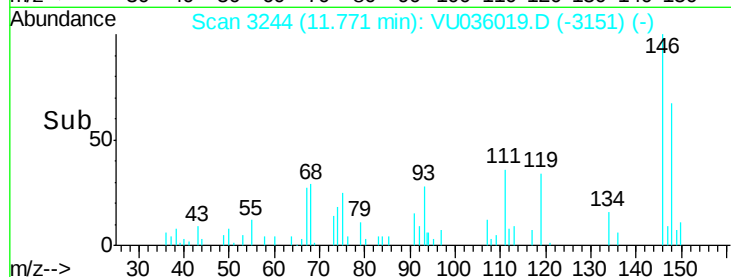
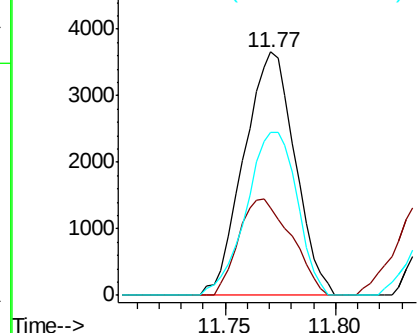



#63
 1,4-Dichlorobenzene
 Concen: 0.411 ug/L
 RT: 11.86 min Scan# 3272
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11

Tgt Ion:146 Resp: 17661
 Ion Ratio Lower Upper
 146 100
 111 38.7 28.5 52.9
 148 64.7 44.4 82.5

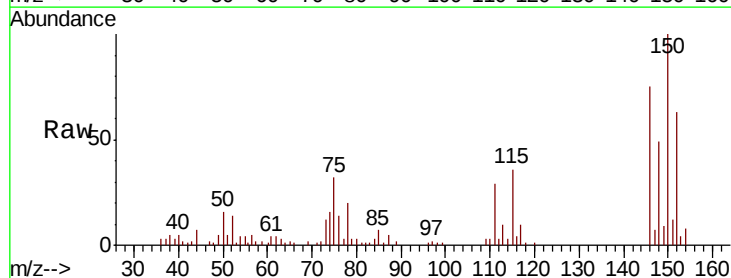

Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

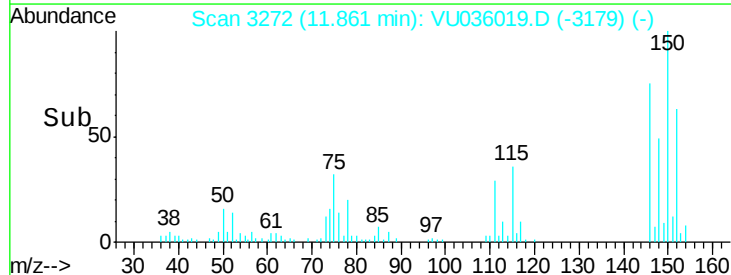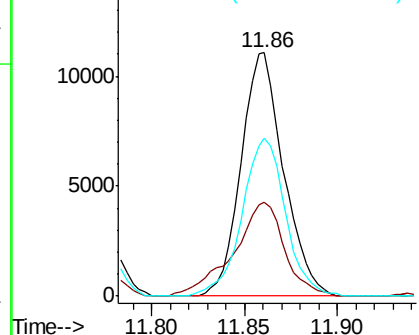


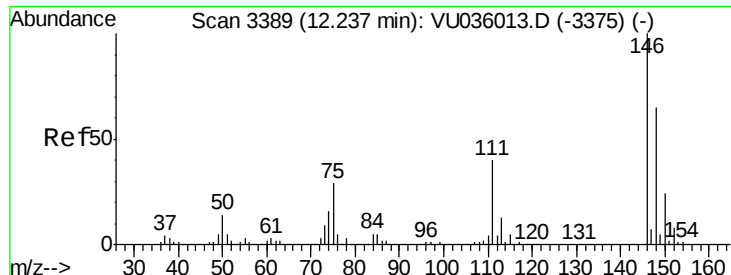

#65
 1,2-Dichlorobenzene
 Concen: 0.450 ug/L
 RT: 12.24 min Scan# 3389
 Delta R.T. 0.00 min
 Lab File: VU036019.D
 Acq: 06 Dec 2019 13:11

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1

Tot Ion	Ratio	Lower	Upper
146	100		
111	47.3	32.6	48.8
148	65.8	50.9	76.3

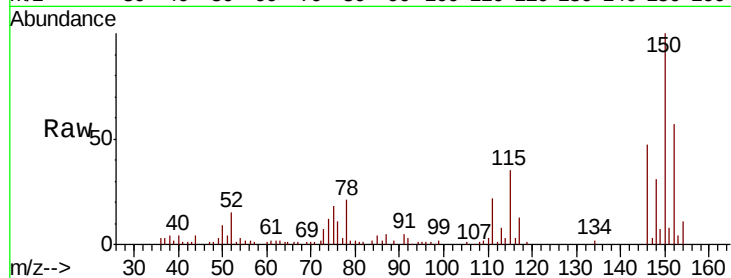

Abundance Ion 145.95 (145.65 to 146.65): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

