


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120619\
 Data File : VU036012.D
 Acq On : 06 Dec 2019 09:09
 Operator : JC/SP
 Sample : BFB13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB13

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 11 06:58:50 2019

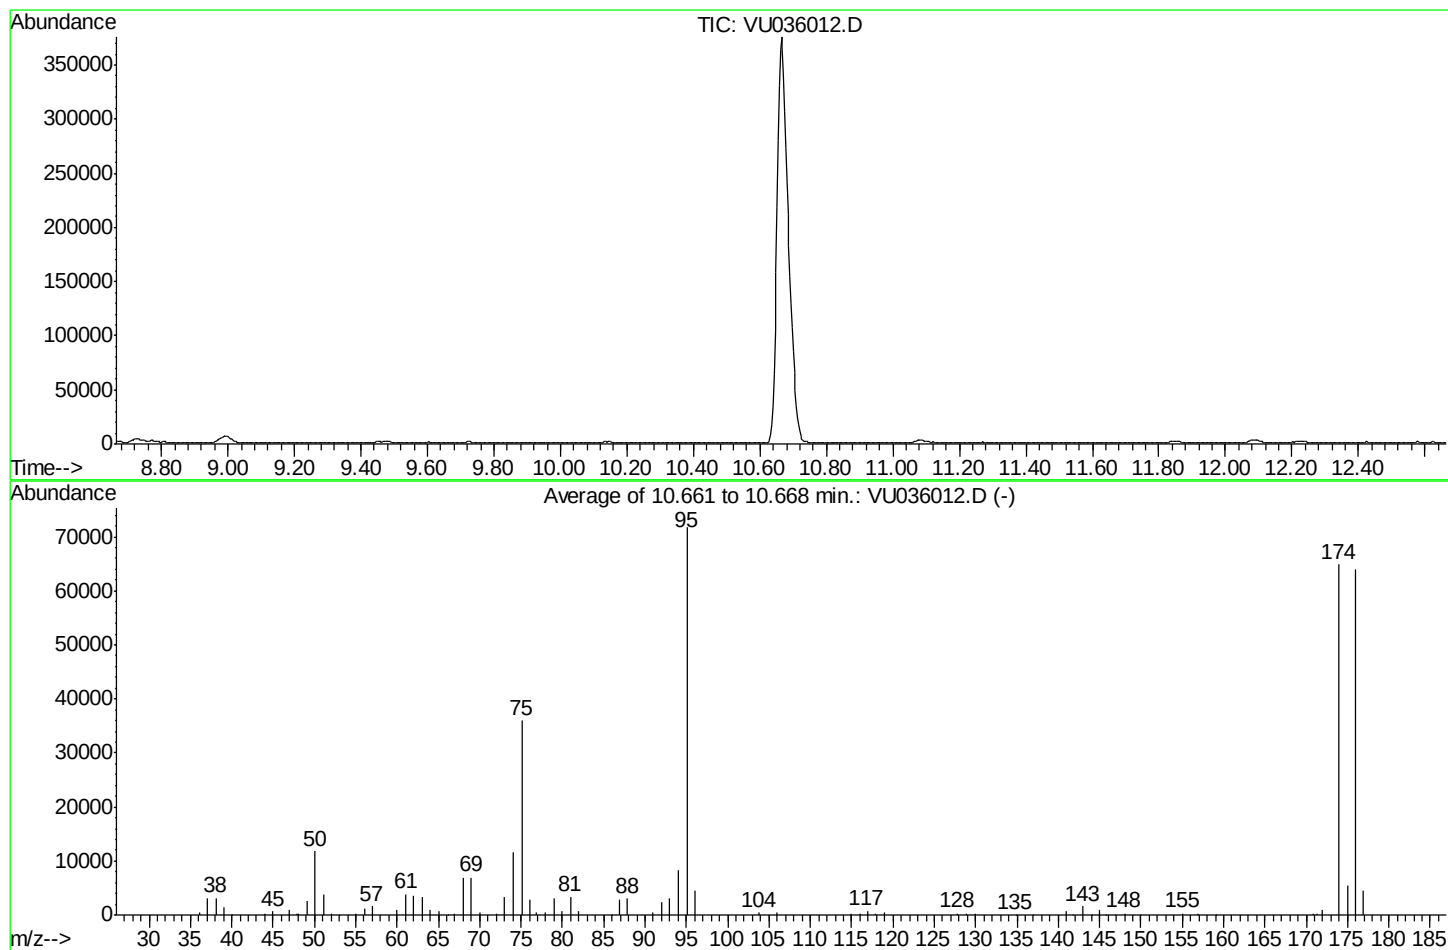

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11797	PASS
75	95	30	80	50.1	35944	PASS
95	95	100	100	100.0	71765	PASS
96	95	5	9	6.4	4604	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.4	64890	PASS
175	174	5	9	8.6	5566	PASS
176	174	95	101	98.7	64018	PASS
177	176	5	9	7.0	4511	PASS

m/z	Abundance
36.00	483.0
37.10	3208.0
38.00	3146.0
39.10	1400.0
40.20	218.0
44.00	1088.0
45.00	685.0
47.00	863.0
47.90	414.0
49.10	2764.0
50.10	11734.0
51.10	3819.0
52.10	116.0
53.00	113.0
55.00	224.0
56.10	1129.0
57.00	1582.0
60.00	796.0
61.10	3746.0
62.10	3603.0
63.10	3333.0
64.00	1056.0
65.00	711.0
66.20	117.0
66.90	166.0
68.00	6841.0
69.00	7252.0
70.10	578.0
72.00	266.0
73.00	2997.0
74.00	11520.0
75.10	36320.0
76.10	2849.0
76.90	408.0
77.90	486.0
79.00	3165.0
80.00	812.0
81.00	3340.0
81.90	749.0
86.00	148.0
87.00	2928.0
87.90	2713.0
91.00	399.0
92.00	2381.0
93.00	3340.0
94.00	8356.0
95.10	70440.0
96.10	4509.0
103.90	373.0
105.90	351.0
115.00	221.0
116.00	253.0
117.00	901.0
117.90	278.0
118.90	665.0
127.80	279.0
128.90	135.0
129.90	306.0
136.90	100.0
140.90	704.0
141.80	116.0
143.00	1563.0
145.00	858.0
145.80	138.0
147.90	312.0
149.90	108.0
155.00	261.0
156.90	177.0
159.00	109.0
171.20	379.0
172.00	1005.0
174.00	63704.0
175.00	5217.0
176.00	62288.0
177.00	4178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.00	366.0
37.10	3257.0
38.10	3293.0
39.10	1328.0
40.10	282.0
44.00	1091.0
45.00	642.0
47.00	914.0
47.90	438.0
49.00	2682.0
50.10	11986.0
51.10	3828.0
52.00	126.0
55.00	212.0
56.10	1291.0
57.00	1699.0
60.00	938.0
61.10	4087.0
62.00	3582.0
63.10	3345.0
64.00	1010.0
65.00	730.0
67.00	180.0
68.00	6948.0
69.00	7207.0
70.10	562.0
72.00	278.0
73.00	3306.0
74.00	11641.0
75.10	36784.0
76.10	2762.0
76.90	479.0
78.00	569.0
78.90	3188.0
79.90	814.0
81.00	3467.0
81.90	822.0
87.00	2976.0
87.90	3004.0
91.00	397.0
92.00	2534.0
93.00	3169.0
94.00	8508.0
95.10	73008.0
96.00	4694.0
103.80	430.0
105.90	388.0
114.90	209.0
115.90	268.0
117.00	810.0
117.90	310.0
118.90	587.0
127.90	325.0
128.90	154.0
129.90	259.0
134.90	102.0
140.90	710.0
141.80	104.0
143.00	1636.0
145.00	900.0
145.80	122.0
146.80	116.0
148.00	279.0
149.90	113.0
155.10	274.0
156.90	137.0
170.80	331.0
171.30	382.0
172.00	962.0
174.00	66000.0
175.00	5583.0
176.00	65488.0
176.90	4558.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

m/z	Abundance
36.10	398.0
37.10	2996.0
38.10	3039.0
39.10	1208.0
40.10	336.0
43.90	1030.0
45.00	560.0
47.00	854.0
48.10	424.0
49.00	2479.0
50.10	11673.0
51.10	3510.0
51.90	158.0
55.00	184.0
56.10	1262.0
57.00	1622.0
60.00	861.0
61.10	3836.0
62.00	3548.0
63.10	3049.0
64.00	942.0
65.00	769.0
67.10	249.0
68.00	6825.0
69.00	6488.0
70.00	501.0
72.10	294.0
73.00	3380.0
74.00	11416.0
75.10	34728.0
76.10	2860.0
76.90	463.0
78.10	657.0
78.90	3201.0
79.90	795.0
81.00	3391.0
81.90	794.0
86.90	2928.0
87.90	3266.0
91.00	337.0
92.00	2484.0
93.00	3038.0
94.00	8030.0
95.10	71848.0
96.00	4611.0
103.90	415.0
105.90	434.0
114.90	159.0
115.90	330.0
116.90	627.0
117.90	348.0
118.90	527.0
127.90	327.0
128.80	144.0
129.90	223.0
134.90	147.0
140.90	719.0
143.00	1494.0
144.10	134.0
145.00	889.0
146.80	102.0
148.10	205.0
155.10	268.0
156.90	111.0
170.80	354.0
171.90	882.0
174.00	64968.0
174.90	5900.0
176.00	64280.0
177.00	4797.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13

Scan 2885 (10.616 min): VU036012.D
BFB13

m/z	Abundance
40.00	254.0
44.00	719.0

Instrument :
MSVOA_U
ClientSampleId :
BFB13