
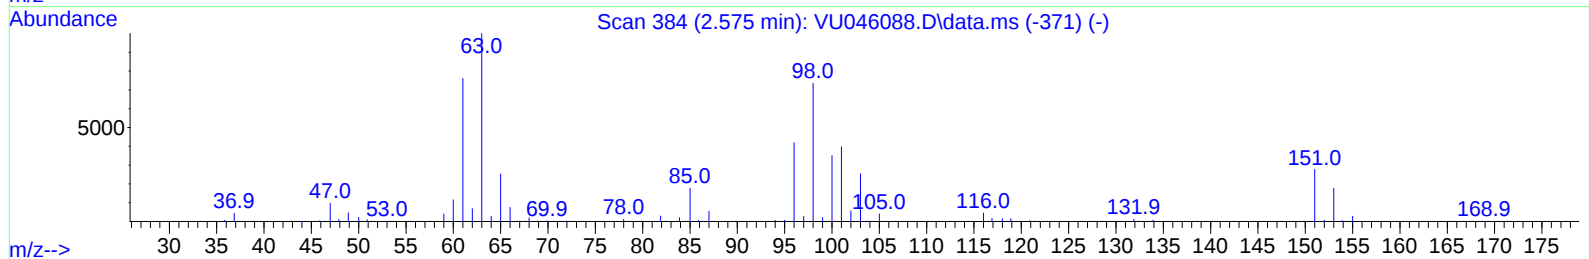
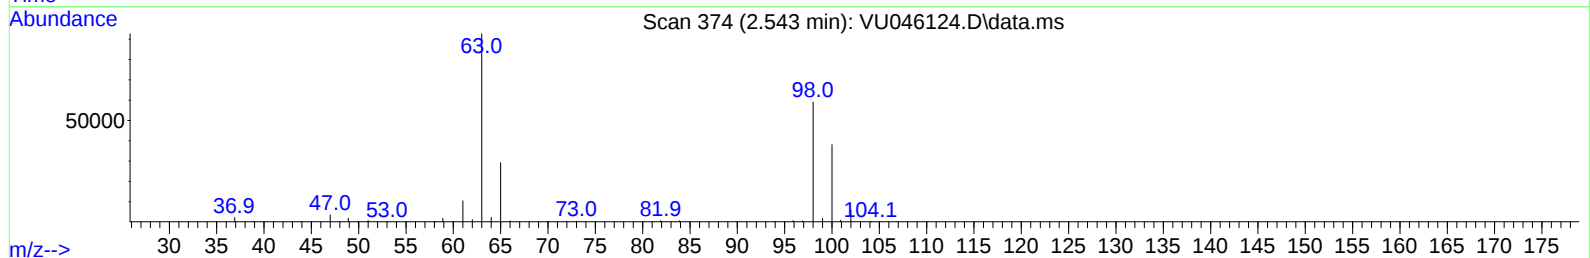


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
Data File : VU046124.D
Acq On : 06 Dec 2021 20:12
Operator : SY/MD
Sample : M4883-16ME
Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 07 01:13:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

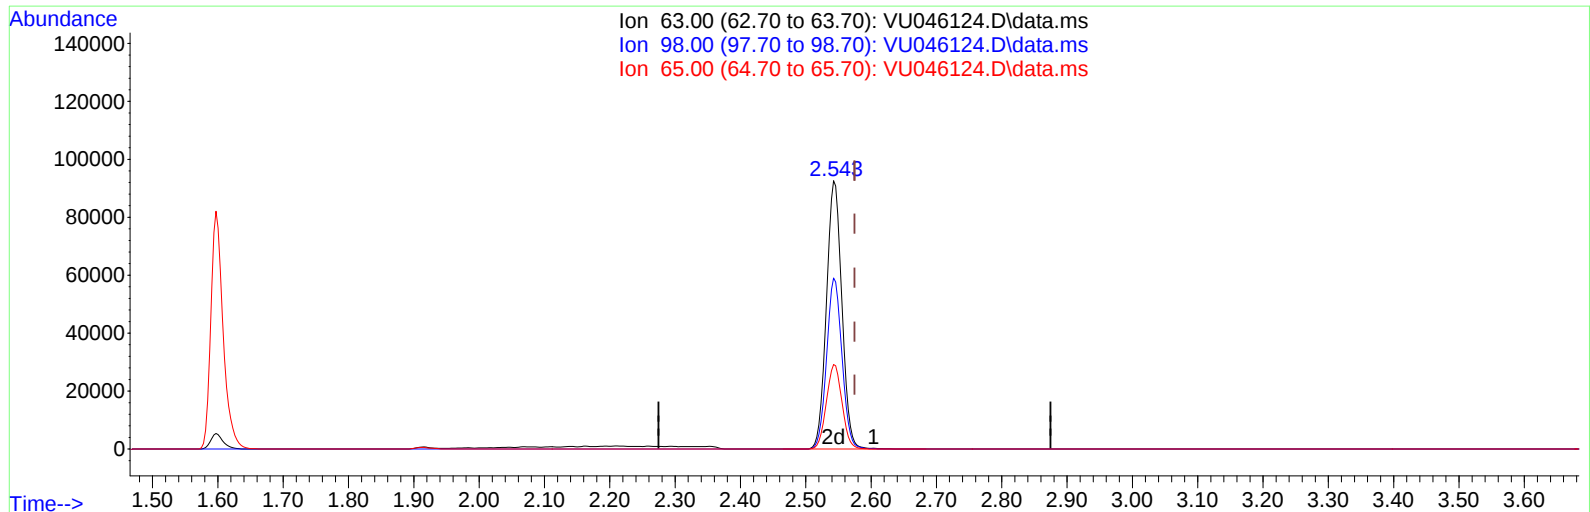

TIC: VU046124.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)




2.543min (-0.032) 50.85 ug/L m

response 152270

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.60	0.00#
65.00	23.90	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046124.D
 Acq On : 06 Dec 2021 20:12
 Operator : SY/MD
 Sample : M4883-16ME
 Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 07 01:13:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

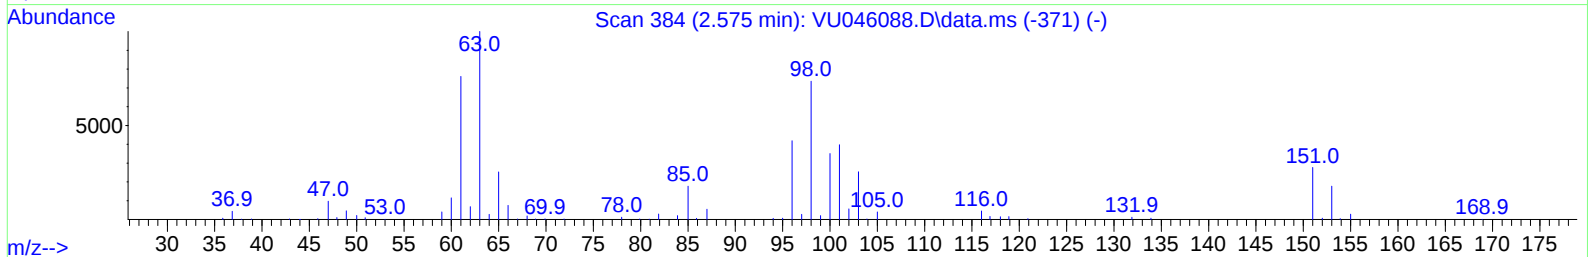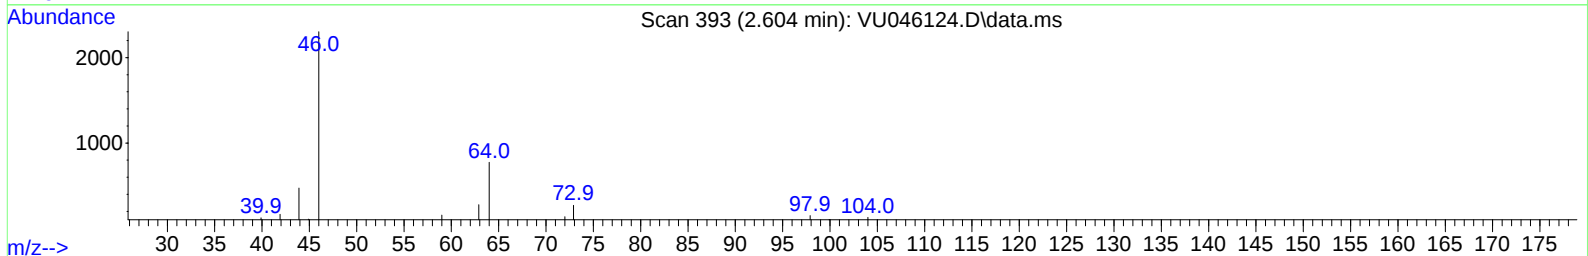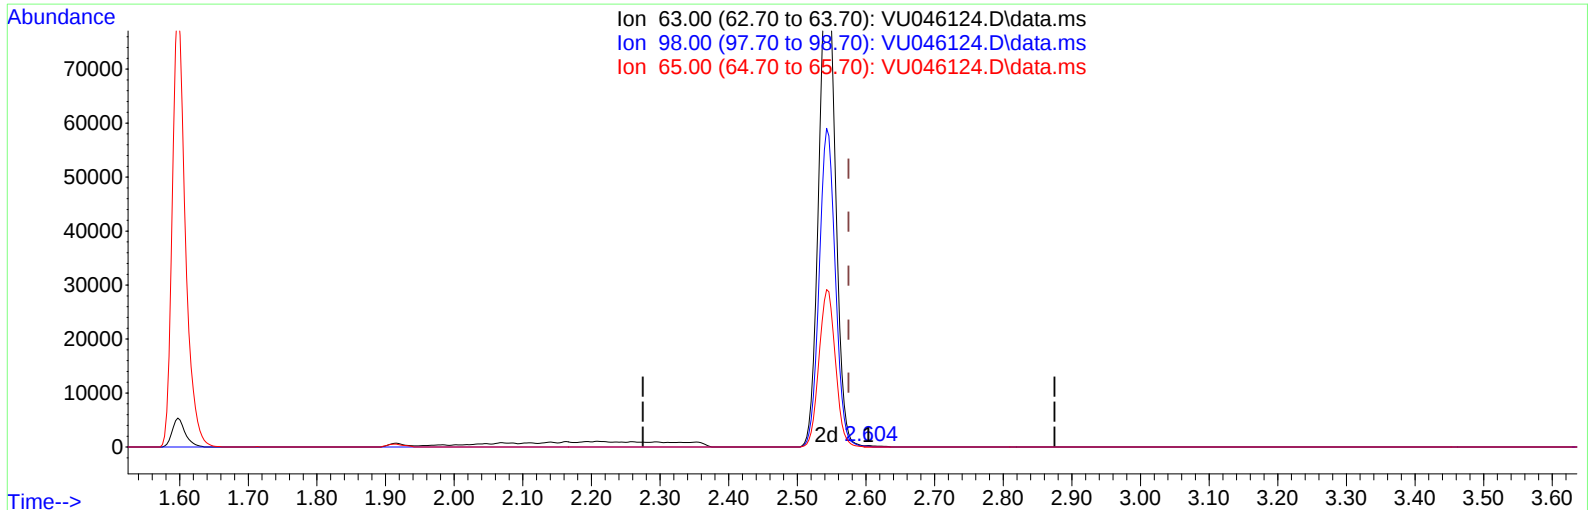

TIC: VU046124.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)**2.604min (+ 0.029) 0.13 ug/L****response 383**

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.60	0.00#
65.00	23.90	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046124.D
 Acq On : 06 Dec 2021 20:12
 Operator : SY/MD
 Sample : M4883-16ME
 Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 07 01:13:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	202493	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	198235	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	101028	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	107038	64.170	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 128.340%		
7) Chloroethane-d5	1.912	69	64282	50.193	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 100.380%		
11) 1,1-Dichloroethene-d2	2.543	63	152270m	50.851	ug/L	-0.03
Spiked Amount	50.000	Range 60 - 125	Recovery	= 101.700%		
21) 2-Butanone-d5	4.649	46	192195	144.943	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 144.940%#		
24) Chloroform-d	5.063	84	201388	72.298	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 144.600%#		
26) 1,2-Dichloroethane-d4	5.703	65	144261	77.170	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 154.340%#		
32) Benzene-d6	5.723	84	468902	82.528	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 165.060%#		
36) 1,2-Dichloropropane-d6	6.690	67	146728	83.327	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 166.660%#		
41) Toluene-d8	7.899	98	436231	84.325	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 168.640%#		
43) trans-1,3-Dichloroprop...	8.182	79	72945	85.814	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 171.620%#		
47) 2-Hexanone-d5	8.674	63	149368	178.906	ug/L	0.04
Spiked Amount	100.000	Range 45 - 130	Recovery	= 178.910%#		
56) 1,1,2,2-Tetrachloroeth...	10.771	84	207567	77.728	ug/L	0.01
Spiked Amount	50.000	Range 65 - 120	Recovery	= 155.460%#		
66) 1,2-Dichlorobenzene-d4	12.201	152	171832	88.317	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 176.640%#		
Target Compounds						Qvalue
25) Chloroform	5.089	83	21105	7.051	ug/L	99
42) Toluene	7.970	91	7695	1.195	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
Data File : VU046124.D
Acq On : 06 Dec 2021 20:12
Operator : SY/MD
Sample : M4883-16ME
Misc : 5.16g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 07 01:13:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

