

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046106.D
 Acq On : 06 Dec 2021 13:04
 Operator : SY/MD
 Sample : M4869-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rBV	104758	114782	13.40%	1.750%
2	1.916	170	179	193	rVB	75308	96177	11.23%	1.466%
3	2.517	361	366	370	rVB	341	365	0.04%	0.006%
4	2.572	370	383	407	rBV	183423	306024	35.72%	4.666%
5	2.704	420	424	425	rBV	271	130	0.02%	0.002%
6	2.745	433	437	441	rBV2	227	250	0.03%	0.004%
7	2.797	447	453	461	rBV	444	816	0.10%	0.012%
8	3.051	523	532	545	rVB3	2291	3982	0.46%	0.061%
9	3.186	567	574	583	rVB	669	1144	0.13%	0.017%
10	3.286	602	605	608	rBV	144	148	0.02%	0.002%
11	3.353	622	626	631	rBV	119	133	0.02%	0.002%
12	4.054	838	844	846	rBB	151	173	0.02%	0.003%
13	4.080	846	852	858	rBV	172	338	0.04%	0.005%
14	4.151	871	874	876	rVV2	224	164	0.02%	0.003%
15	4.163	876	878	882	rVB2	271	196	0.02%	0.003%
16	4.192	883	887	892	rBB2	281	279	0.03%	0.004%
17	4.218	893	895	897	rBV	238	143	0.02%	0.002%
18	4.376	941	944	946	rBV	166	138	0.02%	0.002%
19	4.636	1009	1025	1049	rBV	76872	203345	23.73%	3.100%
20	4.884	1097	1102	1105	rBV2	172	190	0.02%	0.003%
21	4.925	1112	1115	1118	rBV	250	154	0.02%	0.002%
22	5.067	1143	1159	1185	rVV	142652	333981	38.98%	5.092%
23	5.260	1215	1219	1222	rBV	275	207	0.02%	0.003%
24	5.279	1222	1225	1226	rVV	254	160	0.02%	0.002%
25	5.295	1226	1230	1233	rVV	432	463	0.05%	0.007%
26	5.388	1257	1259	1265	rBV	191	122	0.01%	0.002%
27	5.626	1330	1333	1336	rBV	199	172	0.02%	0.003%
28	5.729	1343	1365	1390	rBV2	316126	856771	100.00%	13.063%
29	5.925	1423	1426	1428	rBV	198	150	0.02%	0.002%
30	6.019	1453	1455	1456	rBV	245	118	0.01%	0.002%
31	6.048	1456	1464	1470	rVV3	512	923	0.11%	0.014%
32	6.089	1474	1477	1480	rVV2	209	177	0.02%	0.003%
33	6.115	1481	1485	1492	rVB	210	239	0.03%	0.004%
34	6.176	1499	1504	1507	rBV	221	256	0.03%	0.004%
35	6.199	1507	1511	1514	rBV2	186	154	0.02%	0.002%
36	6.253	1514	1528	1546	rBV	242706	455597	53.18%	6.946%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046106.D
 Acq On : 06 Dec 2021 13:04
 Operator : SY/MD
 Sample : M4869-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.533	1606	1615	1627	rBV3	3957	7374	0.86%	0.112%
38	6.610	1636	1639	1644	rVB	221	236	0.03%	0.004%
39	6.639	1644	1648	1651	rBV	160	184	0.02%	0.003%
40	6.694	1651	1665	1683	rBV	195704	373973	43.65%	5.702%
41	7.041	1767	1773	1776	rBV2	325	356	0.04%	0.005%
42	7.102	1789	1792	1798	rVB	175	224	0.03%	0.003%
43	7.324	1856	1861	1864	rBV	194	246	0.03%	0.004%
44	7.385	1877	1880	1886	rVB	276	239	0.03%	0.004%
45	7.568	1924	1937	1958	rBV	113427	197765	23.08%	3.015%
46	7.652	1961	1963	1967	rVB2	289	175	0.02%	0.003%
47	7.687	1971	1974	1977	rBV2	211	152	0.02%	0.002%
48	7.900	2026	2040	2056	rBV	410586	712756	83.19%	10.867%
49	8.183	2113	2128	2144	rBV	77799	129781	15.15%	1.979%
50	8.269	2152	2155	2157	rBV2	233	126	0.01%	0.002%
51	8.395	2190	2194	2202	rBV2	176	149	0.02%	0.002%
52	8.482	2216	2221	2227	rVV2	199	201	0.02%	0.003%
53	8.636	2256	2269	2302	rBV	246510	429090	50.08%	6.542%
54	8.916	2349	2356	2362	rBV3	591	864	0.10%	0.013%
55	9.166	2428	2434	2438	rBV3	371	399	0.05%	0.006%
56	9.420	2500	2513	2533	rBV	345884	572984	66.88%	8.736%
57	9.572	2555	2560	2567	rBV2	401	503	0.06%	0.008%
58	9.642	2578	2582	2584	rVB2	246	130	0.02%	0.002%
59	9.700	2593	2600	2605	rVB2	891	1264	0.15%	0.019%
60	9.957	2676	2680	2682	rVB	180	138	0.02%	0.002%
61	10.102	2721	2725	2727	rBV2	330	226	0.03%	0.003%
62	10.671	2893	2902	2910	rVV3	2415	3305	0.39%	0.050%
63	10.758	2916	2929	2949	rBV	273563	440388	51.40%	6.715%
64	10.871	2958	2964	2970	rBV2	570	718	0.08%	0.011%
65	10.999	3000	3004	3008	rBV2	197	157	0.02%	0.002%
66	11.031	3008	3014	3017	rBV	104	153	0.02%	0.002%
67	11.096	3030	3034	3038	rBV2	330	290	0.03%	0.004%
68	11.121	3040	3042	3044	rVB2	290	160	0.02%	0.002%
69	11.153	3047	3052	3057	rVB3	255	223	0.03%	0.003%
70	11.362	3113	3117	3120	rBV2	176	161	0.02%	0.002%
71	11.462	3139	3148	3157	rVB4	1441	2467	0.29%	0.038%
72	11.697	3215	3221	3224	rBV	753	831	0.10%	0.013%
73	11.745	3233	3236	3237	rBV	279	140	0.02%	0.002%
74	11.813	3245	3257	3272	rBV	390288	614366	71.71%	9.367%
75	11.896	3282	3283	3289	rVB2	193	182	0.02%	0.003%
76	11.938	3293	3296	3297	rBV	508	215	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046106.D
 Acq On : 06 Dec 2021 13:04
 Operator : SY/MD
 Sample : M4869-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.977	3302	3308	3313	rVB5	1214	1508	0.18%	0.023%
78	12.121	3350	3353	3356	rBV	172	144	0.02%	0.002%
79	12.150	3360	3362	3363	rVV	364	180	0.02%	0.003%
80	12.195	3363	3376	3399	rVB	426591	675458	78.84%	10.299%
81	12.327	3413	3417	3419	rBV2	404	321	0.04%	0.005%
82	12.571	3490	3493	3496	rVB2	201	137	0.02%	0.002%
83	12.610	3502	3505	3507	rBV	277	176	0.02%	0.003%
84	12.890	3590	3592	3596	rVB2	219	126	0.01%	0.002%
85	13.182	3680	3683	3688	rVB2	174	144	0.02%	0.002%
86	13.231	3694	3698	3700	rBV2	346	185	0.02%	0.003%
87	13.571	3801	3804	3807	rBV	253	196	0.02%	0.003%
88	13.841	3884	3888	3889	rBV	465	328	0.04%	0.005%
89	14.005	3937	3939	3947	rVB	185	135	0.02%	0.002%
90	14.044	3948	3951	3955	rVB	220	143	0.02%	0.002%
91	14.092	3956	3966	3976	rBV3	1493	2523	0.29%	0.038%
92	14.330	4036	4040	4041	rBV2	468	296	0.03%	0.005%
93	14.395	4057	4060	4066	rVB2	285	292	0.03%	0.004%
94	14.475	4081	4085	4086	rBV2	282	188	0.02%	0.003%
95	14.571	4112	4115	4116	rBV	260	139	0.02%	0.002%
96	14.694	4151	4153	4158	rBV3	274	197	0.02%	0.003%
97	14.858	4201	4204	4207	rBV2	347	244	0.03%	0.004%
98	15.018	4252	4254	4256	rBV	293	186	0.02%	0.003%
99	15.227	4312	4319	4330	rBV2	1857	3123	0.36%	0.048%
100	16.182	4612	4616	4621	rBV5	500	514	0.06%	0.008%




Sum of corrected areas: 6558735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
Data File : VU046106.D
Acq On : 06 Dec 2021 13:04
Operator : SY/MD
Sample : M4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

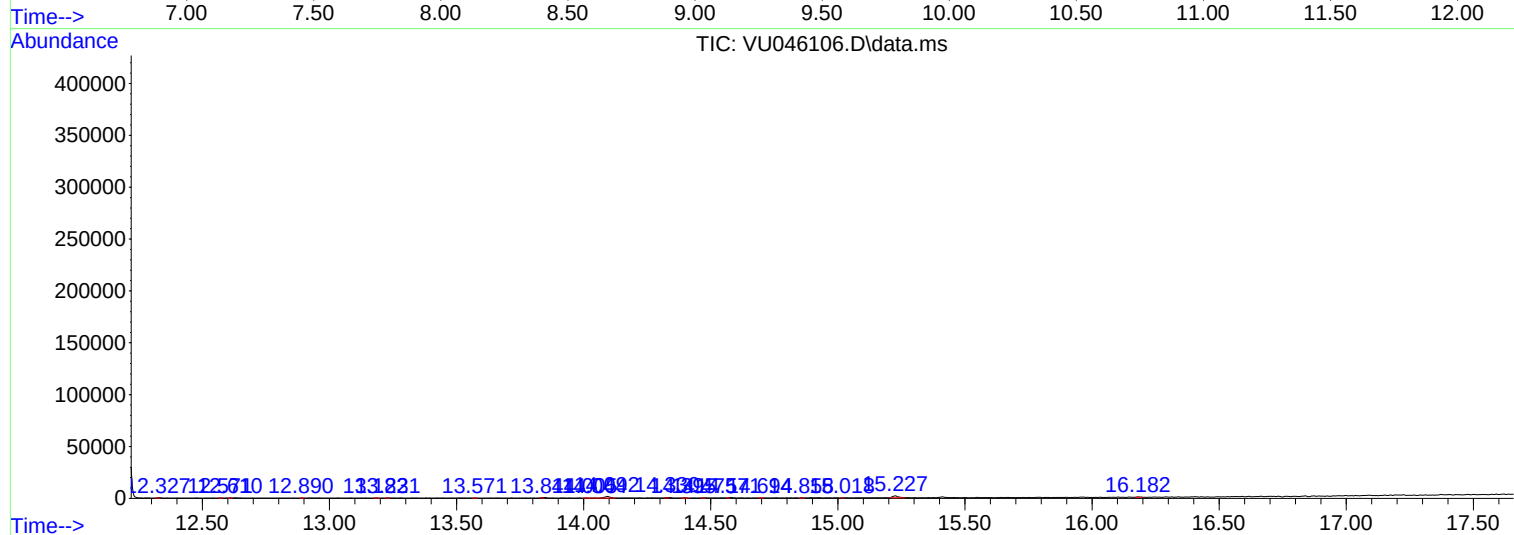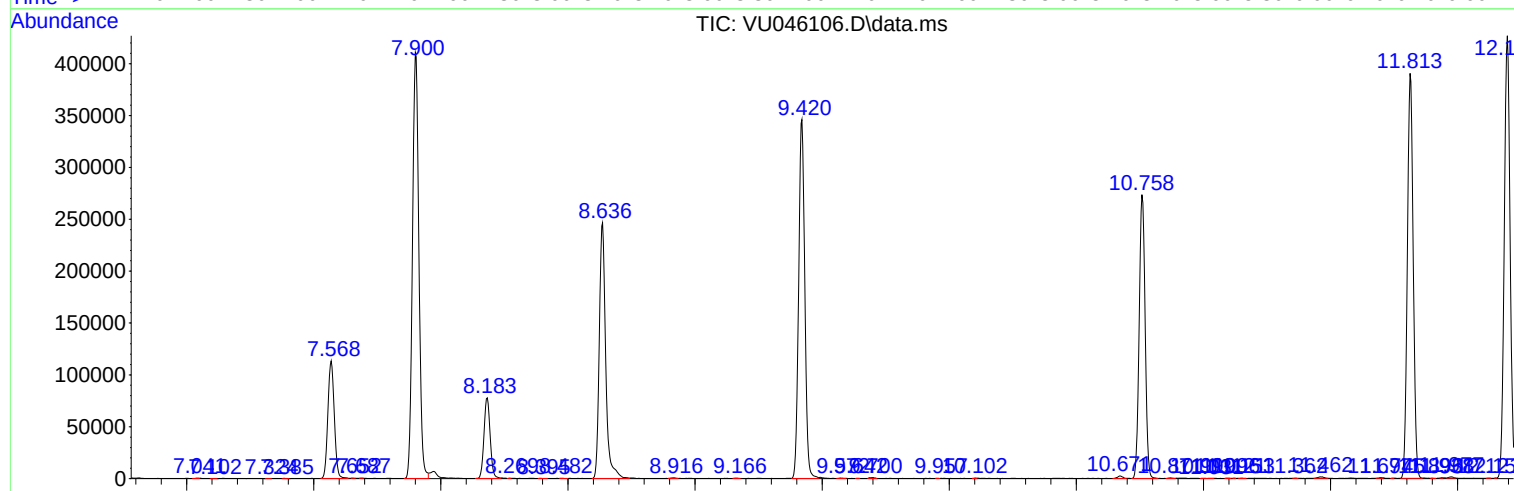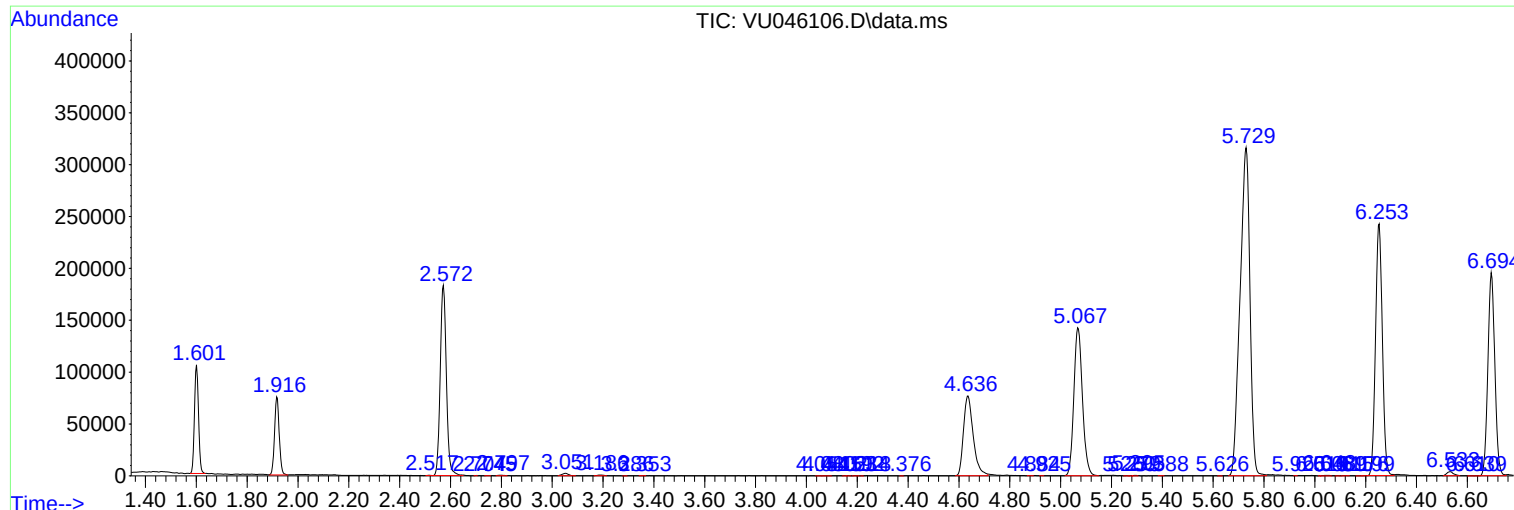

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
Data File : VU046106.D
Acq On : 06 Dec 2021 13:04
Operator : SY/MD
Sample : M4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
Data File : VU046106.D
Acq On : 06 Dec 2021 13:04
Operator : SY/MD
Sample : M4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc