
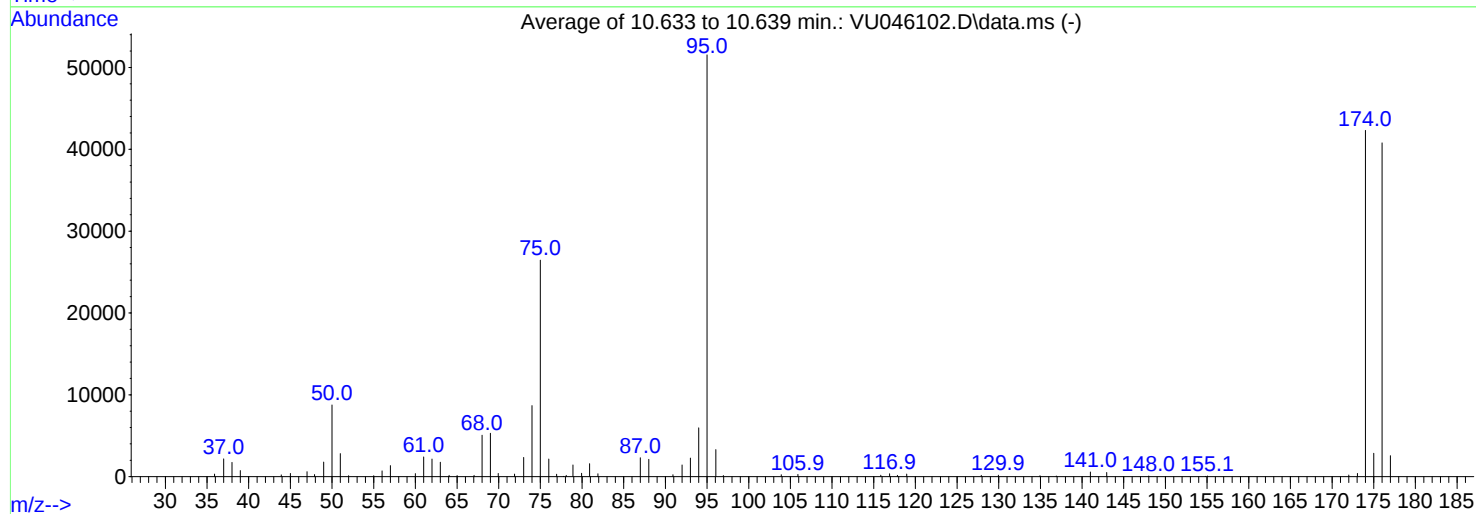


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120621\
 Data File : VU046102.D
 Acq On : 06 Dec 2021 09:53
 Operator : SY/MD
 Sample : BFB024
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB024

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

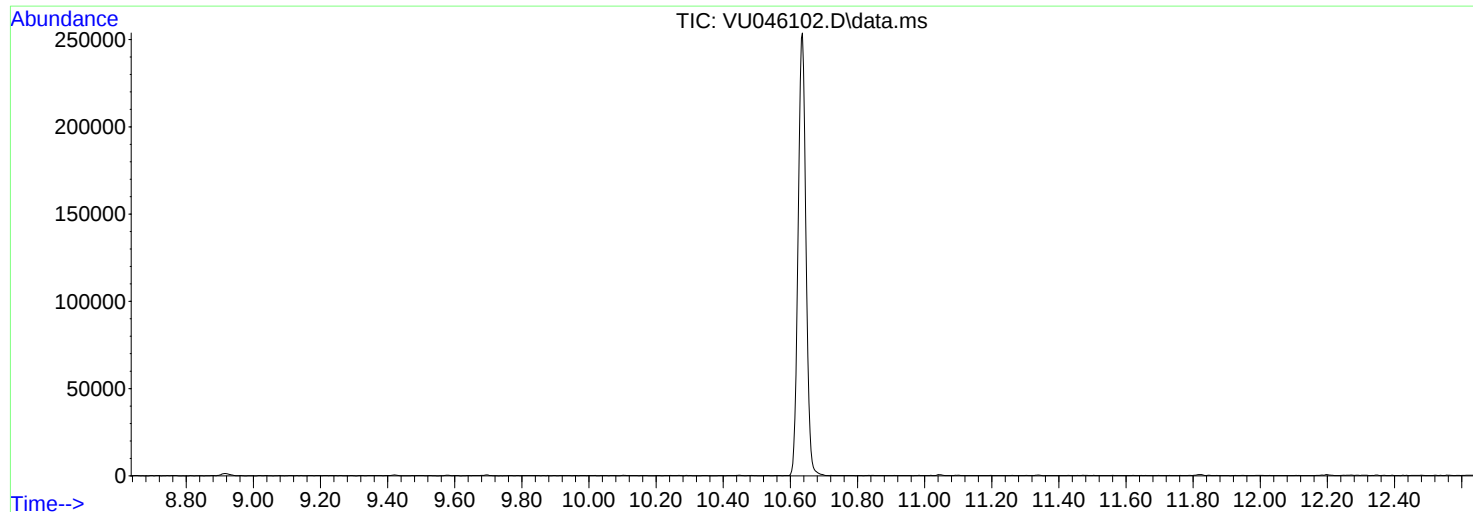

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8765	PASS
75	95	30	80	51.3	26445	PASS
95	95	100	100	100.0	51539	PASS
96	95	5	9	6.4	3297	PASS
173	174	0.00	2	0.9	395	PASS
174	95	50	120	82.1	42301	PASS
175	174	5	9	6.7	2854	PASS
176	174	95	101	96.4	40792	PASS
177	176	5	9	6.3	2562	PASS

m/z	Abundance
43.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	350.0
37.00	2311.0
38.00	1729.0
39.00	767.0
44.00	380.0
45.00	401.0
47.00	662.0
47.90	284.0
49.00	1893.0
50.00	9064.0
51.00	2888.0
52.00	126.0
55.00	131.0
56.00	711.0
57.00	1229.0
60.00	411.0
61.00	2466.0
62.00	2126.0
63.00	1695.0
64.00	152.0
65.00	132.0
67.00	141.0
68.00	5207.0
69.00	5404.0
70.00	415.0
71.90	306.0
73.00	2360.0
74.00	8924.0
75.00	27624.0
76.00	2247.0
77.00	354.0
78.10	177.0
78.90	1469.0
80.00	429.0
80.90	1662.0
81.90	360.0
87.00	2351.0
88.00	2322.0
90.90	210.0
92.00	1408.0
93.00	2298.0
94.00	6221.0
95.00	52720.0
96.00	3469.0
96.90	130.0
103.90	243.0
105.90	242.0
115.90	184.0
116.90	337.0
117.90	159.0
119.00	344.0
127.90	149.0
129.90	180.0
135.00	140.0
141.00	605.0
142.90	491.0
148.00	136.0
155.10	117.0
172.00	213.0
173.00	382.0
174.00	42424.0
175.00	2958.0
176.00	40880.0
177.00	2521.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	306.0
37.00	2250.0
38.00	1773.0
39.00	769.0
43.90	378.0
45.00	403.0
47.00	635.0
47.90	250.0
49.00	1832.0
50.00	8998.0
51.00	2913.0
52.00	124.0
55.00	122.0
56.00	720.0
57.00	1399.0
60.00	370.0
61.00	2452.0
62.00	2207.0
63.00	1815.0
64.10	149.0
65.00	136.0
67.00	169.0
68.00	5223.0
69.00	5456.0
69.90	400.0
71.90	327.0
73.00	2440.0
74.00	8974.0
75.00	27208.0
76.00	2193.0
77.00	304.0
78.10	151.0
78.90	1467.0
80.00	401.0
80.90	1647.0
81.90	361.0
87.00	2379.0
88.00	2175.0
90.90	257.0
92.00	1472.0
93.00	2351.0
94.00	6164.0
95.00	53080.0
96.00	3386.0
96.90	155.0
103.90	255.0
105.90	279.0
115.90	187.0
116.90	361.0
117.90	164.0
119.00	332.0
127.90	165.0
130.00	171.0
135.00	124.0
136.90	112.0
141.00	610.0
143.00	521.0
148.00	124.0
155.00	105.0
172.00	191.0
173.00	409.0
174.00	43696.0
175.00	2922.0
176.00	42216.0
177.00	2641.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024

m/z	Abundance
35.90	258.0
37.00	1946.0
38.00	1696.0
39.00	693.0
43.90	360.0
45.00	375.0
47.00	538.0
47.90	205.0
49.00	1625.0
50.00	8232.0
51.00	2623.0
52.00	105.0
55.00	110.0
56.00	671.0
57.00	1424.0
60.00	316.0
61.00	2270.0
62.00	2109.0
63.00	1753.0
64.10	149.0
65.00	125.0
67.10	167.0
68.00	4773.0
69.00	5039.0
69.90	360.0
71.90	297.0
73.00	2219.0
74.00	8122.0
75.00	24504.0
76.00	2004.0
76.90	237.0
77.80	148.0
78.10	150.0
78.90	1373.0
79.90	376.0
80.90	1471.0
81.90	324.0
87.00	2197.0
88.00	1867.0
90.90	251.0
92.00	1414.0
93.00	2162.0
94.00	5498.0
95.00	48816.0
96.10	3035.0
97.00	149.0
103.90	238.0
105.90	292.0
115.80	185.0
116.90	349.0
117.80	154.0
118.90	274.0
127.90	167.0
129.90	175.0
134.90	100.0
136.90	106.0
141.00	499.0
143.00	502.0
154.80	107.0
172.00	160.0
173.10	395.0
174.00	40784.0
175.00	2683.0
176.00	39280.0
177.00	2525.0

Instrument :
MSVOA_U
ClientSampleId :
BFB024