

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120622\
 Data File : VU052184.D
 Acq On : 06 Dec 2022 11:14
 Operator : JC/MD
 Sample : VU1206WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK145

Quant Time: Dec 06 21:25:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 06 21:24:57 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	197073	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	204572	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	75580	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	108703	5.671	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	113.400%	
7) Chloroethane-d5	1.913	69	88202	5.924	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	118.400%	
11) 1,1-Dichloroethene-d2	2.565	65	40396	5.879	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	117.600%	
20) 2-Butanone-d5	4.646	46	178515	51.376	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.760%	
24) Chloroform-d	5.060	84	166074	5.896	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	118.000%	
26) 1,2-Dichloroethane-d4	5.700	65	82200	5.778	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	115.600%	
32) Benzene-d6	5.726	84	336026	5.533	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	110.600%	
36) 1,2-Dichloropropane-d6	6.687	67	107003	5.693	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	113.800%	
41) Toluene-d8	7.896	98	253485	4.613	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...	8.179	79	33397	4.876	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.600%	
46) 2-Hexanone-d5	8.636	63	129465	44.602	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.200%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	85495	5.246	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.000%	
66) 1,2-Dichlorobenzene-d4	12.192	152	83234	5.752	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	115.000%	
Target Compounds						Qvalue
16) Methylene chloride	3.044	84	5309	0.274	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120622\
Data File : VU052184.D
Acq On : 06 Dec 2022 11:14
Operator : JC/MD
Sample : VU1206WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK145


Quant Time: Dec 06 21:25:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 06 21:24:57 2022
Response via : Initial Calibration

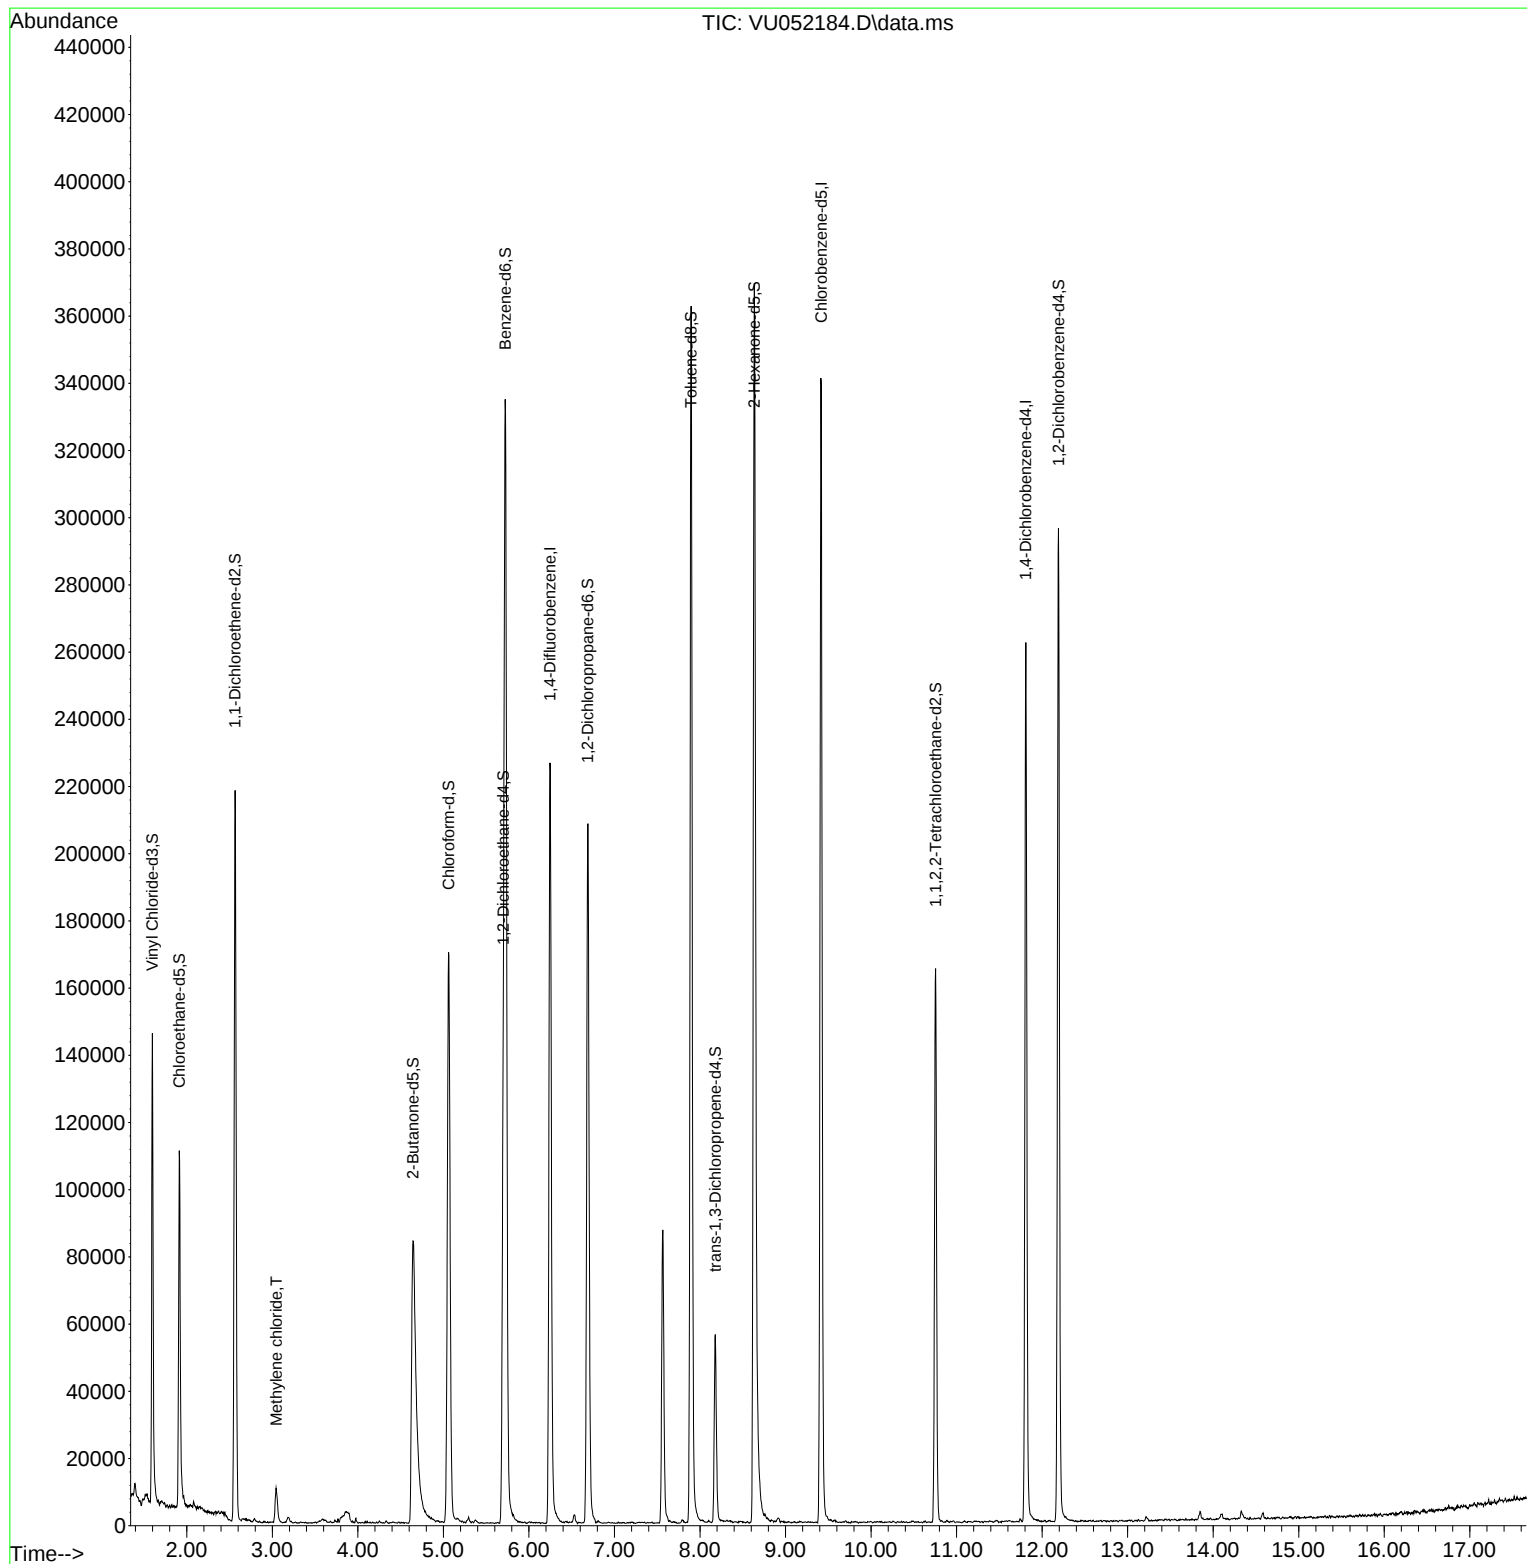

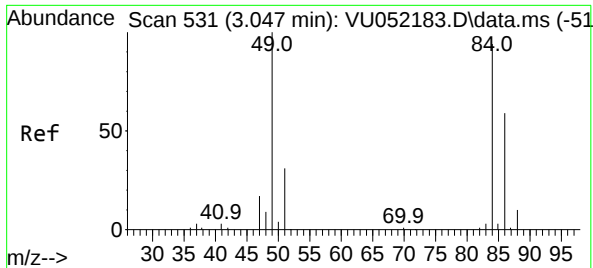

#16
Methylene chloride
Concen: 0.274 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU052184.D
Acq: 06 Dec 2022 11:14

Instrument :
MSVOA_U
ClientSampleId :
VBLK145

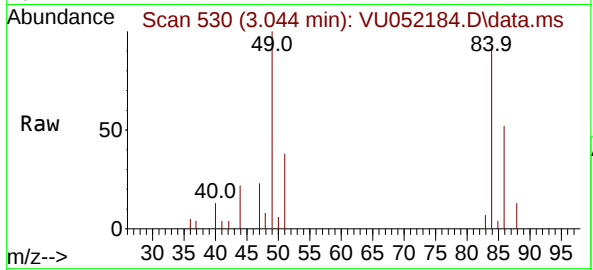

Tgt Ion:	84	Resp:	5309
Ion	Ratio	Lower	Upper
84	100		
86	56.3	43.8	81.4
49	108.2	75.9	141.1

