


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120622\
Data File : VU052182.D
Acq On : 06 Dec 2022 09:21
Operator : JC/MD
Sample : BFB173
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB173

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 08 04:19:43 2022

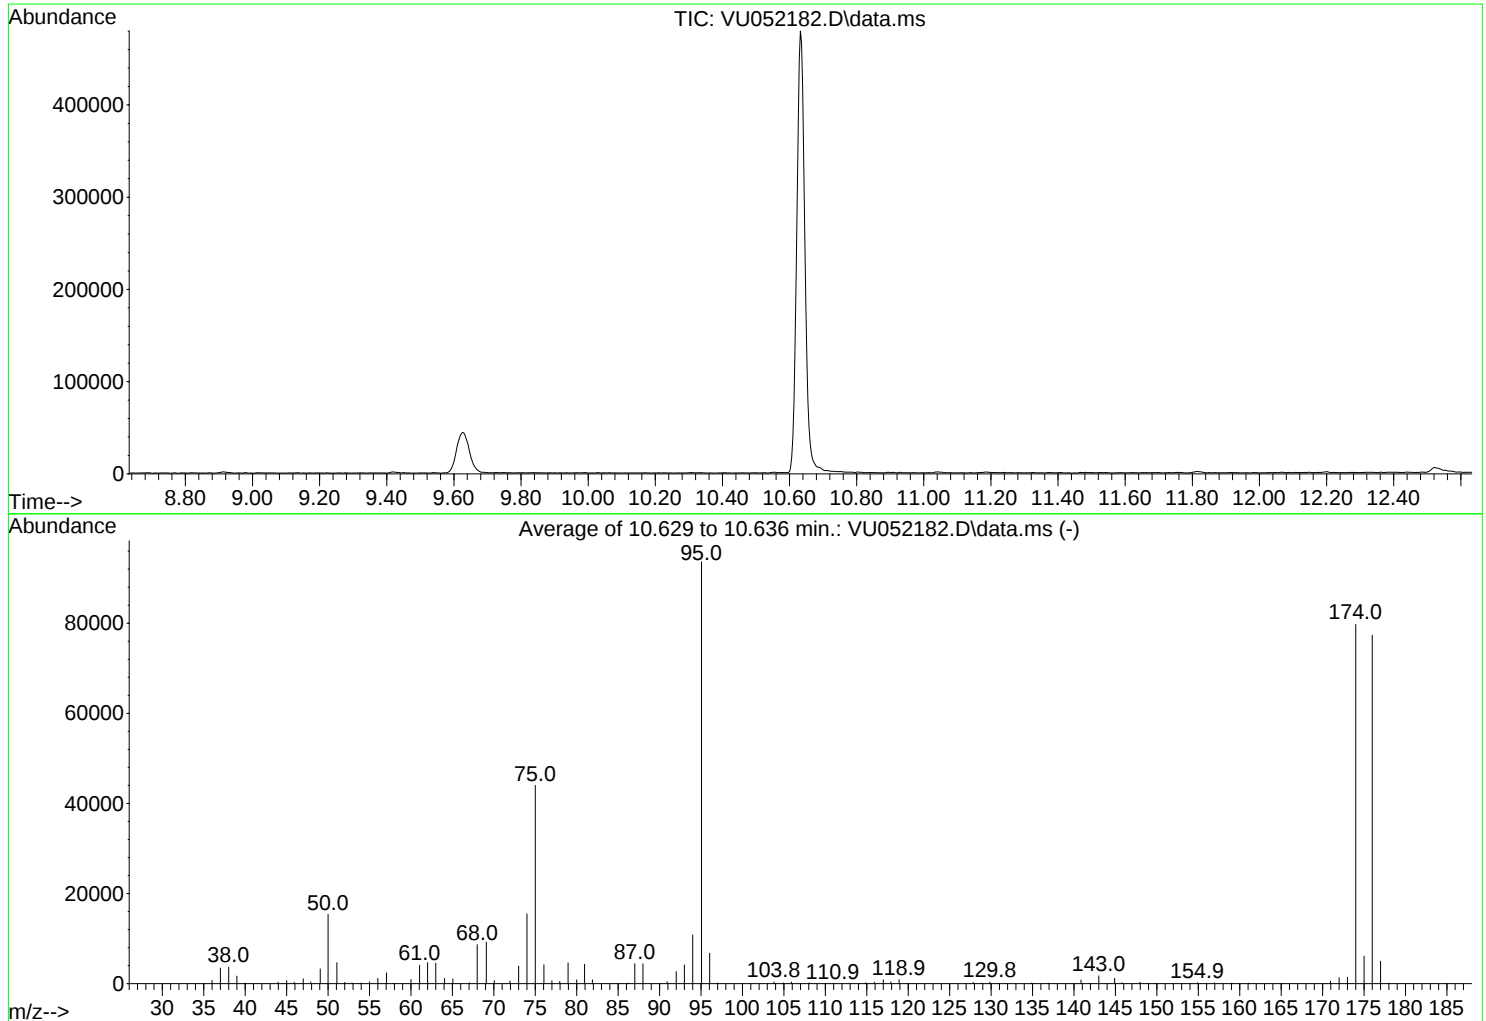

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	15366	PASS
75	95	30	80	47.0	43984	PASS
95	95	100	100	100.0	93619	PASS
96	95	5	9	7.2	6733	PASS
173	174	0.00	2	1.8	1423	PASS
174	95	50	120	85.2	79744	PASS
175	174	5	9	7.7	6115	PASS
176	174	95	101	97.0	77333	PASS
177	176	5	9	6.4	4961	PASS

Scan 2876 (10.587 min): VU052182.D\data.ms
BFB173

m/z	Abundance
40.00	264.0
44.00	894.0
150.00	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
36.00	685.0
37.00	3625.0
38.00	3677.0
39.00	1684.0
40.00	322.0
43.90	1259.0
45.00	673.0
45.90	335.0
47.00	980.0
47.90	412.0
49.10	3144.0
50.00	14992.0
51.10	4523.0
52.00	269.0
52.80	145.0
53.90	100.0
55.00	431.0
56.00	1117.0
57.10	2466.0
57.90	109.0
60.00	901.0
61.00	3873.0
62.00	4363.0
63.00	4414.0
64.10	1224.0
65.10	965.0
67.10	193.0
68.00	8482.0
69.10	9073.0
70.10	679.0
72.00	734.0
73.00	3701.0
74.00	15452.0
75.00	42392.0
76.10	4041.0
77.00	671.0
78.00	449.0
78.90	4666.0
80.00	789.0
81.00	4316.0
81.90	851.0
86.20	164.0
87.00	4293.0
88.00	4104.0
90.90	431.0
92.00	2635.0
93.00	3834.0
94.00	10595.0
95.00	91008.0
96.00	6481.0
97.00	129.0
103.80	358.0
105.00	129.0
105.90	333.0
108.10	174.0
114.80	189.0
115.90	298.0
117.00	847.0
117.90	315.0
118.90	909.0
127.80	284.0
128.90	108.0
129.80	361.0
134.80	134.0
136.80	127.0
140.80	823.0
143.00	1674.0
144.90	1231.0
145.80	236.0
148.00	302.0
148.80	107.0
149.90	187.0
153.90	116.0
154.90	233.0
156.90	168.0
159.10	122.0
161.00	120.0
170.90	546.0
172.00	1067.0
173.00	1397.0
174.00	75656.0
175.00	6176.0
176.00	73168.0
177.00	4619.0
178.00	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
36.00	735.0
37.00	3535.0
38.00	3734.0
39.00	1751.0
40.00	367.0
43.90	1213.0
45.00	695.0
45.90	347.0
47.00	1113.0
47.90	371.0
49.00	3376.0
50.00	15788.0
51.10	4778.0
52.00	289.0
52.90	149.0
54.00	140.0
55.00	426.0
56.00	1206.0
57.00	2483.0
57.90	103.0
60.00	951.0
61.00	4158.0
62.00	4779.0
63.00	4762.0
64.10	1190.0
65.00	1090.0
67.00	232.0
68.00	8957.0
69.10	9536.0
70.00	705.0
72.00	632.0
73.00	4055.0
74.00	16079.0
75.00	45152.0
76.00	4359.0
77.00	669.0
77.90	520.0
79.00	4683.0
80.00	871.0
81.00	4418.0
81.90	878.0
86.20	170.0
87.00	4541.0
88.00	4542.0
90.90	472.0
92.00	2723.0
93.00	4341.0
94.00	11141.0
95.00	96376.0
96.10	7048.0
97.00	121.0
103.80	396.0
105.00	136.0
105.90	363.0
108.00	187.0
114.80	180.0
115.90	302.0
117.00	889.0
117.90	422.0
118.90	882.0
127.80	299.0
128.90	116.0
129.90	346.0
134.80	131.0
136.90	110.0
140.90	850.0
142.00	110.0
143.00	1821.0
144.90	1211.0
145.80	196.0
147.90	312.0
150.00	197.0
153.90	127.0
154.90	228.0
157.00	169.0
159.00	159.0
161.00	119.0
171.00	585.0
172.00	1348.0
173.00	1449.0
174.00	82176.0
175.00	6347.0
176.00	79976.0
177.00	5108.0
178.00	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
36.00	691.0
37.00	3144.0
38.00	3593.0
39.00	1577.0
40.00	381.0
44.00	1221.0
45.00	690.0
45.90	336.0
47.00	1131.0
47.90	355.0
49.00	3332.0
50.00	15317.0
51.00	4689.0
52.00	288.0
53.00	176.0
54.10	167.0
55.00	368.0
56.00	1163.0
57.00	2191.0
60.00	886.0
61.10	4157.0
62.00	4770.0
63.00	4494.0
64.00	1056.0
65.00	1102.0
67.00	255.0
68.00	8570.0
69.10	9115.0
70.00	649.0
71.90	471.0
73.00	4001.0
74.00	14932.0
75.00	44408.0
76.00	4193.0
77.00	620.0
77.90	552.0
79.00	4491.0
80.00	909.0
80.90	4171.0
81.90	783.0
86.20	143.0
87.00	4488.0
88.00	4548.0
90.90	418.0
92.00	2641.0
93.00	4303.0
94.00	10684.0
95.10	93472.0
96.10	6671.0
97.00	160.0
103.80	407.0
104.90	139.0
105.90	357.0
108.00	184.0
110.90	111.0
114.90	158.0
115.90	320.0
117.00	862.0
117.90	496.0
118.90	867.0
127.90	303.0
128.80	119.0
129.90	333.0
130.80	124.0
134.90	143.0
137.00	106.0
140.90	810.0
141.90	139.0
143.00	1743.0
143.90	107.0
144.90	1035.0
145.80	177.0
147.90	306.0
150.00	245.0
154.90	233.0
156.90	155.0
159.00	144.0
161.10	102.0
171.00	554.0
172.00	1492.0
173.00	1424.0
174.00	81400.0
175.00	5821.0
176.00	78856.0
177.00	5157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173