

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
 Data File : VU056659.D
 Acq On : 06 Dec 2023 13:19
 Operator : MD/SY
 Sample : 05642-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.470	48	56	67	rBV	99587	107384	12.91%	1.561%
2	1.596	87	95	106	rVB	87475	106000	12.75%	1.541%
3	1.911	183	193	204	rBV	75240	111191	13.37%	1.616%
4	2.563	385	396	414	rBV	158156	260111	31.28%	3.781%
5	4.621	1026	1036	1061	rBV	120682	318464	38.30%	4.629%
6	5.055	1154	1171	1190	rBV	162028	366284	44.05%	5.324%
7	5.721	1355	1378	1399	rBV2	294931	781062	93.93%	11.352%
8	6.245	1526	1541	1564	rBV	284940	567774	68.28%	8.252%
9	6.685	1665	1678	1701	rBV	189016	374493	45.04%	5.443%
10	7.563	1940	1951	1966	rBV2	89914	159772	19.21%	2.322%
11	7.894	2038	2054	2074	rBV	321828	598496	71.98%	8.699%
12	8.177	2132	2142	2153	rBV3	49896	91959	11.06%	1.337%
13	8.470	2226	2233	2240	rVB4	7347	11163	1.34%	0.162%
14	8.631	2272	2283	2311	rBV2	418913	831502	100.00%	12.086%
15	9.412	2515	2526	2543	rBV	401154	717416	86.28%	10.427%
16	10.750	2931	2942	2959	rBV2	142500	241027	28.99%	3.503%
17	10.888	2975	2985	2994	rBV3	16796	26163	3.15%	0.380%
18	11.807	3257	3271	3289	rBV	396120	667085	80.23%	9.696%
19	12.190	3377	3390	3406	rBV	314918	532989	64.10%	7.747%
20	14.569	4124	4130	4140	rVB3	5636	9816	1.18%	0.143%


Sum of corrected areas: 6880151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056659.D
Acq On : 06 Dec 2023 13:19
Operator : MD/SY
Sample : 05642-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

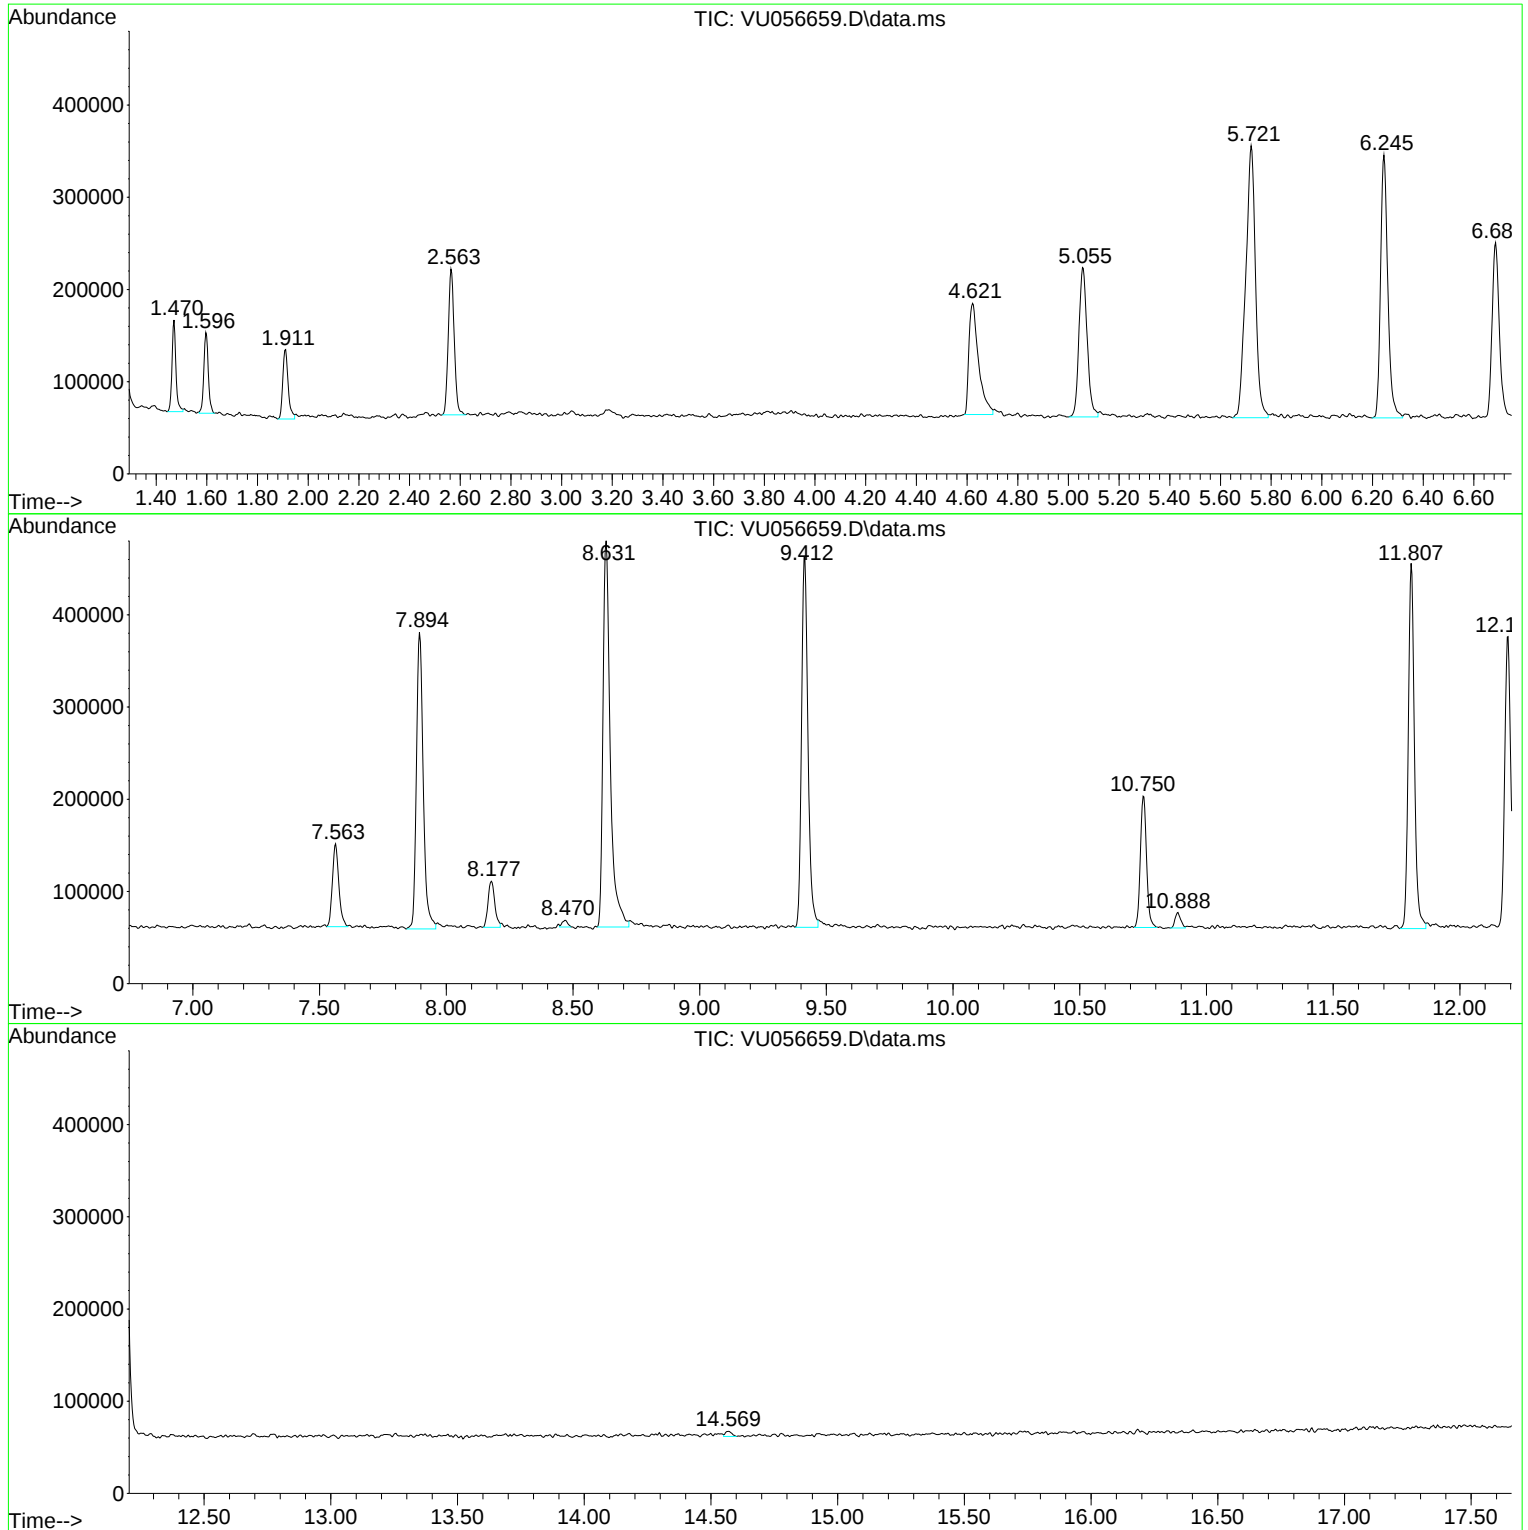

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056659.D
Acq On : 06 Dec 2023 13:19
Operator : MD/SY
Sample : 05642-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056659.D
Acq On : 06 Dec 2023 13:19
Operator : MD/SY
Sample : 05642-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc