

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
 Data File : VU056664.D
 Acq On : 06 Dec 2023 15:20
 Operator : MD/SY
 Sample : 05642-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	85	95	111	rBV	91387	113392	12.86%	1.607%
2	1.911	181	193	204	rBV	76200	105639	11.98%	1.497%
3	2.451	351	361	364	rBV	7768	11507	1.31%	0.163%
4	2.563	385	396	413	rVB	161642	265506	30.11%	3.762%
5	3.181	575	588	599	rBV5	17715	42062	4.77%	0.596%
6	4.624	1026	1037	1057	rBV	127783	348347	39.51%	4.936%
7	5.055	1158	1171	1188	rBV	164741	379963	43.09%	5.384%
8	5.721	1356	1378	1403	rBV3	304435	811981	92.09%	11.506%
9	6.245	1528	1541	1564	rBV	287068	574119	65.11%	8.135%
10	6.685	1665	1678	1696	rBV	200424	402636	45.66%	5.705%
11	7.560	1937	1950	1964	rBV2	90682	163445	18.54%	2.316%
12	7.894	2039	2054	2081	rBV	339414	624261	70.80%	8.846%
13	8.177	2131	2142	2161	rVB2	54222	101930	11.56%	1.444%
14	8.631	2273	2283	2314	rBV2	435980	881759	100.00%	12.495%
15	9.415	2510	2527	2545	rBV	412353	741155	84.05%	10.502%
16	10.749	2932	2942	2961	rBV	149002	248276	28.16%	3.518%
17	10.891	2976	2986	2990	rBV3	7218	10353	1.17%	0.147%
18	11.807	3259	3271	3288	rBV	406052	669686	75.95%	9.490%
19	12.187	3377	3389	3409	rBV	320369	561039	63.63%	7.950%




Sum of corrected areas: 7057056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056664.D
Acq On : 06 Dec 2023 15:20
Operator : MD/SY
Sample : 05642-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

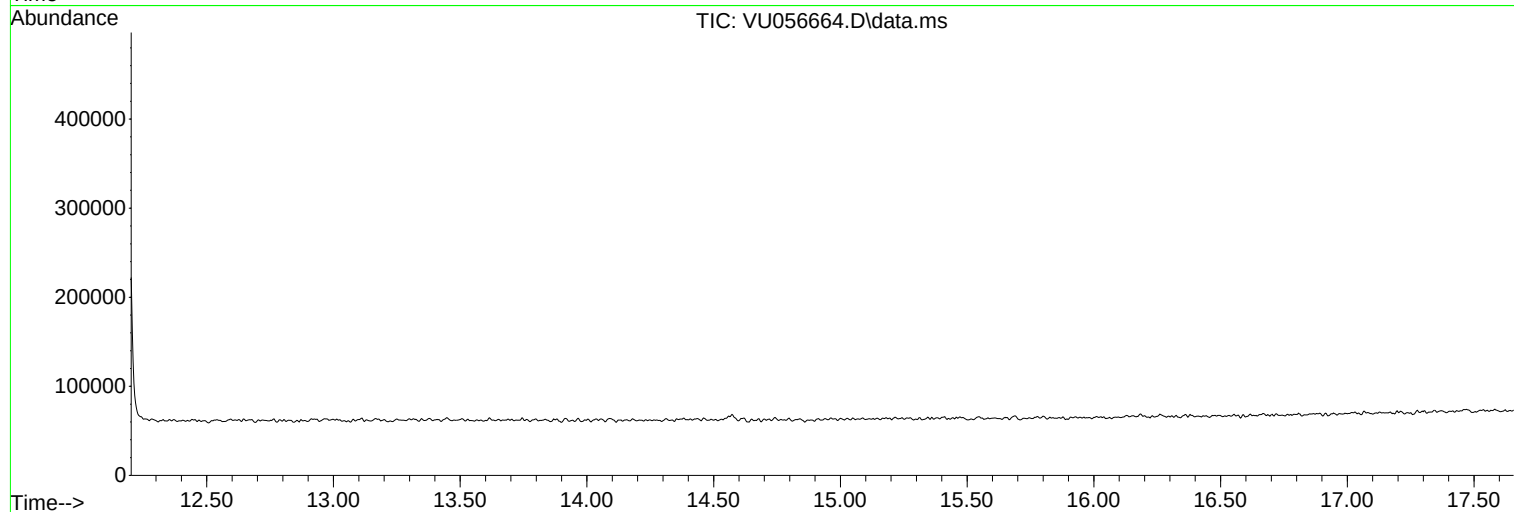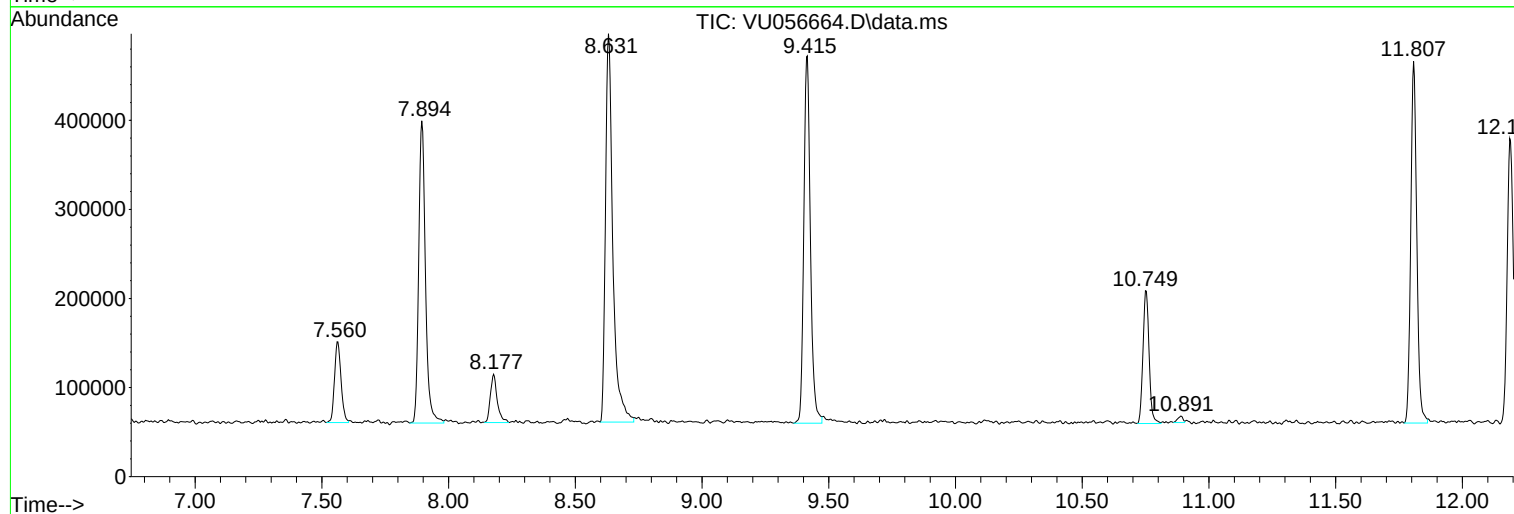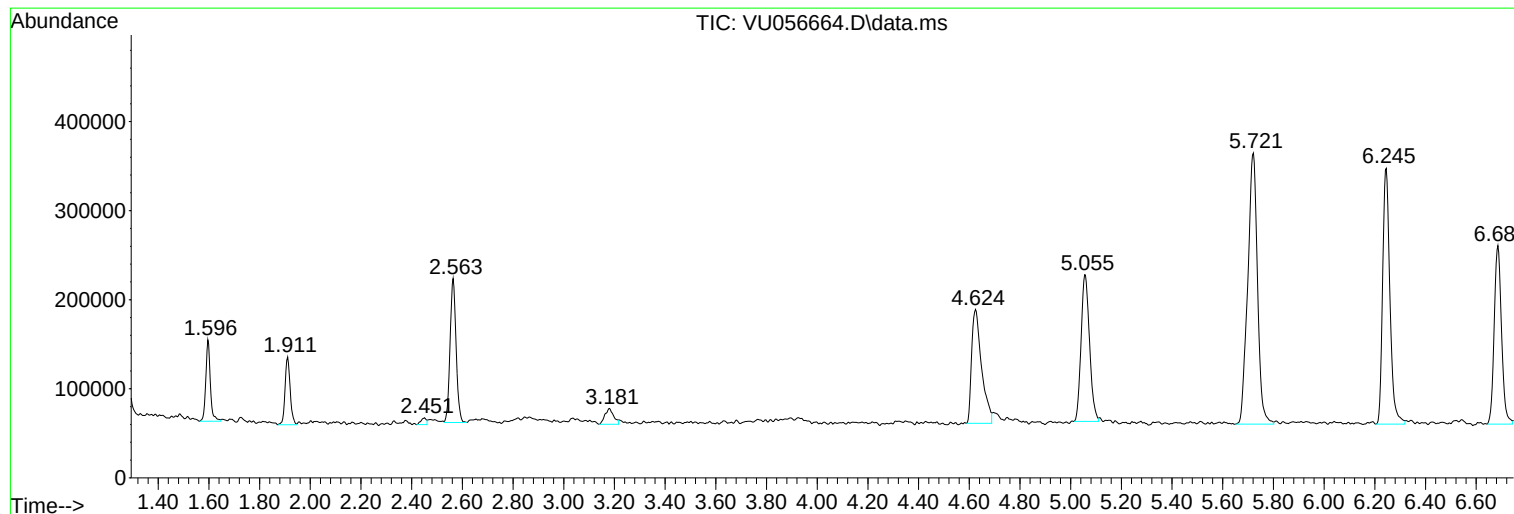

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056664.D
Acq On : 06 Dec 2023 15:20
Operator : MD/SY
Sample : 05642-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056664.D
Acq On : 06 Dec 2023 15:20
Operator : MD/SY
Sample : 05642-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc