

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
 Data File : VU056672.D
 Acq On : 06 Dec 2023 18:34
 Operator : MD/SY
 Sample : 05642-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G62

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	108	rBV	85620	99174	11.18%	1.423%
2	1.911	184	193	205	rVB	72403	100318	11.31%	1.440%
3	2.563	385	396	412	rVB	152738	250383	28.23%	3.593%
4	3.181	584	588	598	rVB2	8565	12603	1.42%	0.181%
5	4.621	1026	1036	1065	rBV2	122107	360463	40.64%	5.173%
6	5.055	1158	1171	1188	rBV	159725	344986	38.90%	4.951%
7	5.721	1360	1378	1401	rBV2	289760	762281	85.95%	10.939%
8	6.242	1530	1540	1568	rVB	296356	588940	66.40%	8.451%
9	6.541	1622	1633	1644	rBV4	25156	45206	5.10%	0.649%
10	6.685	1664	1678	1695	rBV	186651	368209	41.52%	5.284%
11	7.563	1935	1951	1964	rBV	83776	157438	17.75%	2.259%
12	7.894	2040	2054	2079	rBV	313845	582633	65.69%	8.361%
13	8.177	2130	2142	2155	rBV2	53350	94475	10.65%	1.356%
14	8.467	2225	2232	2240	rVB4	10522	16621	1.87%	0.239%
15	8.631	2272	2283	2316	rBV2	434300	886927	100.00%	12.728%
16	9.412	2512	2526	2554	rBV	422901	774787	87.36%	11.118%
17	10.749	2930	2942	2955	rBV	147273	247862	27.95%	3.557%
18	10.888	2978	2985	2997	rVB2	16221	25760	2.90%	0.370%
19	11.807	3256	3271	3291	rBV	422966	701145	79.05%	10.062%
20	12.190	3379	3390	3410	rVB	320175	535782	60.41%	7.689%
21	14.576	4124	4132	4139	rVB2	7834	12485	1.41%	0.179%




Sum of corrected areas: 6968478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056672.D
Acq On : 06 Dec 2023 18:34
Operator : MD/SY
Sample : 05642-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

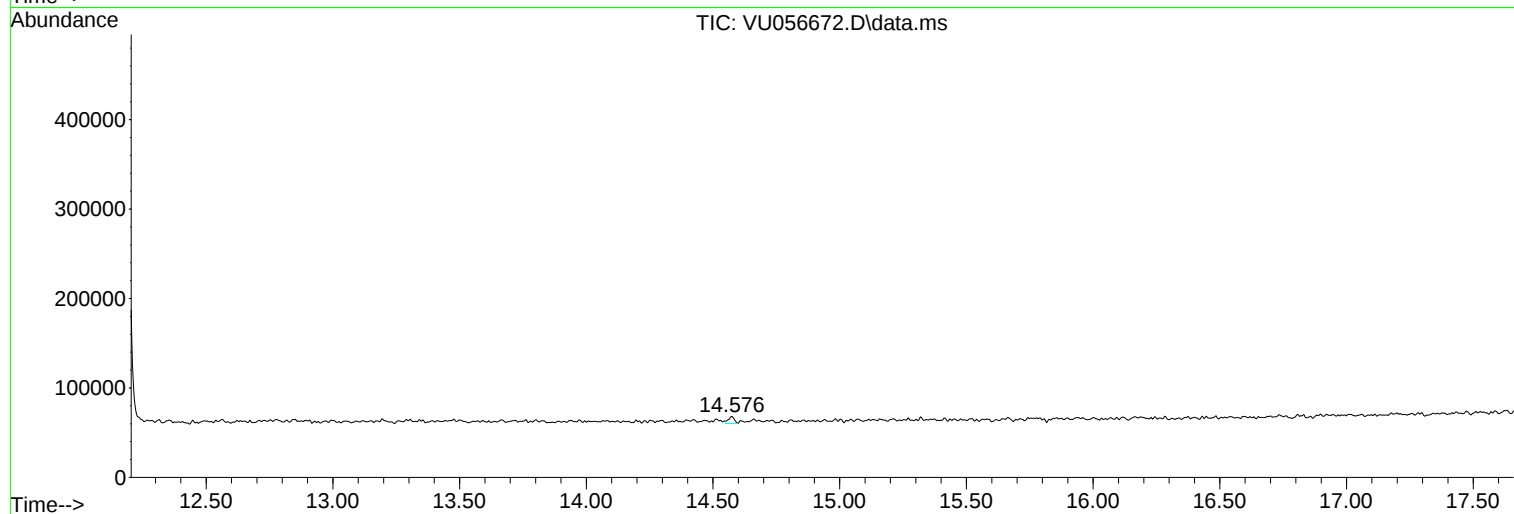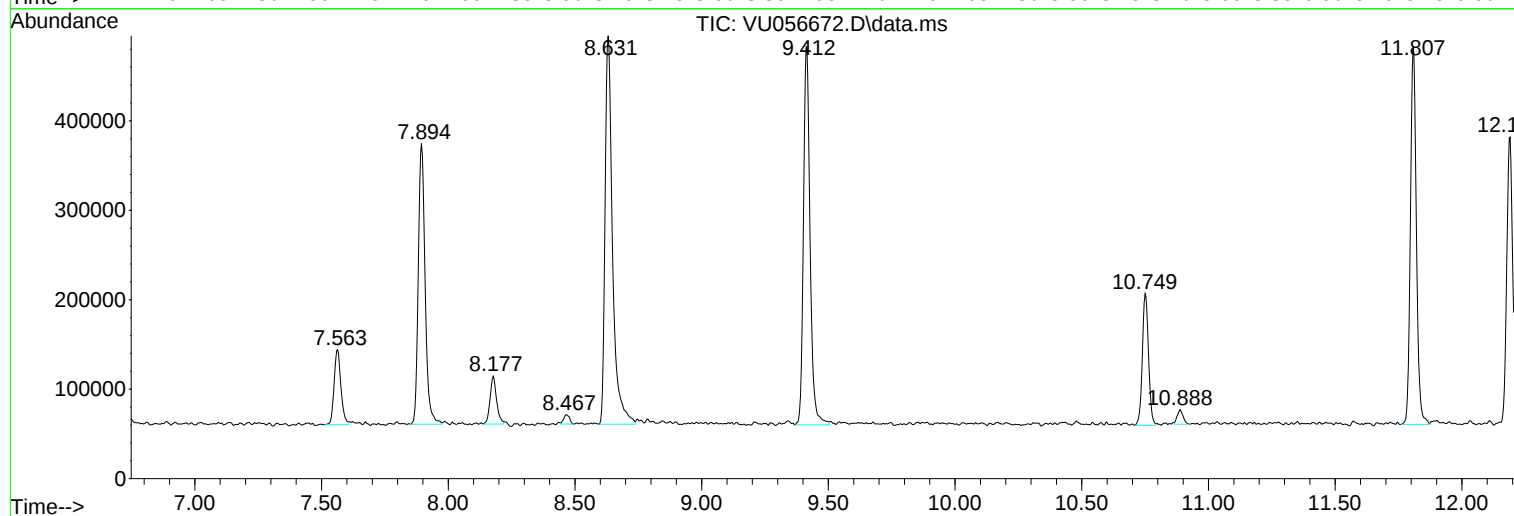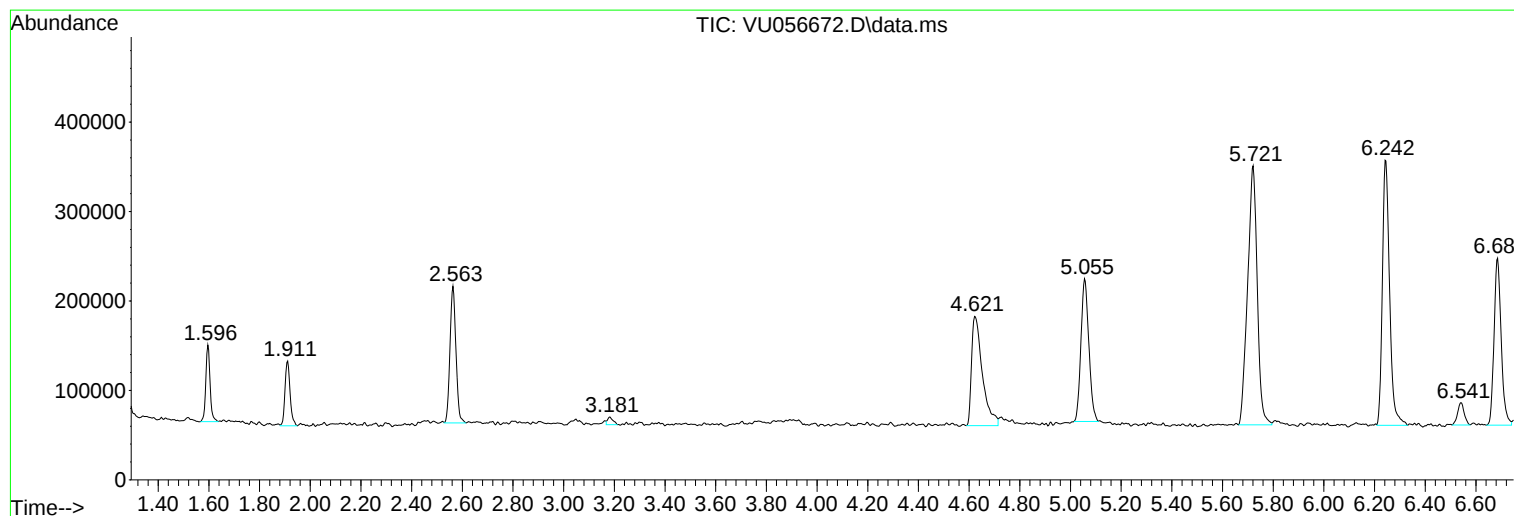

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056672.D
Acq On : 06 Dec 2023 18:34
Operator : MD/SY
Sample : 05642-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056672.D
Acq On : 06 Dec 2023 18:34
Operator : MD/SY
Sample : 05642-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc