


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120623\
Data File : VU056655.D
Acq On : 06 Dec 2023 09:11
Operator : MD/SY
Sample : BFB087
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB087

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 08 20:56:24 2023

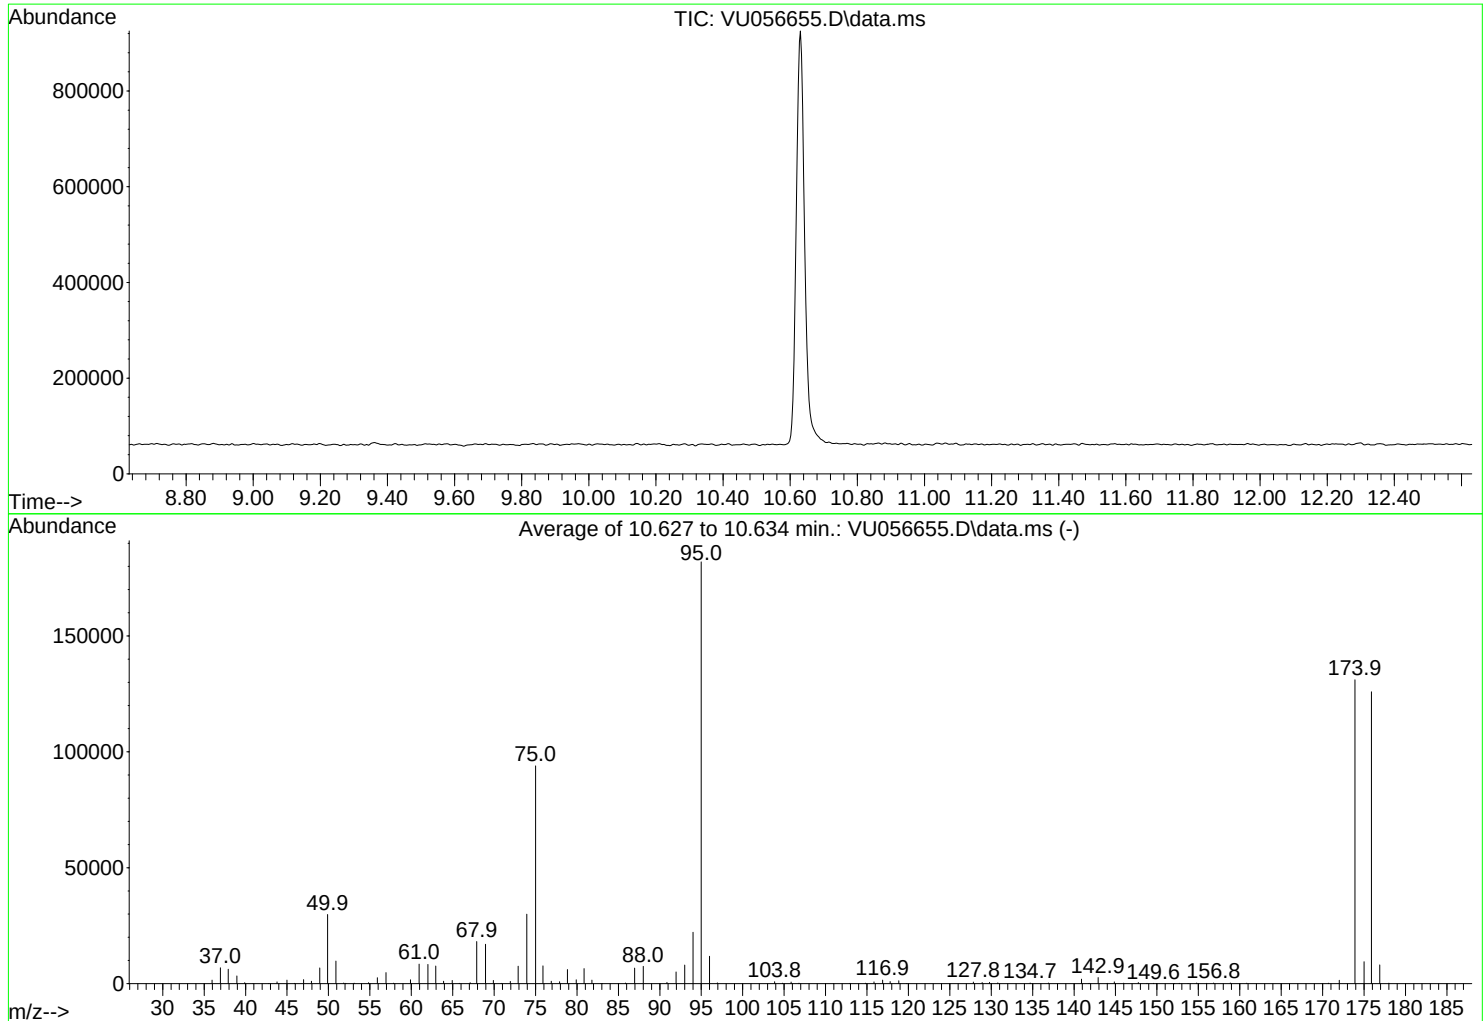

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	29792	PASS
75	95	30	80	51.6	93984	PASS
95	95	100	100	100.0	181973	PASS
96	95	5	9	6.5	11778	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	131083	PASS
175	174	5	9	7.2	9456	PASS
176	174	95	101	96.1	125933	PASS
177	176	5	9	6.4	8097	PASS

Scan 2890 (10.582 min): VU056655.D\data.ms
BFB087

m/z	Abundance
36.00	195.0
39.90	60176.0
43.80	438.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	1544.0
36.90	6882.0
37.90	6508.0
38.90	3284.0
39.90	60096.0
40.90	126.0
43.90	1344.0
45.00	1532.0
45.90	243.0
47.00	1734.0
47.90	1176.0
49.00	6726.0
49.90	30920.0
50.90	9915.0
51.80	454.0
53.10	235.0
54.80	481.0
55.90	2526.0
56.90	4848.0
57.80	213.0
59.90	1603.0
61.00	8557.0
62.00	7845.0
63.00	7680.0
63.90	1107.0
65.00	1423.0
65.80	162.0
67.10	428.0
67.90	17952.0
69.00	17040.0
69.90	1517.0
70.90	145.0
72.00	857.0
72.90	7752.0
73.90	30592.0
75.00	95408.0
75.90	7736.0
76.90	1091.0
77.90	833.0
78.80	6180.0
79.90	1709.0
80.80	6518.0
81.80	1711.0
82.90	123.0
85.90	308.0
87.00	6706.0
88.00	7345.0
90.90	652.0
92.00	5317.0
93.00	7787.0
94.00	22584.0
95.00	183872.0
96.00	11678.0
96.90	446.0
103.90	862.0
104.80	193.0
105.90	728.0
106.80	173.0
110.90	161.0
112.90	136.0
114.80	195.0
115.90	672.0
116.90	1616.0
117.80	958.0
118.90	1166.0
119.80	116.0
127.90	688.0
128.90	406.0
129.80	531.0
130.80	321.0
134.70	339.0
136.90	207.0
140.90	1940.0
141.80	198.0
142.90	2684.0
144.00	142.0
144.90	818.0
146.00	275.0
147.80	468.0
148.90	197.0
149.60	117.0
152.00	108.0
154.80	262.0
156.00	127.0
156.80	255.0
158.90	225.0
160.80	208.0
170.80	233.0
171.90	1480.0
173.90	129184.0
175.00	9224.0
175.90	123544.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

176.908128.0

178.00252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	1717.0
37.00	7011.0
37.90	6375.0
39.00	3437.0
39.90	60488.0
40.90	116.0
43.80	1167.0
45.00	1667.0
45.90	177.0
47.00	1763.0
47.90	1040.0
48.90	7011.0
49.90	30688.0
50.90	10035.0
51.90	396.0
53.10	178.0
54.90	402.0
55.90	2677.0
56.90	4997.0
57.90	229.0
59.90	1730.0
60.90	8682.0
62.00	8463.0
63.00	7864.0
63.90	1100.0
64.90	1398.0
65.80	161.0
67.10	472.0
67.90	18760.0
68.90	17424.0
69.90	1382.0
70.90	139.0
71.90	975.0
72.90	7570.0
73.90	30536.0
75.00	96496.0
75.90	7888.0
76.90	1047.0
77.90	872.0
78.80	6214.0
79.90	1667.0
80.90	6735.0
81.80	1514.0
83.10	134.0
85.80	297.0
86.90	6847.0
88.00	7785.0
90.90	589.0
91.90	5163.0
93.00	8347.0
94.00	22928.0
95.00	187072.0
96.00	12195.0
96.90	369.0
103.90	883.0
104.80	259.0
105.90	724.0
106.80	191.0
111.00	121.0
112.90	157.0
114.90	222.0
115.80	814.0
116.90	1623.0
117.80	965.0
118.80	1249.0
119.80	123.0
127.90	711.0
128.90	491.0
129.80	610.0
130.80	343.0
134.70	350.0
136.90	278.0
140.90	1997.0
141.80	145.0
142.90	2703.0
144.00	160.0
144.90	729.0
146.00	248.0
147.80	502.0
148.80	143.0
149.60	152.0
150.00	108.0
152.70	164.0
153.70	135.0
154.80	278.0
156.00	187.0
156.90	306.0
158.90	291.0
160.90	187.0
170.70	219.0
172.00	1473.0
173.90	134720.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

175.00	9687.0
175.90	129680.0
176.90	8355.0
178.00	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
36.00	1855.0
37.00	6692.0
37.90	5844.0
39.00	3225.0
39.90	61112.0
42.80	151.0
43.90	1101.0
45.00	1463.0
47.00	1650.0
48.00	888.0
48.90	6601.0
49.90	27768.0
50.90	9252.0
52.10	362.0
53.10	114.0
54.90	322.0
55.90	2457.0
57.00	4447.0
57.90	214.0
59.90	1636.0
60.90	7987.0
62.00	8467.0
62.90	7278.0
63.90	1020.0
64.90	1344.0
65.80	139.0
67.10	440.0
67.90	17712.0
68.90	16592.0
69.90	1229.0
70.80	109.0
71.90	981.0
72.90	7245.0
74.00	28792.0
75.00	90048.0
75.90	7303.0
76.90	1040.0
77.90	813.0
78.90	5897.0
79.90	1576.0
80.90	6222.0
81.80	1322.0
83.00	121.0
85.80	273.0
86.90	6628.0
88.00	7208.0
90.80	481.0
91.90	4748.0
93.00	8002.0
94.00	20904.0
95.00	174976.0
96.00	11460.0
97.00	323.0
103.80	863.0
104.80	255.0
105.80	663.0
106.80	208.0
113.00	164.0
114.90	203.0
115.80	838.0
116.90	1423.0
117.80	838.0
118.80	1244.0
127.80	719.0
128.90	486.0
129.80	535.0
130.80	295.0
134.70	255.0
136.90	300.0
140.90	1848.0
141.80	127.0
142.90	2418.0
144.00	145.0
144.80	716.0
146.00	218.0
147.70	423.0
148.70	120.0
149.60	131.0
149.90	124.0
152.70	202.0
153.80	136.0
154.80	266.0
156.00	151.0
156.90	356.0
158.80	250.0
160.90	159.0
170.60	172.0
172.10	1401.0
173.90	129344.0
175.00	9456.0
175.90	124576.0
176.90	7807.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

178.00

131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087