

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
 Data File : VU028532.D
 Acq On : 07 Dec 2018 15:23
 Operator : MD/SY
 Sample : J6299-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F39

Quant Time: Dec 11 01:22:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 11 00:46:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	104216	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	100504	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46513	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	65614	67.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	134.84%
7) Chloroethane-d5	1.68	69	49468	67.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	135.60%#
11) 1,1-Dichloroethene-d2	2.27	63	87229	50.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.66%
21) 2-Butanone-d5	4.17	46	106420	136.15	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	136.15%#
24) Chloroform-d	4.65	84	102323	66.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	132.86%#
26) 1,2-Dichloroethane-d4	5.31	65	70667	69.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	139.16%#
32) Benzene-d6	5.34	84	217331	69.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	138.32%#
36) 1,2-Dichloropropane-d6	6.33	67	78372	69.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	138.88%#
41) Toluene-d8	7.57	98	188849	65.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	131.82%#
43) trans-1,3-Dichloropropene-	7.85	79	35350	68.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	136.98%#
47) 2-Hexanone-d5	8.31	63	75364	137.90	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	137.90%#
57) 1,1,2,2-Tetrachloroethane-	10.43	84	97114	66.24	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	132.48%#
64) 1,2-Dichlorobenzene-d4	11.86	152	66894	70.89	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	141.78%#


Target Compounds					Qvalue
13) Acetone	2.32	43	6792	7.772 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
Data File : VU028532.D
Acq On : 07 Dec 2018 15:23
Operator : MD/SY
Sample : J6299-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F39

Quant Time: Dec 11 01:22:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 11 00:46:45 2018
Response via : Initial Calibration

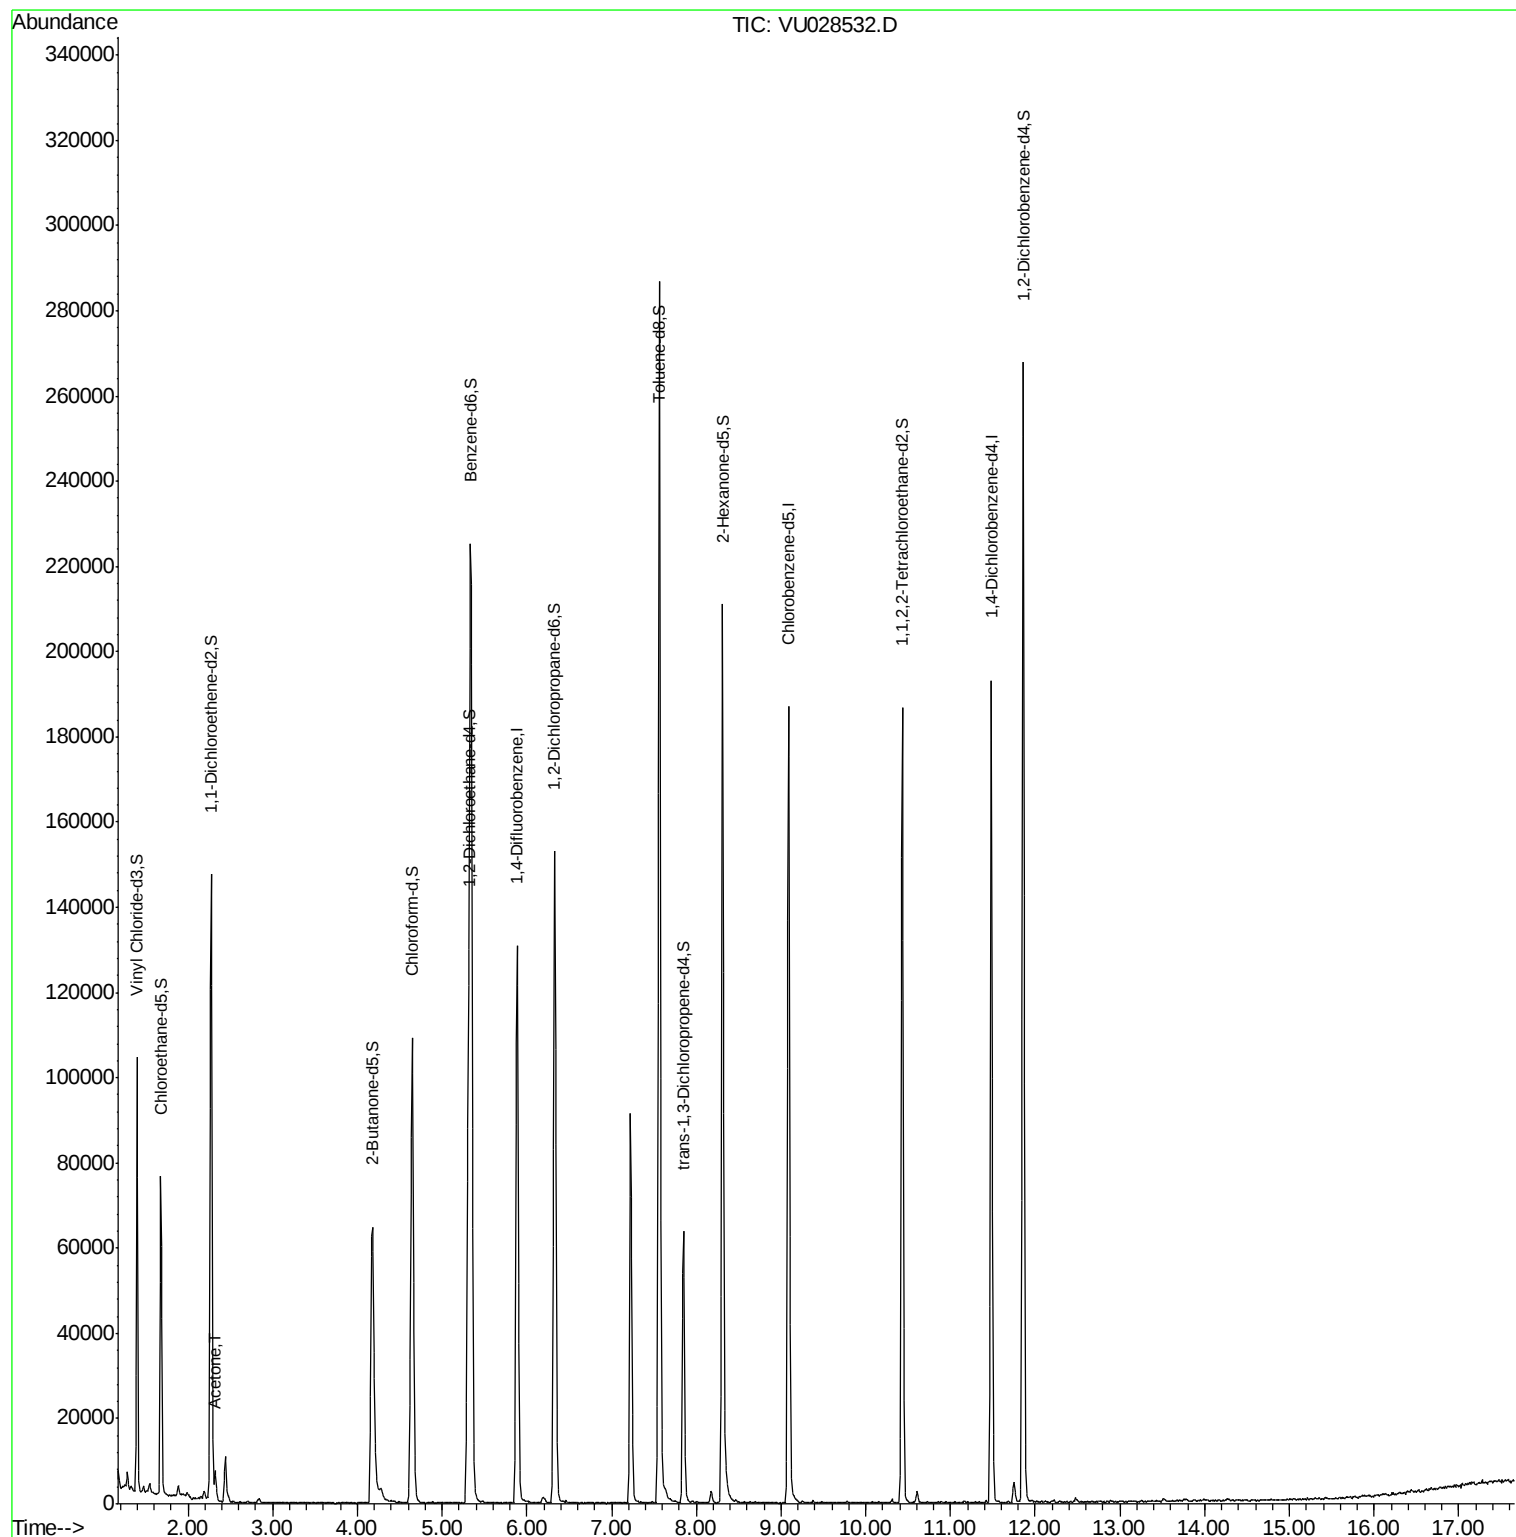

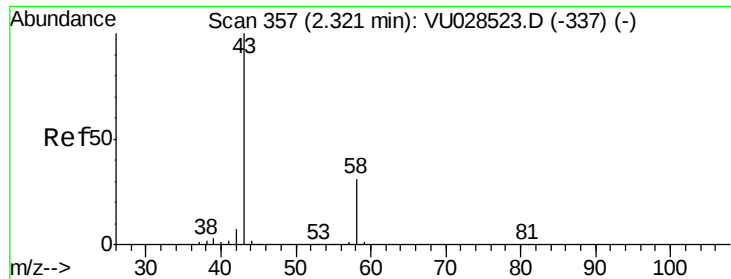

#13

Acetone

Concen: 7.772 ug/L

RT: 2.32 min Scan# 356

Delta R.T. -0.00 min

Lab File: VU028532.D

Acq: 07 Dec 2018 15:23

Instrument :

MSVOA_U

ClientSampleId :

F9F39

Tgt Ion: 43 Resp: 6792

Ion Ratio Lower Upper

43 100

58 26.9 0.0 62.0

