

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
 Data File : VU028534.D
 Acq On : 07 Dec 2018 16:10
 Operator : MD/SY
 Sample : J6236-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F38

Quant Time: Dec 11 01:27:53 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 11 00:46:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	133145	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	124897	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	58118	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	60757	48.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.72%
7) Chloroethane-d5	1.68	69	47271	50.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	101.44%
11) 1,1-Dichloroethene-d2	2.27	63	82702	37.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.44%
21) 2-Butanone-d5	4.18	46	106544	106.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.69%
24) Chloroform-d	4.65	84	98080	49.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.68%
26) 1,2-Dichloroethane-d4	5.31	65	67124	51.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.46%
32) Benzene-d6	5.34	84	204420	52.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.70%
36) 1,2-Dichloropropane-d6	6.33	67	74826	53.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.70%
41) Toluene-d8	7.57	98	179640	50.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.90%
43) trans-1,3-Dichloropropene-	7.85	79	33620	52.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	104.82%
47) 2-Hexanone-d5	8.31	63	75009	110.44	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.44%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	93906	51.54	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.08%
64) 1,2-Dichlorobenzene-d4	11.86	152	62224	52.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.54%


Target Compounds					Qvalue
13) Acetone	2.32	43	7007	6.276 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
Data File : VU028534.D
Acq On : 07 Dec 2018 16:10
Operator : MD/SY
Sample : J6236-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F38

Quant Time: Dec 11 01:27:53 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 11 00:46:45 2018
Response via : Initial Calibration

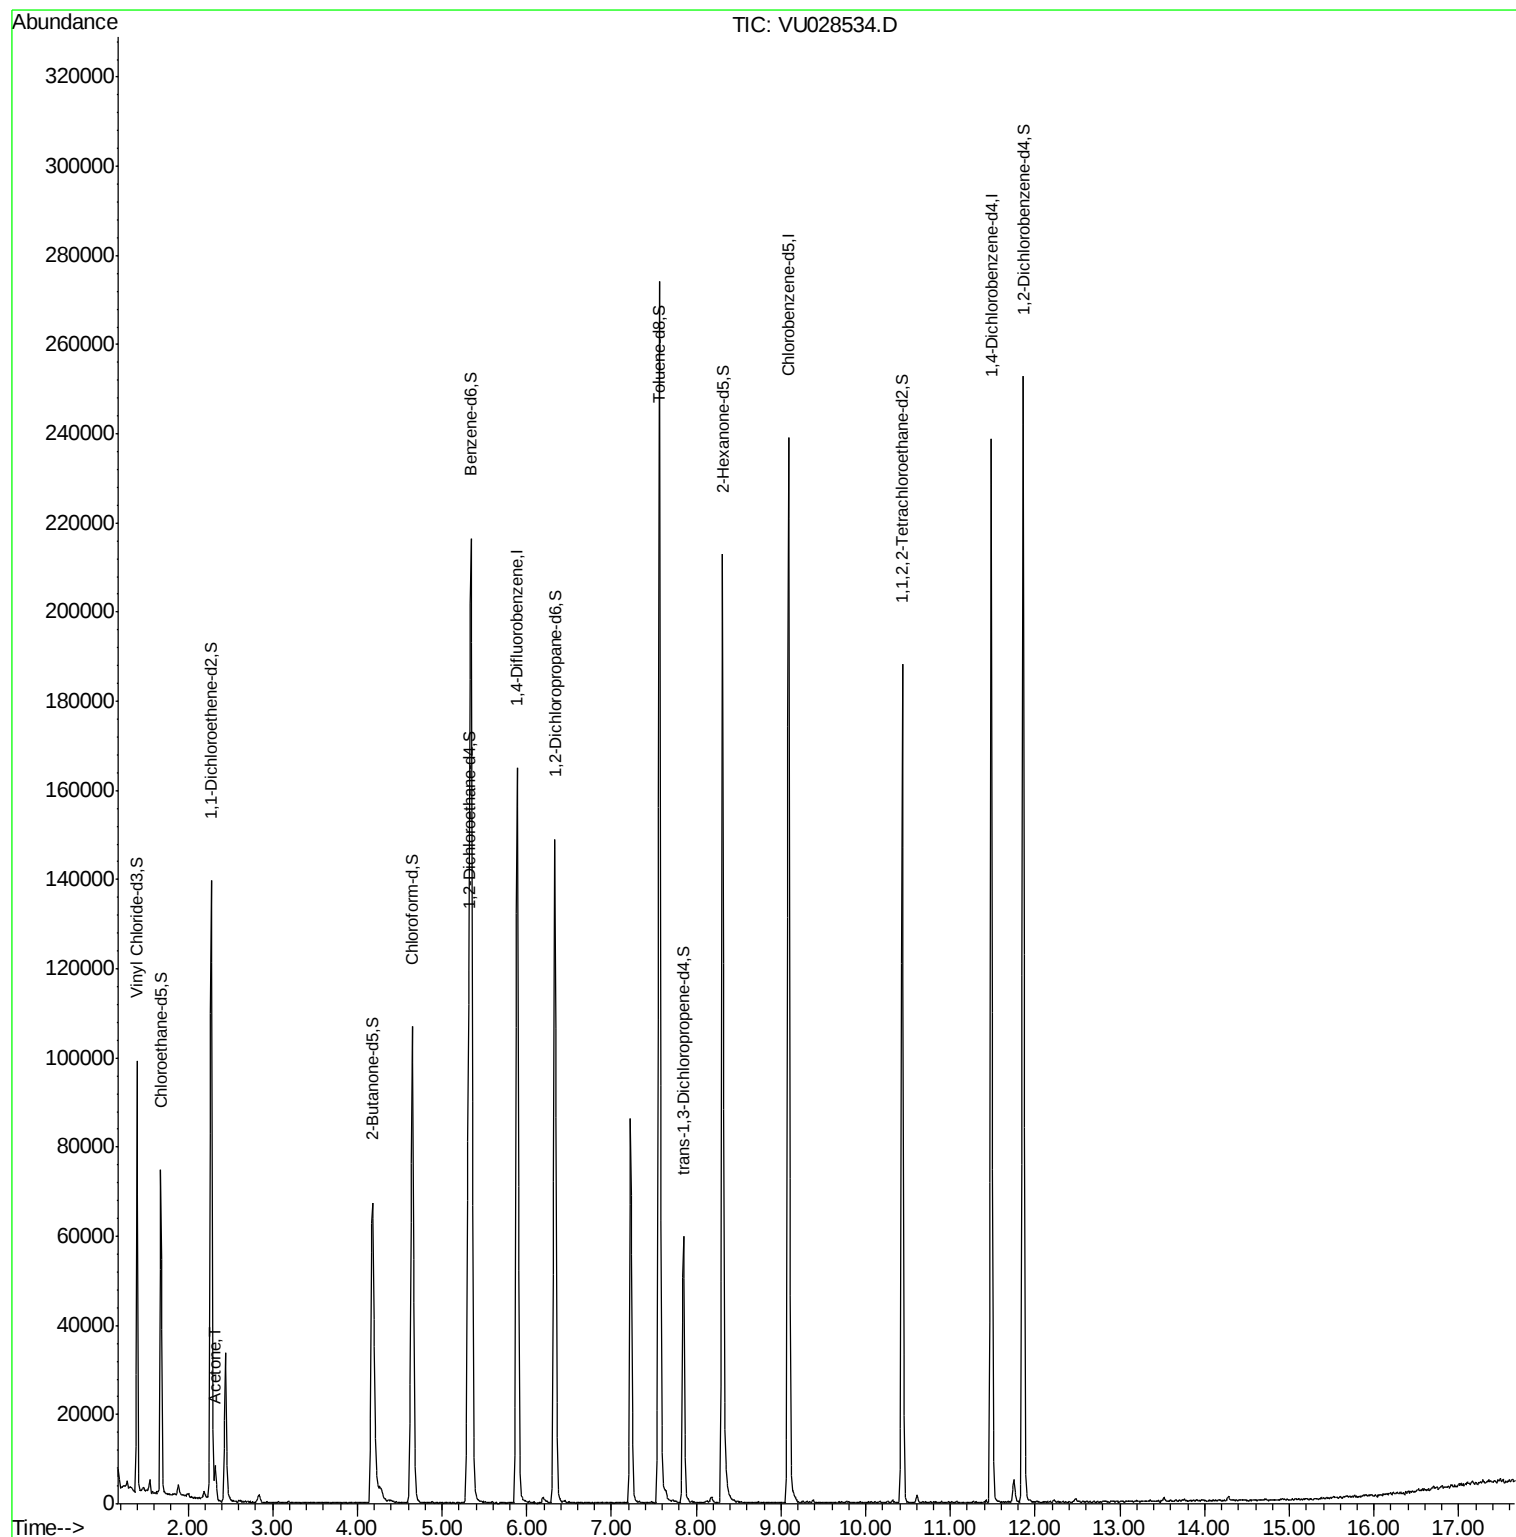

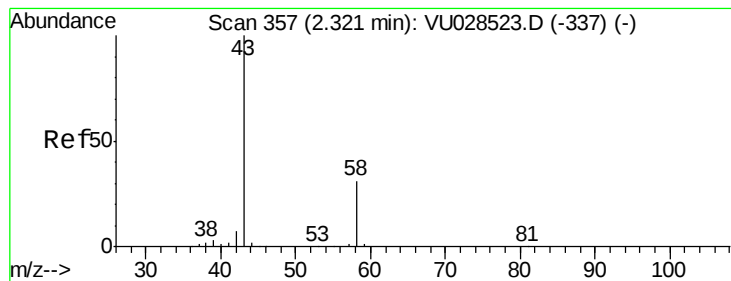

#13
 Acetone
 Concen: 6.276 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. -0.00 min
 Lab File: VU028534.D
 Acq: 07 Dec 2018 16:10

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F38

Tgt Ion: 43 Resp: 7007
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 62.0

