

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U120718\
 Data File : VU028537.D
 Acq On : 07 Dec 2018 17:23
 Operator : MD/SY
 Sample : J6299-12RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F39RE

Quant Time: Dec 11 01:41:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 11 00:46:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	130723	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	125734	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	59216	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	80700	66.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	132.20%
7) Chloroethane-d5	1.68	69	63472	69.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	138.72%#
11) 1,1-Dichloroethene-d2	2.27	63	111261	51.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.36%
21) 2-Butanone-d5	4.17	46	145017	147.91	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	147.91%#
24) Chloroform-d	4.65	84	133371	69.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	138.04%#
26) 1,2-Dichloroethane-d4	5.31	65	92041	72.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	144.50%#
32) Benzene-d6	5.34	84	280776	71.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	142.84%#
36) 1,2-Dichloropropane-d6	6.33	67	102217	72.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	144.80%#
41) Toluene-d8	7.57	98	248762	69.40	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	138.80%#
43) trans-1,3-Dichloropropene-	7.85	79	46179	71.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	143.04%#
47) 2-Hexanone-d5	8.31	63	101501	148.45	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	148.45%#
57) 1,1,2,2-Tetrachloroethane-	10.43	84	128969	70.31	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	140.62%#
64) 1,2-Dichlorobenzene-d4	11.86	152	87827	73.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	146.20%#


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.32	43	6884	6.280	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
Data File : VU028537.D
Acq On : 07 Dec 2018 17:23
Operator : MD/SY
Sample : J6299-12RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9F39RE

Quant Time: Dec 11 01:41:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 11 00:46:45 2018
Response via : Initial Calibration

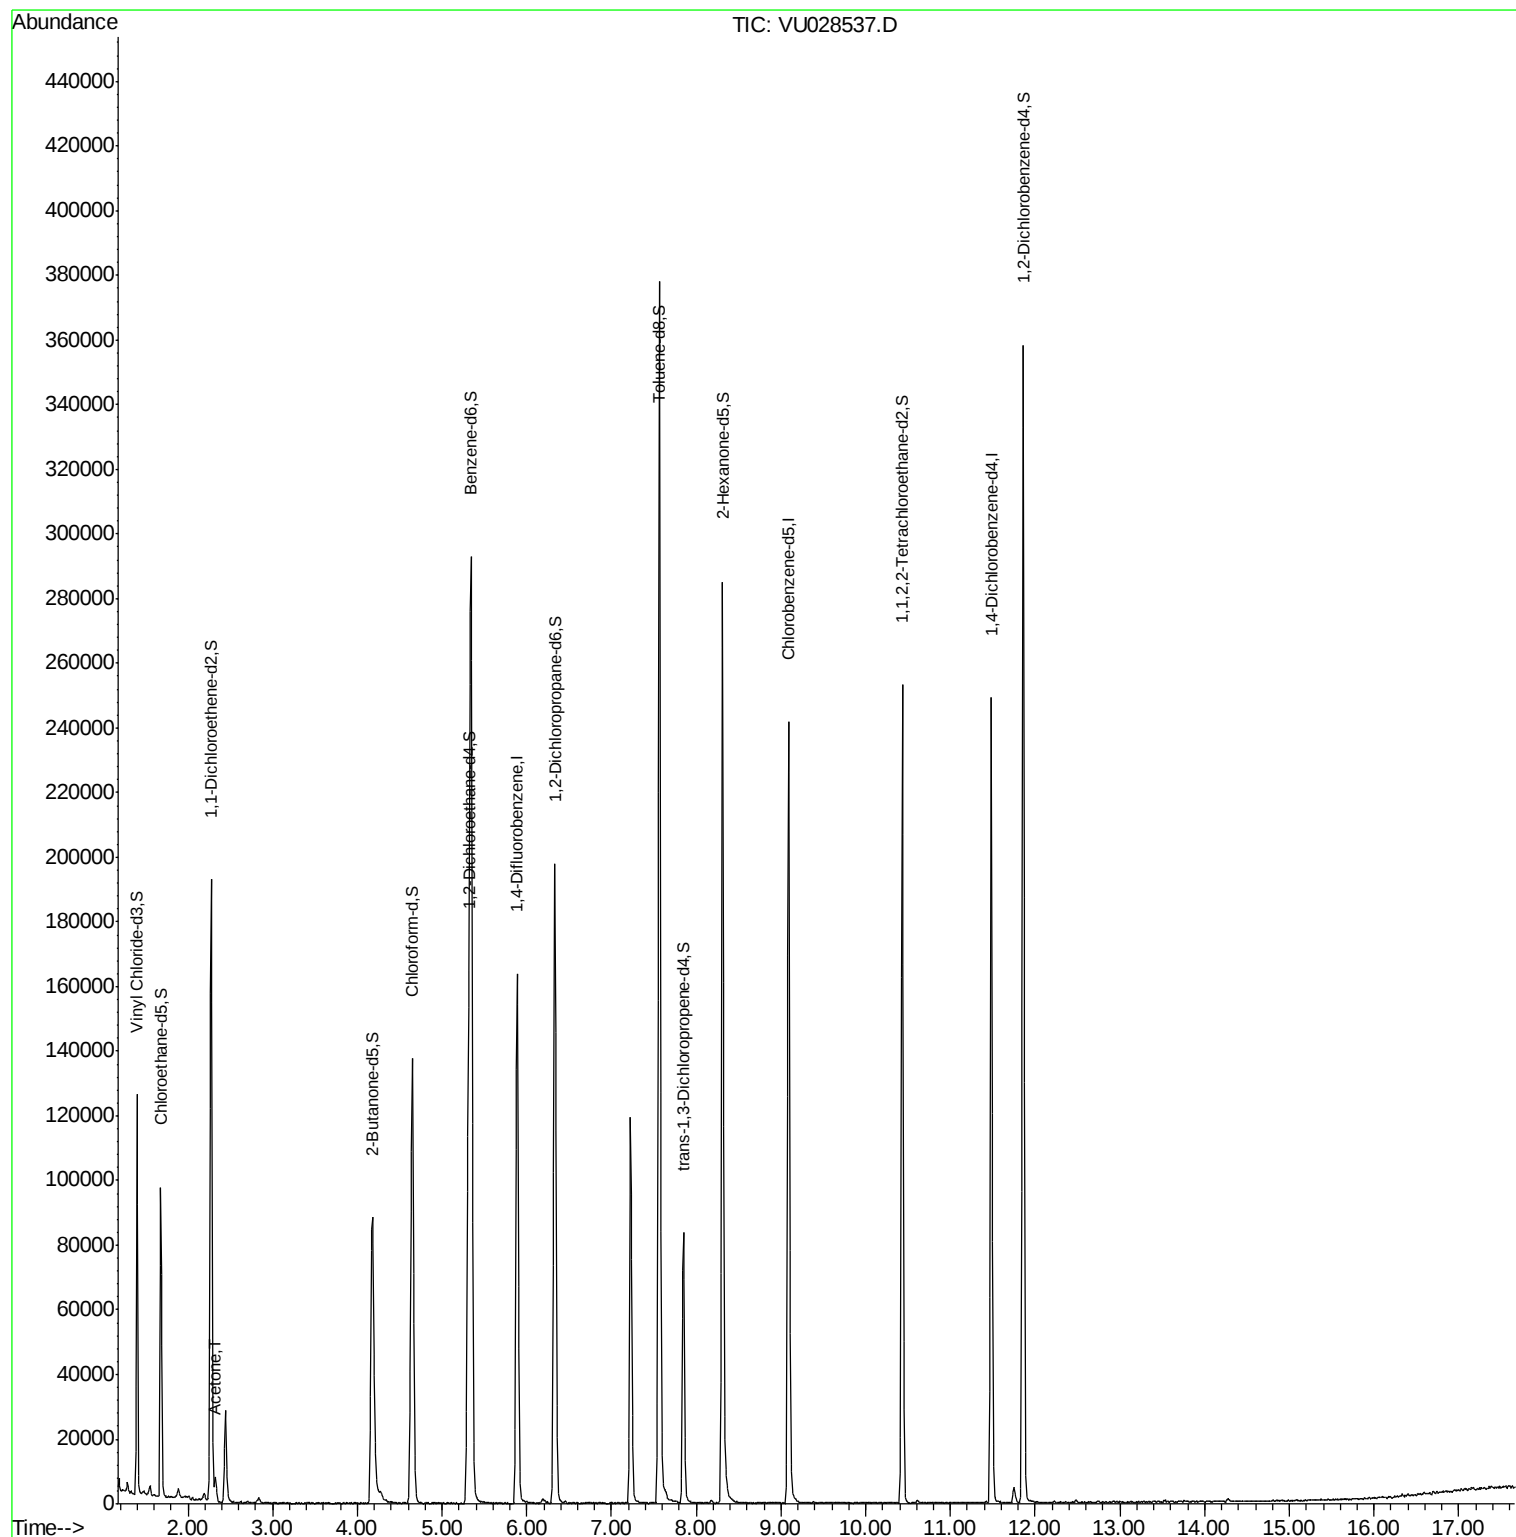

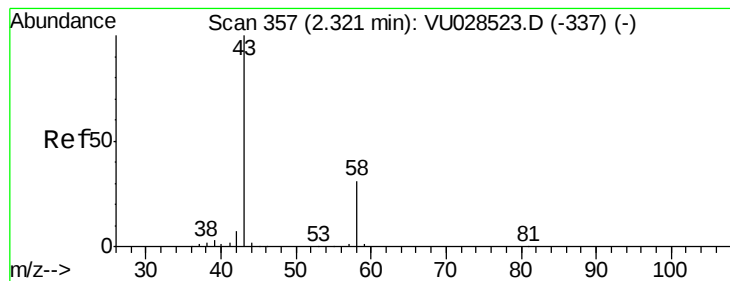

#13
 Acetone
 Concen: 6.280 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. -0.00 min
 Lab File: VU028537.D
 Acq: 07 Dec 2018 17:23

Instrument :
 MSVOA_U
 ClientSampleId :
 F9F39RE

Tgt Ion: 43 Resp: 6884
 Ion Ratio Lower Upper
 43 100
 58 29.6 0.0 62.0

