


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU120718\
 Data File : VU028520.D
 Acq On : 07 Dec 2018 09:06
 Operator : MD/SY
 Sample : BFB61
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 12 05:44:10 2018

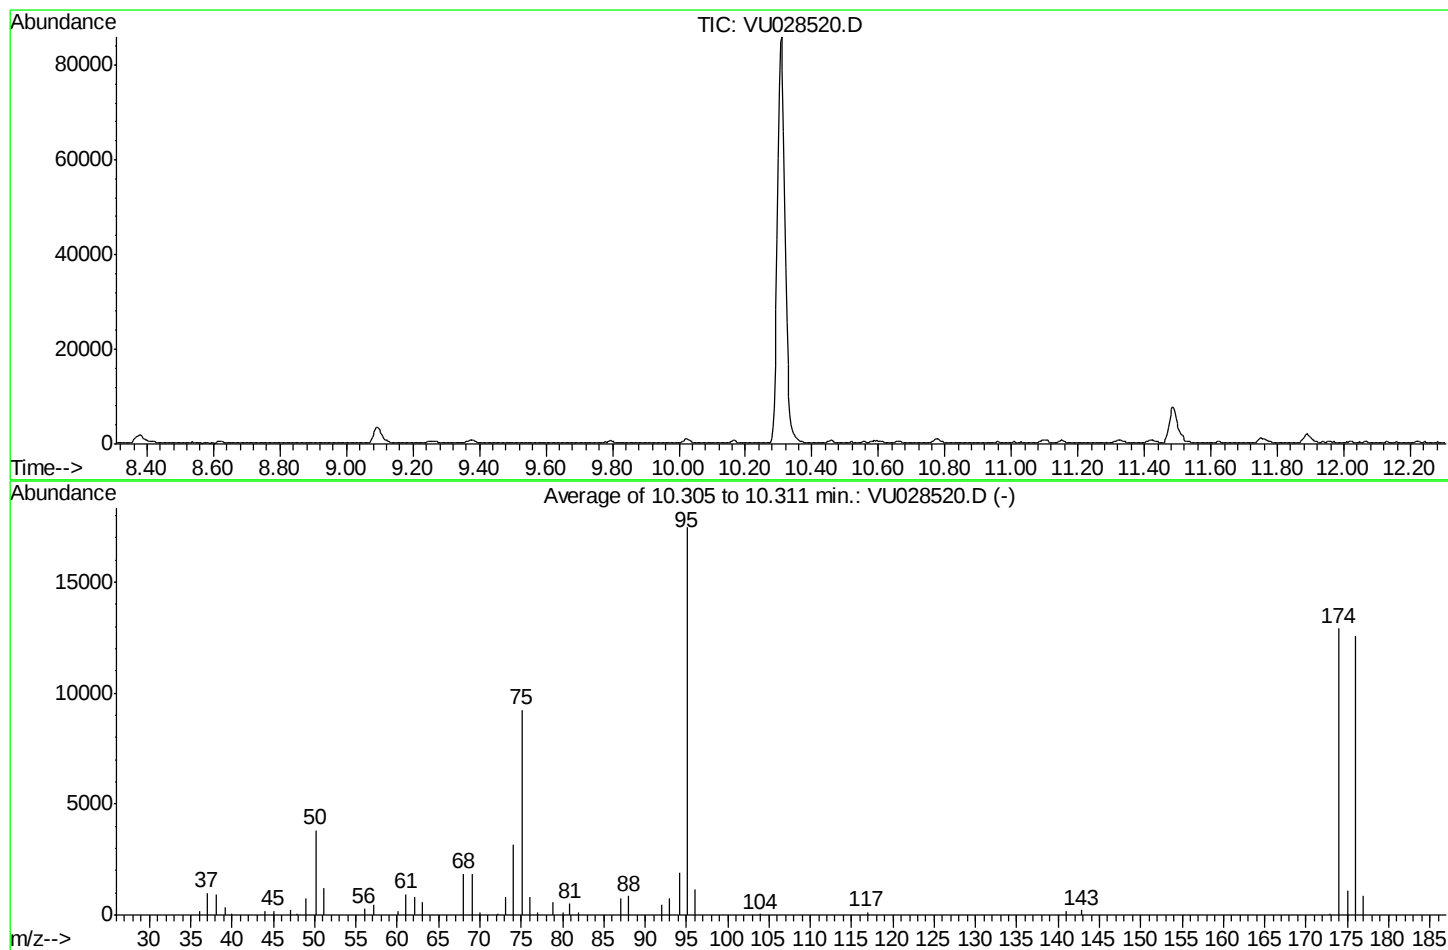

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	3817	PASS
75	95	30	80	52.9	9249	PASS
95	95	100	100	100.0	17469	PASS
96	95	5	9	6.7	1176	PASS
173	174	0.00	2	0.5	68	PASS
174	95	50	120	73.8	12899	PASS
175	174	5	9	8.5	1092	PASS
176	174	95	101	97.4	12563	PASS
177	176	5	9	6.8	852	PASS

m/z	Abundance
44.00	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

m/z	Abundance
36.00	214.0
37.00	1003.0
38.10	983.0
39.10	380.0
40.00	104.0
44.00	351.0
45.00	181.0
47.00	278.0
47.90	116.0
49.00	769.0
50.10	3987.0
51.10	1307.0
56.00	306.0
57.10	520.0
60.10	180.0
61.00	981.0
62.00	841.0
63.10	579.0
68.10	1899.0
69.10	1804.0
70.00	127.0
73.00	907.0
74.10	3278.0
75.10	9567.0
76.10	806.0
76.90	108.0
78.90	621.0
80.90	558.0
81.90	122.0
87.00	723.0
88.00	776.0
92.00	471.0
93.00	723.0
94.10	1915.0
95.10	17880.0
96.10	1240.0
104.00	100.0
116.90	139.0
140.90	178.0
142.90	201.0
172.90	205.0
174.00	13136.0
175.00	1086.0
176.00	12424.0
177.00	818.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

m/z	Abundance
36.00	195.0
37.00	1036.0
38.10	993.0
39.10	369.0
44.00	337.0
45.00	173.0
47.00	268.0
47.90	102.0
49.00	754.0
50.10	3966.0
51.10	1281.0
56.00	263.0
57.10	482.0
60.00	162.0
61.00	991.0
62.10	813.0
63.10	568.0
68.00	1924.0
69.10	1908.0
70.00	139.0
72.10	101.0
73.10	864.0
74.10	3305.0
75.10	9593.0
76.10	835.0
76.90	116.0
78.90	622.0
80.00	125.0
80.90	535.0
81.90	121.0
87.00	805.0
88.00	879.0
92.00	455.0
93.00	783.0
94.10	2000.0
95.10	17984.0
96.10	1212.0
116.90	126.0
140.90	185.0
142.90	247.0
174.00	13292.0
175.00	1150.0
176.00	12960.0
177.00	883.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

m/z	Abundance
36.00	187.0
37.00	904.0
38.10	873.0
39.10	339.0
44.00	336.0
45.00	189.0
47.00	238.0
49.00	730.0
50.10	3499.0
51.10	1105.0
56.00	222.0
57.10	419.0
60.00	118.0
61.10	888.0
62.10	731.0
63.00	514.0
68.00	1789.0
69.10	1852.0
70.00	153.0
73.10	736.0
74.10	3028.0
75.10	8589.0
76.10	781.0
76.90	107.0
78.90	524.0
80.00	160.0
80.90	455.0
82.00	110.0
87.00	774.0
88.00	895.0
92.00	416.0
93.00	686.0
94.10	1867.0
95.10	16544.0
96.00	1078.0
116.90	118.0
140.90	151.0
142.90	232.0
174.00	12271.0
175.00	1041.0
176.00	12305.0
177.00	855.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61