


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120720\
 Data File : VU041480.D
 Acq On : 07 Dec 2020 09:06
 Operator : SY/MD
 Sample : BFB20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Dec 08 17:21:56 2020

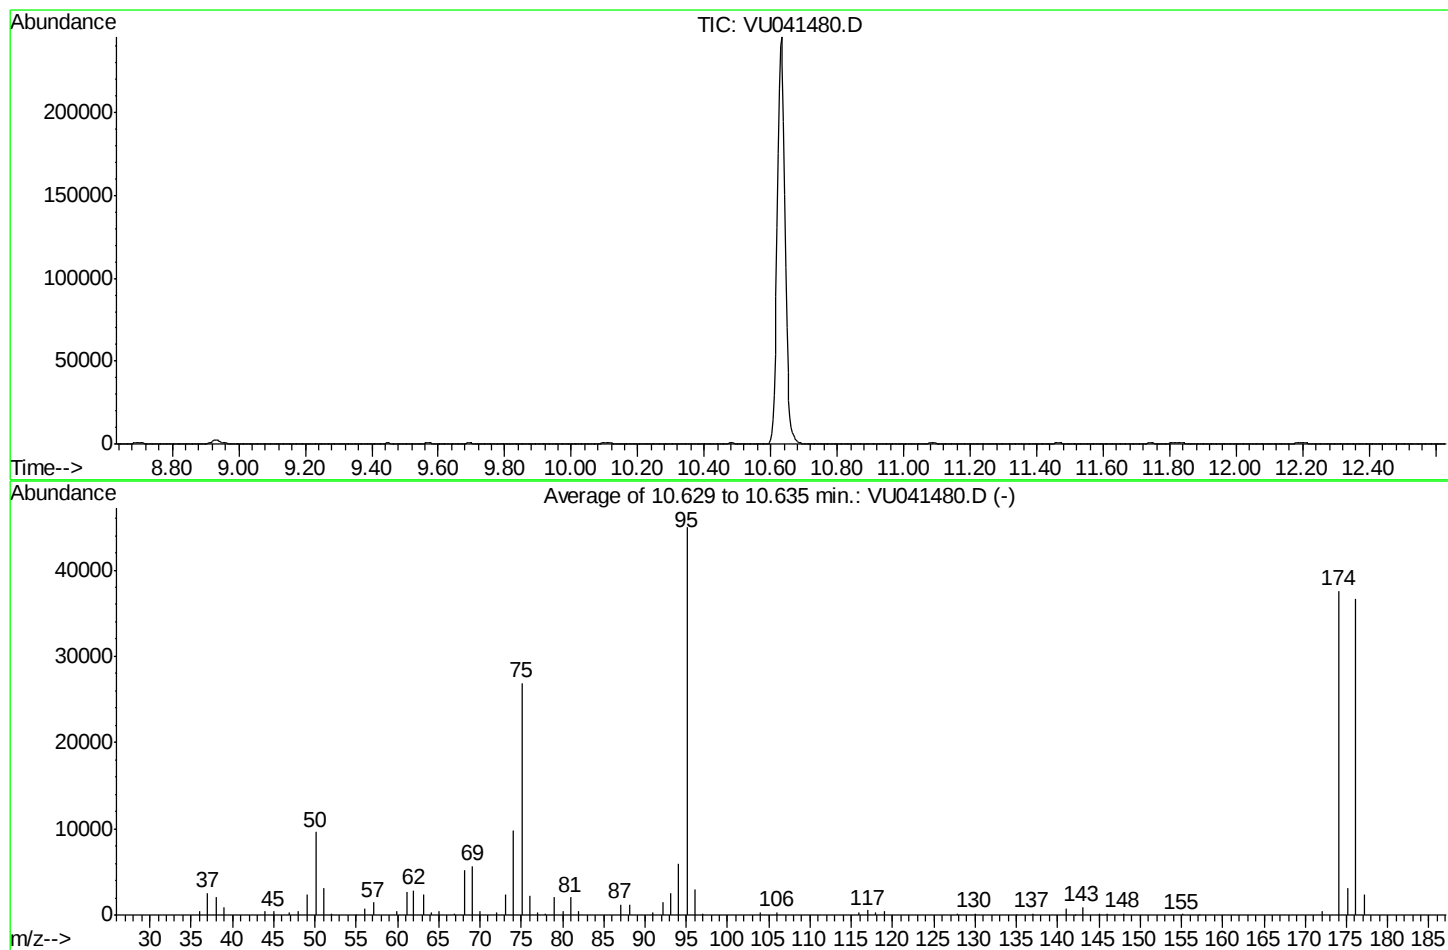

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	9592	PASS
75	95	30	80	59.9	26912	PASS
95	95	100	100	100.0	44952	PASS
96	95	5	9	6.7	2994	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	37594	PASS
175	174	5	9	8.2	3094	PASS
176	174	95	101	97.3	36594	PASS
177	176	5	9	6.5	2392	PASS

m/z	Abundance
35.90	480.0
37.00	2608.0
38.00	2261.0
39.00	950.0
44.00	378.0
45.00	449.0
46.90	280.0
48.00	502.0
49.00	2543.0
50.10	9943.0
51.10	2997.0
52.00	171.0
56.00	755.0
57.10	1588.0
59.90	501.0
61.10	2844.0
62.00	2851.0
63.10	2430.0
64.10	323.0
65.10	497.0
66.90	131.0
68.10	5290.0
69.10	5801.0
70.00	515.0
72.00	281.0
73.10	2316.0
74.10	9863.0
75.10	27376.0
76.10	2302.0
76.90	268.0
77.90	161.0
79.00	2049.0
80.00	470.0
81.00	2078.0
82.00	433.0
87.00	1357.0
88.10	1117.0
90.90	259.0
92.10	1516.0
93.10	2493.0
94.10	6144.0
95.10	45344.0
96.10	2986.0
97.00	132.0
103.90	225.0
106.10	373.0
115.90	247.0
117.00	556.0
117.90	222.0
118.90	402.0
127.90	167.0
129.90	196.0
134.90	123.0
137.00	150.0
141.00	765.0
142.10	132.0
143.00	1003.0
145.00	203.0
146.00	144.0
148.00	124.0
155.10	120.0
172.10	425.0
174.10	37120.0
175.10	3152.0
176.10	36288.0
177.10	2354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	491.0
37.00	2633.0
38.00	2191.0
39.00	885.0
44.00	409.0
45.00	435.0
46.80	302.0
48.00	506.0
49.00	2555.0
50.10	9839.0
51.10	3251.0
52.00	136.0
56.00	722.0
57.10	1551.0
59.90	455.0
61.10	2817.0
62.00	2900.0
63.10	2423.0
64.10	302.0
65.10	491.0
66.80	134.0
68.10	5291.0
69.10	5917.0
70.00	471.0
72.00	256.0
73.10	2480.0
74.10	10148.0
75.10	27568.0
76.10	2338.0
76.90	292.0
78.00	143.0
79.00	2081.0
80.00	473.0
81.00	2069.0
82.00	430.0
87.10	1297.0
88.10	1191.0
90.90	284.0
92.10	1561.0
93.10	2573.0
94.10	6179.0
95.10	46256.0
96.10	3095.0
97.00	131.0
103.90	250.0
106.10	356.0
115.90	246.0
117.00	576.0
117.90	254.0
118.90	420.0
127.90	149.0
129.90	163.0
135.00	103.0
137.00	169.0
141.00	728.0
143.00	968.0
145.10	212.0
146.00	109.0
148.00	168.0
155.10	113.0
157.10	108.0
172.10	432.0
174.10	38824.0
175.10	3189.0
176.10	37744.0
177.10	2464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	532.0
37.00	2422.0
38.00	2002.0
39.00	784.0
44.00	385.0
45.00	406.0
46.90	310.0
48.00	399.0
49.00	2231.0
50.10	8994.0
51.10	3149.0
55.00	106.0
56.00	692.0
57.10	1300.0
60.00	389.0
61.10	2582.0
62.00	2735.0
63.10	2216.0
64.10	275.0
65.10	386.0
66.80	110.0
68.10	4880.0
69.10	5420.0
70.10	357.0
72.10	225.0
73.10	2457.0
74.10	9322.0
75.10	25792.0
76.10	2211.0
76.90	268.0
78.00	111.0
79.00	1942.0
80.00	453.0
81.00	1920.0
81.90	409.0
87.00	1128.0
88.10	1093.0
90.90	258.0
92.10	1451.0
93.10	2436.0
94.10	5587.0
95.10	43256.0
96.10	2902.0
103.90	243.0
106.00	280.0
115.90	210.0
117.00	484.0
117.90	247.0
119.00	347.0
127.90	148.0
130.00	156.0
137.00	170.0
141.00	647.0
143.00	860.0
145.10	239.0
148.00	203.0
155.10	126.0
157.10	110.0
172.10	404.0
174.10	36840.0
175.10	2942.0
176.10	35752.0
177.10	2358.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB20