
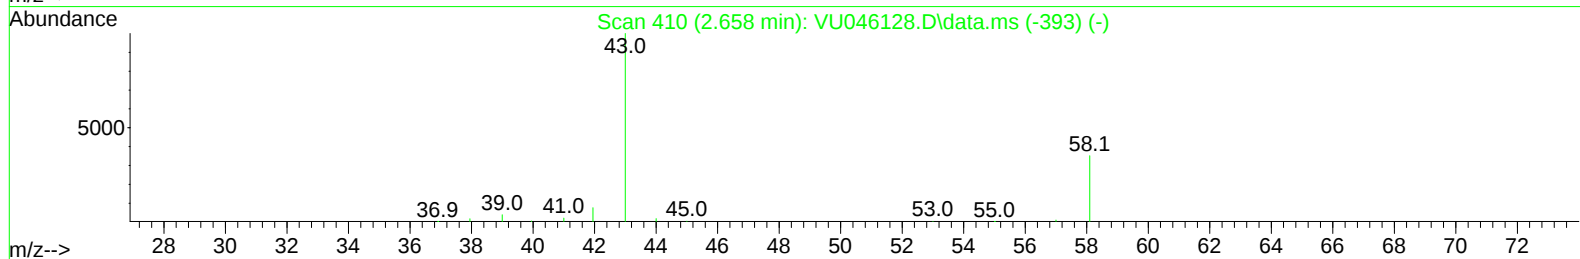
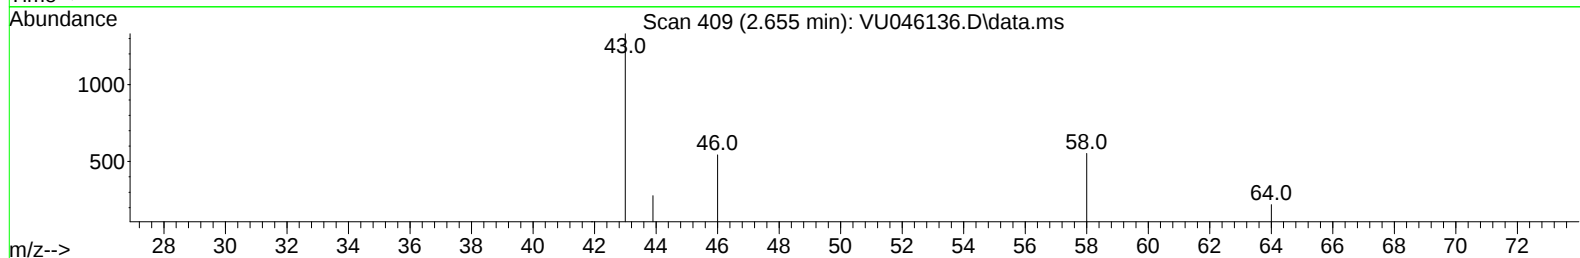


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046136.D
Acq On : 07 Dec 2021 13:33
Operator : SY/MD
Sample : M4960-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 08 04:52:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

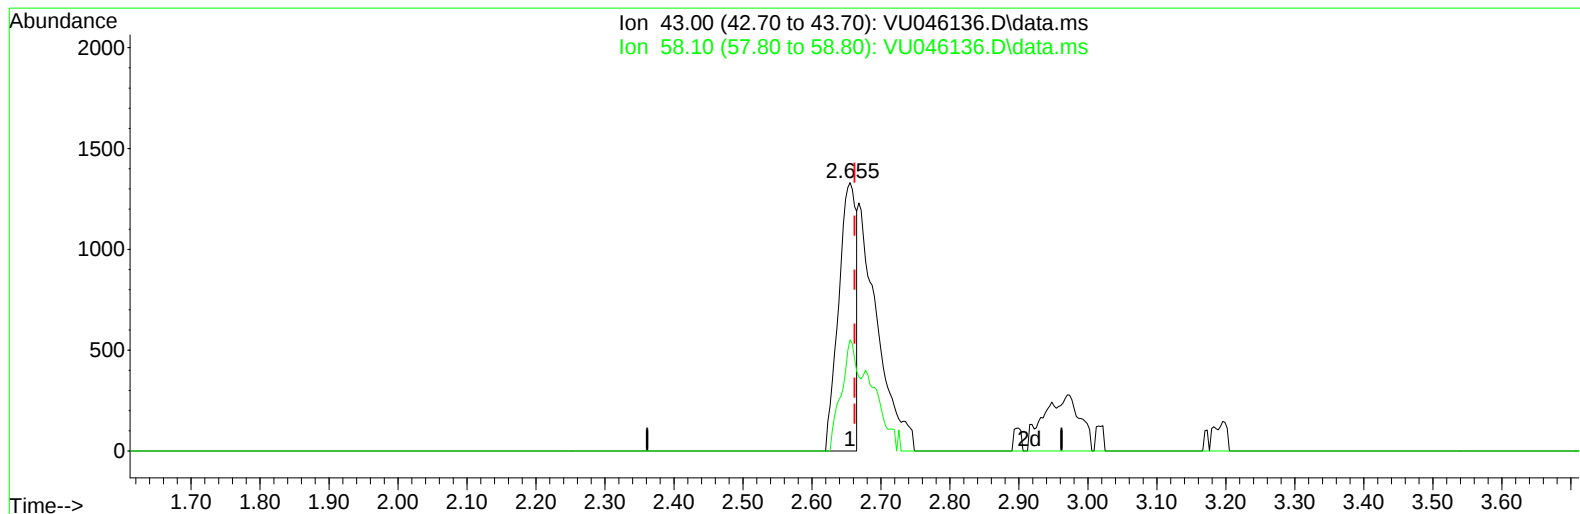

TIC: VU046136.D\data.ms

(13) Acetone (T)




2.655min (-0.006) 1.50 ug/L

response 2349

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.40	40.32
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046136.D
Acq On : 07 Dec 2021 13:33
Operator : SY/MD
Sample : M4960-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 08 04:52:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

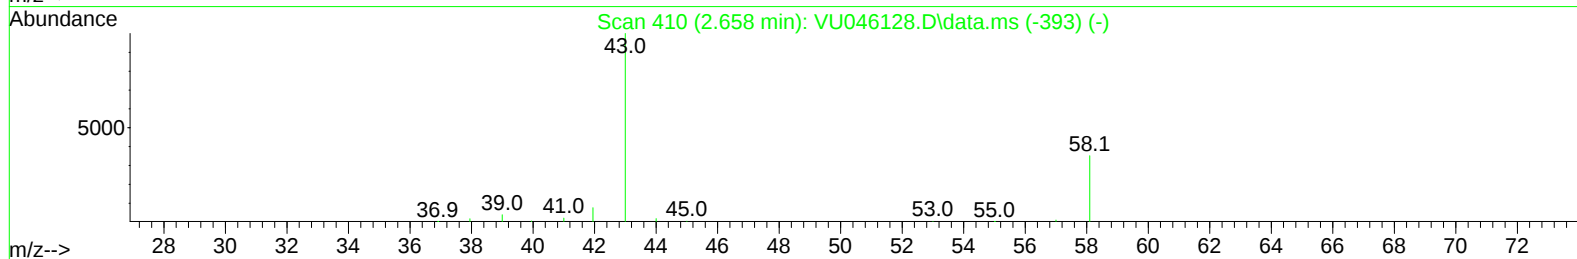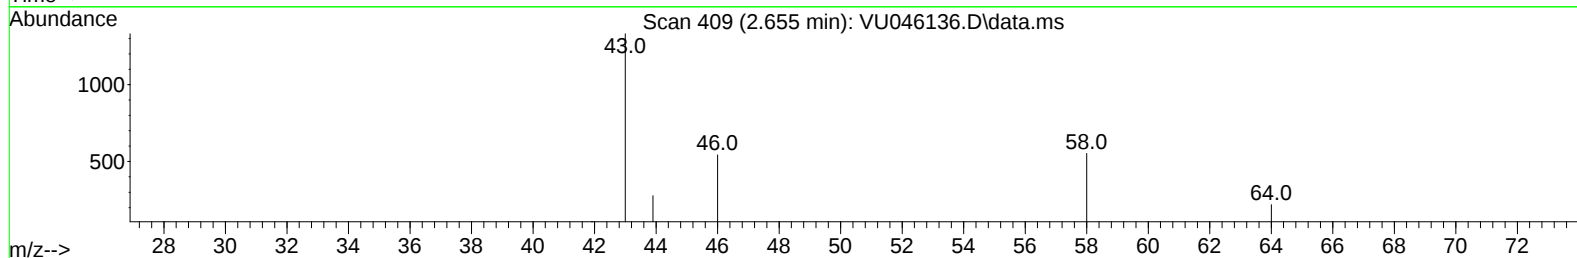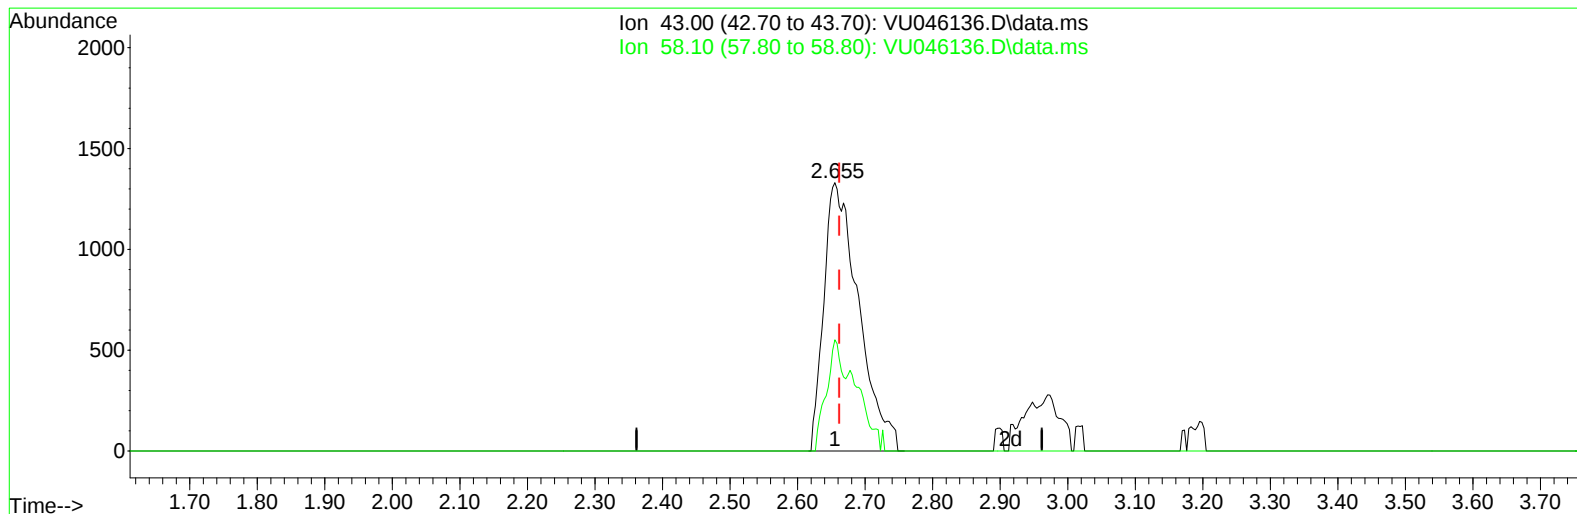

TIC: VU046136.D\data.ms

(13) Acetone (T)

2.655min (-0.006) 3.03 ug/L m

response 4751

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	33.40	19.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046136.D
 Acq On : 07 Dec 2021 13:33
 Operator : SY/MD
 Sample : M4960-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 08 04:52:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	191315	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	188784	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	99774	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	93915	59.592	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	119.180%
7) Chloroethane-d5	1.919	69	68311	56.455	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.920%
11) 1,1-Dichloroethene-d2	2.572	63	130108	45.989	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.980%
21) 2-Butanone-d5	4.639	46	145667	116.272	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.270%
24) Chloroform-d	5.067	84	155135	58.947	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.900%
26) 1,2-Dichloroethane-d4	5.707	65	105350	59.648	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.300%
32) Benzene-d6	5.729	84	347138	64.156	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	128.320%#
36) 1,2-Dichloropropane-d6	6.694	67	103393	61.656	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	123.320%#
41) Toluene-d8	7.899	98	320574	65.070	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	130.140%#
43) trans-1,3-Dichloroprop...	8.179	79	50764	62.710	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	125.420%#
47) 2-Hexanone-d5	8.632	63	104806	131.816	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	131.820%#
56) 1,1,2,2-Tetrachloroeth...	10.758	84	152904	60.124	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	120.240%#
66) 1,2-Dichlorobenzene-d4	12.192	152	127987	66.609	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	133.220%#
Target Compounds						
13) Acetone	2.655	43	4751m	3.034	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046136.D
Acq On : 07 Dec 2021 13:33
Operator : SY/MD
Sample : M4960-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 08 04:52:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

