

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046137.D
 Acq On : 07 Dec 2021 13:55
 Operator : SY/MD
 Sample : M4960-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 08 04:53:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	209867	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	206455	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	108841	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	91477	52.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.820%
7) Chloroethane-d5	1.919	69	66738	50.279	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.560%
11) 1,1-Dichloroethene-d2	2.572	63	126841	40.871	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.740%
21) 2-Butanone-d5	4.636	46	138424	100.724	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.720%
24) Chloroform-d	5.067	84	150957	52.289	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.580%
26) 1,2-Dichloroethane-d4	5.707	65	103080	53.203	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.400%
32) Benzene-d6	5.729	84	340270	57.504	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.000%
36) 1,2-Dichloropropane-d6	6.694	67	101594	55.398	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.800%
41) Toluene-d8	7.899	98	313501	58.188	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.380%
43) trans-1,3-Dichloroprop...	8.179	79	49110	55.474	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	110.940%
47) 2-Hexanone-d5	8.632	63	99731	114.697	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	114.700%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	146991	52.852	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.700%
66) 1,2-Dichlorobenzene-d4	12.195	152	123424	58.883	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	117.760%
Target Compounds						
13) Acetone	2.652	43	4981	2.900	ug/L	Qvalue 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046137.D
Acq On : 07 Dec 2021 13:55
Operator : SY/MD
Sample : M4960-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 08 04:53:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

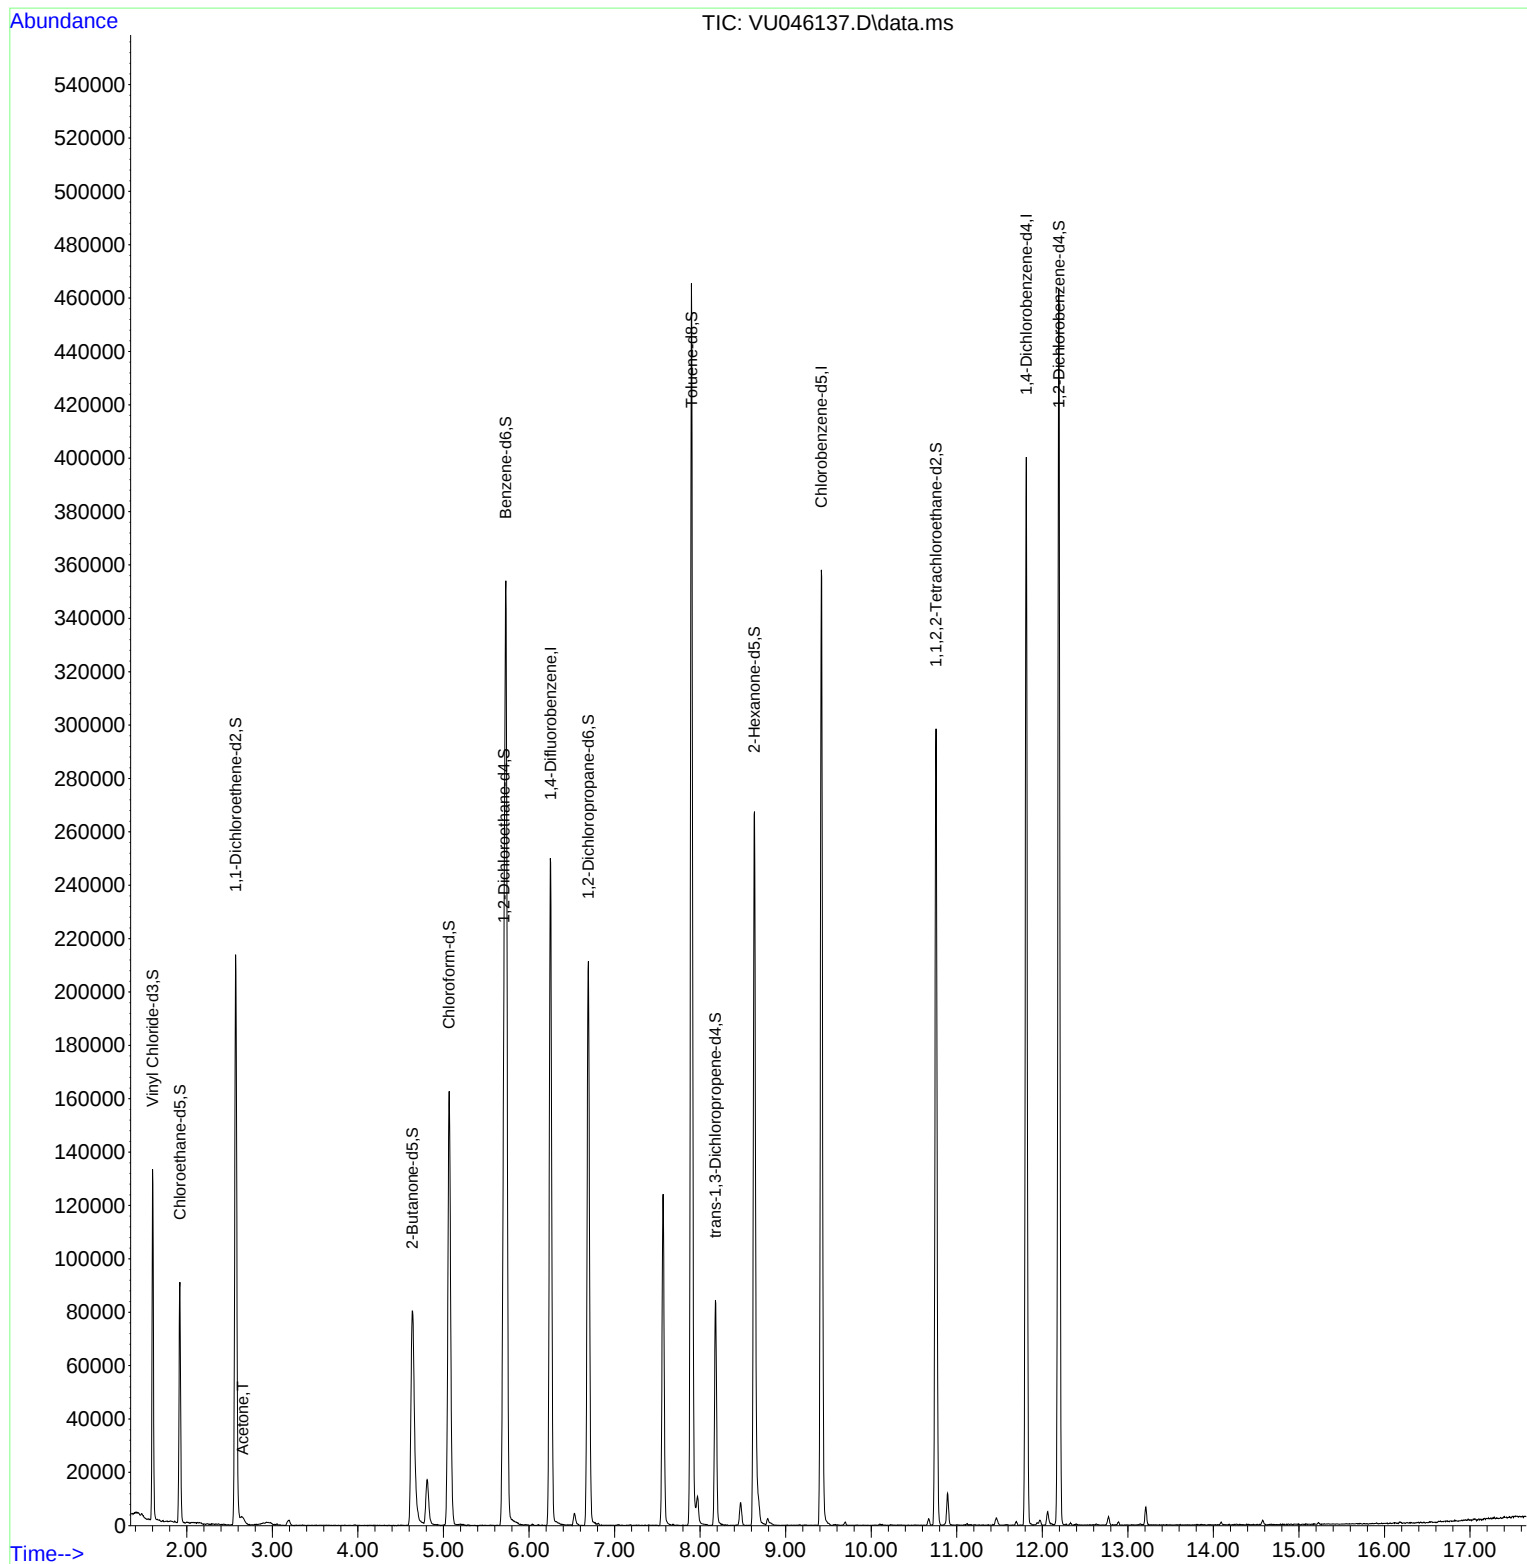

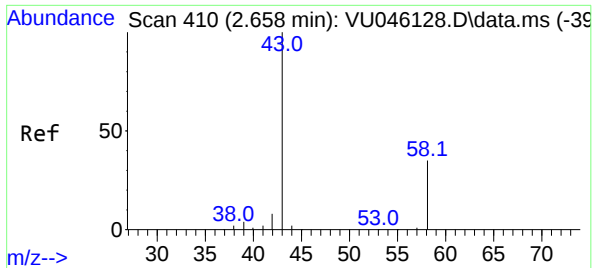

#13
 Acetone
 Concen: 2.900 ug/L
 RT: 2.652 min Scan# 408
 Delta R.T. -0.010 min
 Lab File: VU046137.D
 Acq: 07 Dec 2021 13:55

Tgt Ion: 43 Resp: 4981

Ion	Ratio	Lower	Upper
43	100		
58	16.1	0.0	66.8

