

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046137.D
 Acq On : 07 Dec 2021 13:55
 Operator : SY/MD
 Sample : M4960-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKR7

Quant Time: Dec 08 04:53:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	209867	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	206455	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	108841	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	91477	52.914	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 105.820%			
7) Chloroethane-d5	1.919	69	66738	50.279	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 100.560%			
11) 1,1-Dichloroethene-d2	2.572	63	126841	40.871	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 81.740%			
21) 2-Butanone-d5	4.636	46	138424	100.724	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 100.720%			
24) Chloroform-d	5.067	84	150957	52.289	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.580%			
26) 1,2-Dichloroethane-d4	5.707	65	103080	53.203	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.400%			
32) Benzene-d6	5.729	84	340270	57.504	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 115.000%			
36) 1,2-Dichloropropane-d6	6.694	67	101594	55.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 110.800%			
41) Toluene-d8	7.899	98	313501	58.188	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 116.380%			
43) trans-1,3-Dichloroprop...	8.179	79	49110	55.474	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 110.940%			
47) 2-Hexanone-d5	8.632	63	99731	114.697	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 114.700%			
56) 1,1,2,2-Tetrachloroeth...	10.758	84	146991	52.852	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 105.700%			
66) 1,2-Dichlorobenzene-d4	12.195	152	123424	58.883	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 117.760%			
Target Compounds					Qvalue	
13) Acetone	2.652	43	4981	2.900	ug/L	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046137.D
Acq On : 07 Dec 2021 13:55
Operator : SY/MD
Sample : M4960-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKR7

Quant Time: Dec 08 04:53:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

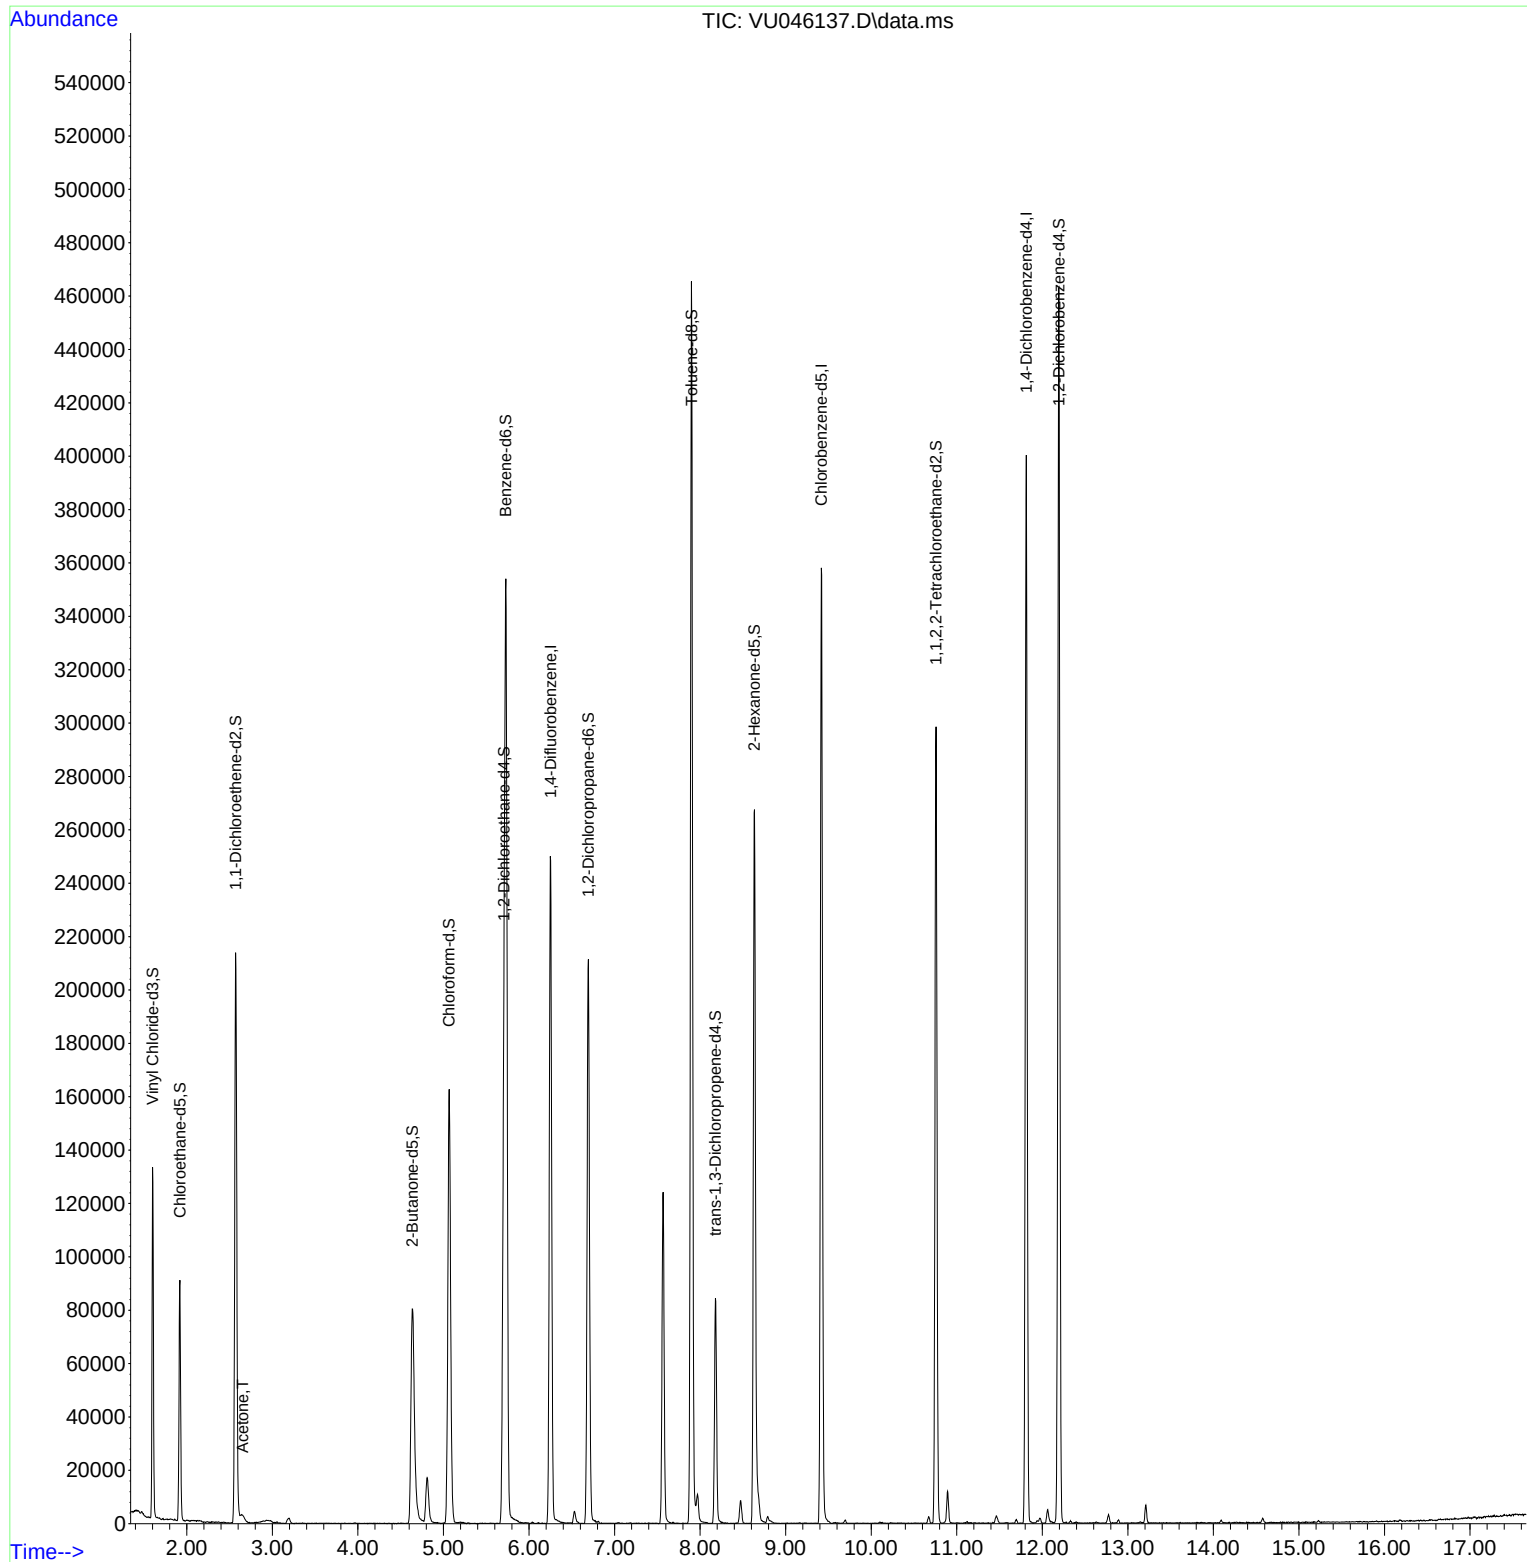

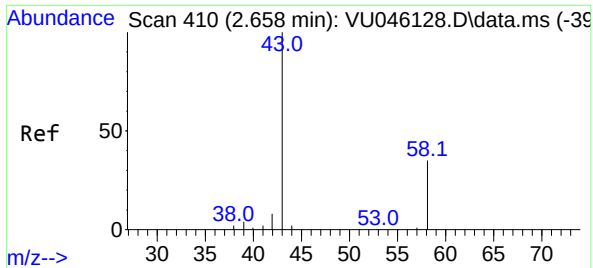

#13
 Acetone
 Concen: 2.900 ug/L
 RT: 2.652 min Scan# 40
 Delta R.T. -0.010 min
 Lab File: VU046137.D
 Acq: 07 Dec 2021 13:55

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKR7

Tgt Ion: 43 Resp: 4981
 Ion Ratio Lower Upper
 43 100
 58 16.1 0.0 66.8

