

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046134.D
 Acq On : 07 Dec 2021 12:49
 Operator : SY/MD
 Sample : M4938-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	95	rBV	88825	96496	13.12%	1.693%
2	1.919	171	180	194	rVB	66137	83646	11.37%	1.467%
3	2.575	371	384	414	rBV	153467	255246	34.69%	4.478%
4	2.797	448	453	461	rBV2	324	442	0.06%	0.008%
5	3.051	524	532	542	rVB3	1743	2781	0.38%	0.049%
6	3.131	554	557	565	rVB	97	123	0.02%	0.002%
7	3.189	565	575	587	rBV2	1672	3392	0.46%	0.060%
8	3.353	620	626	627	rBV	184	194	0.03%	0.003%
9	3.723	738	741	743	rBV	162	136	0.02%	0.002%
10	4.035	836	838	841	rVB	175	116	0.02%	0.002%
11	4.057	842	845	848	rBB	135	114	0.02%	0.002%
12	4.083	848	853	859	rBV	184	309	0.04%	0.005%
13	4.128	864	867	871	rBB	145	152	0.02%	0.003%
14	4.154	872	875	878	rBV	187	185	0.03%	0.003%
15	4.237	896	901	906	rBV	165	271	0.04%	0.005%
16	4.375	942	944	947	rBV	186	143	0.02%	0.003%
17	4.465	970	972	974	rBV	179	126	0.02%	0.002%
18	4.539	992	995	999	rBB	126	135	0.02%	0.002%
19	4.639	1010	1026	1061	rBV	65296	197380	26.83%	3.463%
20	4.851	1090	1092	1096	rVB2	455	323	0.04%	0.006%
21	4.906	1106	1109	1115	rVB2	253	302	0.04%	0.005%
22	4.935	1115	1118	1122	rBV	228	269	0.04%	0.005%
23	5.070	1143	1160	1183	rBV	126847	290048	39.42%	5.088%
24	5.176	1191	1193	1197	rVB2	291	170	0.02%	0.003%
25	5.205	1197	1202	1205	rBV2	341	415	0.06%	0.007%
26	5.289	1225	1228	1233	rVB3	381	310	0.04%	0.005%
27	5.356	1246	1249	1255	rBB	157	179	0.02%	0.003%
28	5.388	1256	1259	1263	rBV	173	209	0.03%	0.004%
29	5.478	1285	1287	1289	rBV	151	108	0.01%	0.002%
30	5.539	1302	1306	1308	rBV	149	158	0.02%	0.003%
31	5.729	1343	1365	1383	rBV2	273185	735714	100.00%	12.907%
32	5.896	1415	1417	1420	rVB2	323	143	0.02%	0.003%
33	5.990	1443	1446	1449	rBV2	313	258	0.04%	0.005%
34	6.044	1460	1463	1465	rBV	136	100	0.01%	0.002%
35	6.060	1466	1468	1471	rVB	403	186	0.03%	0.003%
36	6.089	1472	1477	1481	rBV	222	269	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046134.D
 Acq On : 07 Dec 2021 12:49
 Operator : SY/MD
 Sample : M4938-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.118	1483	1486	1490	rVB	246	198	0.03%	0.003%
38	6.141	1490	1493	1496	rBB	171	140	0.02%	0.002%
39	6.253	1512	1528	1546	rBV	216983	409024	55.60%	7.176%
40	6.533	1603	1615	1626	rBV3	3163	6402	0.87%	0.112%
41	6.588	1630	1632	1636	rBV	137	143	0.02%	0.003%
42	6.694	1651	1665	1683	rBV	168747	326986	44.44%	5.736%
43	6.809	1698	1701	1703	rBV	261	195	0.03%	0.003%
44	6.993	1752	1758	1760	rBV	177	219	0.03%	0.004%
45	7.044	1768	1774	1782	rBV3	397	626	0.09%	0.011%
46	7.192	1816	1820	1822	rBV	190	131	0.02%	0.002%
47	7.379	1874	1878	1881	rBV	189	213	0.03%	0.004%
48	7.417	1886	1890	1893	rBV	223	220	0.03%	0.004%
49	7.475	1905	1908	1910	rBV	187	155	0.02%	0.003%
50	7.568	1924	1937	1951	rBV	91638	158342	21.52%	2.778%
51	7.671	1966	1969	1971	rBV2	199	119	0.02%	0.002%
52	7.690	1971	1975	1979	rVB2	190	212	0.03%	0.004%
53	7.797	2005	2008	2011	rVV2	192	135	0.02%	0.002%
54	7.899	2026	2040	2056	rBV	343634	597807	81.26%	10.488%
55	8.179	2115	2127	2150	rBV	61103	102871	13.98%	1.805%
56	8.295	2161	2163	2166	rVB	217	102	0.01%	0.002%
57	8.314	2166	2169	2171	rVB2	236	155	0.02%	0.003%
58	8.337	2172	2176	2179	rBV	176	202	0.03%	0.004%
59	8.395	2191	2194	2197	rBV	148	149	0.02%	0.003%
60	8.636	2255	2269	2309	rBV	218226	395025	53.69%	6.930%
61	8.915	2348	2356	2364	rVB3	709	1028	0.14%	0.018%
62	9.012	2382	2386	2392	rVB	126	121	0.02%	0.002%
63	9.086	2404	2409	2415	rBV	91	127	0.02%	0.002%
64	9.163	2431	2433	2436	rVV	169	108	0.01%	0.002%
65	9.417	2499	2512	2545	rVB	305033	514372	69.91%	9.024%
66	9.562	2555	2557	2559	rBV	169	100	0.01%	0.002%
67	9.694	2592	2598	2600	rBV3	773	657	0.09%	0.012%
68	9.803	2630	2632	2635	rBV	194	107	0.01%	0.002%
69	10.108	2725	2727	2729	rVB	261	105	0.01%	0.002%
70	10.211	2756	2759	2761	rBV2	140	100	0.01%	0.002%
71	10.671	2896	2902	2909	rBV2	1180	1306	0.18%	0.023%
72	10.758	2917	2929	2947	rVB	246913	392955	53.41%	6.894%
73	10.832	2947	2952	2955	rBV	148	134	0.02%	0.002%
74	11.308	3097	3100	3102	rVV	135	99	0.01%	0.002%
75	11.340	3106	3110	3112	rBV	192	114	0.02%	0.002%
76	11.449	3140	3144	3146	rBV2	578	471	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046134.D
 Acq On : 07 Dec 2021 12:49
 Operator : SY/MD
 Sample : M4938-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.584	3185	3186	3190	rVB	286	158	0.02%	0.003%
78	11.700	3219	3222	3224	rVB	331	146	0.02%	0.003%
79	11.812	3245	3257	3279	rVB	345388	539370	73.31%	9.462%
80	11.931	3292	3294	3297	rBV2	162	113	0.02%	0.002%
81	11.947	3297	3299	3300	rVV2	270	120	0.02%	0.002%
82	11.970	3304	3306	3312	rVB	563	564	0.08%	0.010%
83	12.021	3318	3322	3327	rBV	199	215	0.03%	0.004%
84	12.073	3336	3338	3341	rBV	215	139	0.02%	0.002%
85	12.192	3363	3375	3394	rBV	355679	574336	78.07%	10.076%
86	12.263	3394	3397	3401	rVB	262	210	0.03%	0.004%
87	12.288	3401	3405	3407	rBV	155	128	0.02%	0.002%
88	12.899	3592	3595	3598	rBV2	198	169	0.02%	0.003%
89	13.054	3639	3643	3647	rBV	206	163	0.02%	0.003%
90	13.298	3716	3719	3721	rBV	183	105	0.01%	0.002%
91	13.844	3886	3889	3891	rBV	201	113	0.02%	0.002%
92	13.906	3904	3908	3910	rBV	244	151	0.02%	0.003%
93	14.336	4039	4042	4044	rVB2	325	212	0.03%	0.004%
94	14.353	4044	4047	4050	rBV	119	106	0.01%	0.002%
95	14.504	4091	4094	4100	rVV2	257	228	0.03%	0.004%
96	14.777	4175	4179	4182	rBV2	265	275	0.04%	0.005%
97	15.053	4262	4265	4268	rBV2	307	202	0.03%	0.004%
98	15.160	4296	4298	4300	rBV2	245	109	0.01%	0.002%
99	15.343	4349	4355	4357	rBV	302	356	0.05%	0.006%
100	15.378	4363	4366	4368	rBV	266	202	0.03%	0.004%




Sum of corrected areas: 5700113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046134.D
Acq On : 07 Dec 2021 12:49
Operator : SY/MD
Sample : M4938-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

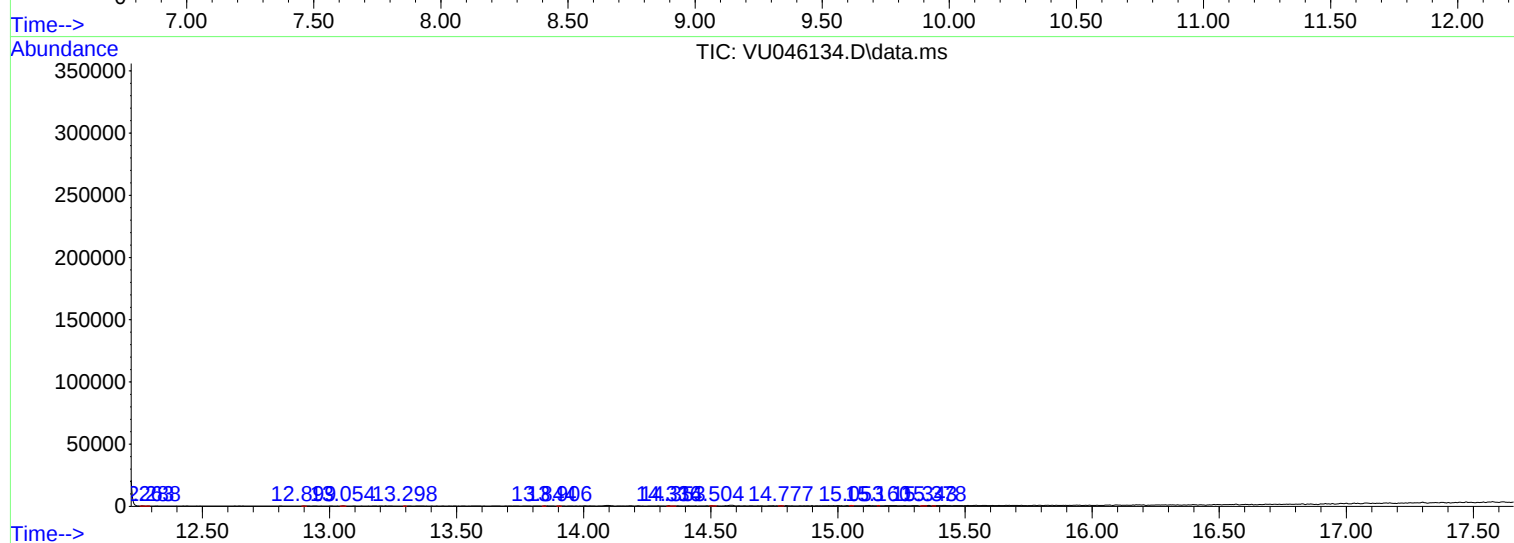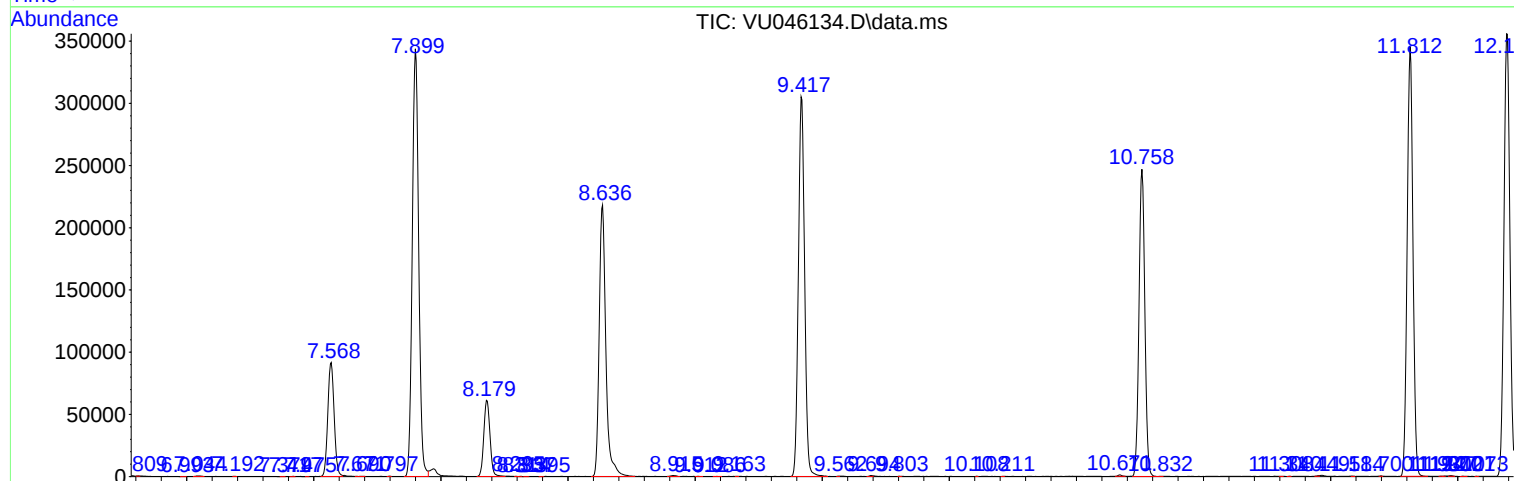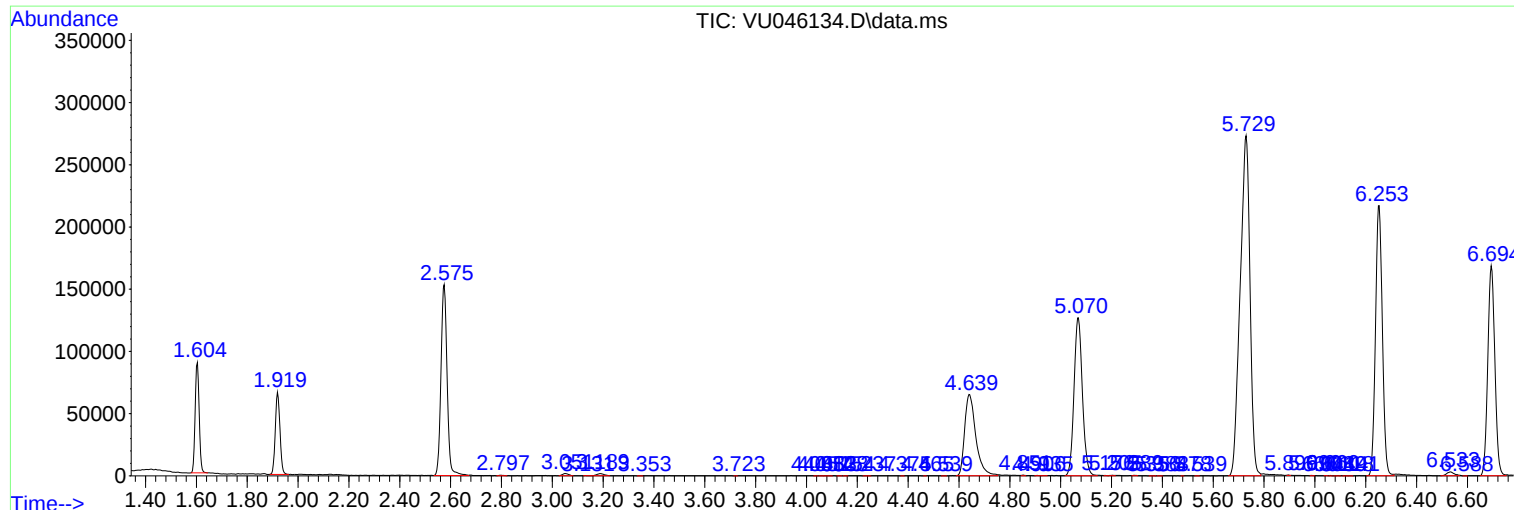

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046134.D
Acq On : 07 Dec 2021 12:49
Operator : SY/MD
Sample : M4938-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
Data File : VU046134.D
Acq On : 07 Dec 2021 12:49
Operator : SY/MD
Sample : M4938-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc