


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120721\
 Data File : VU046127.D
 Acq On : 07 Dec 2021 09:42
 Operator : SY/MD
 Sample : BFB025
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB025

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

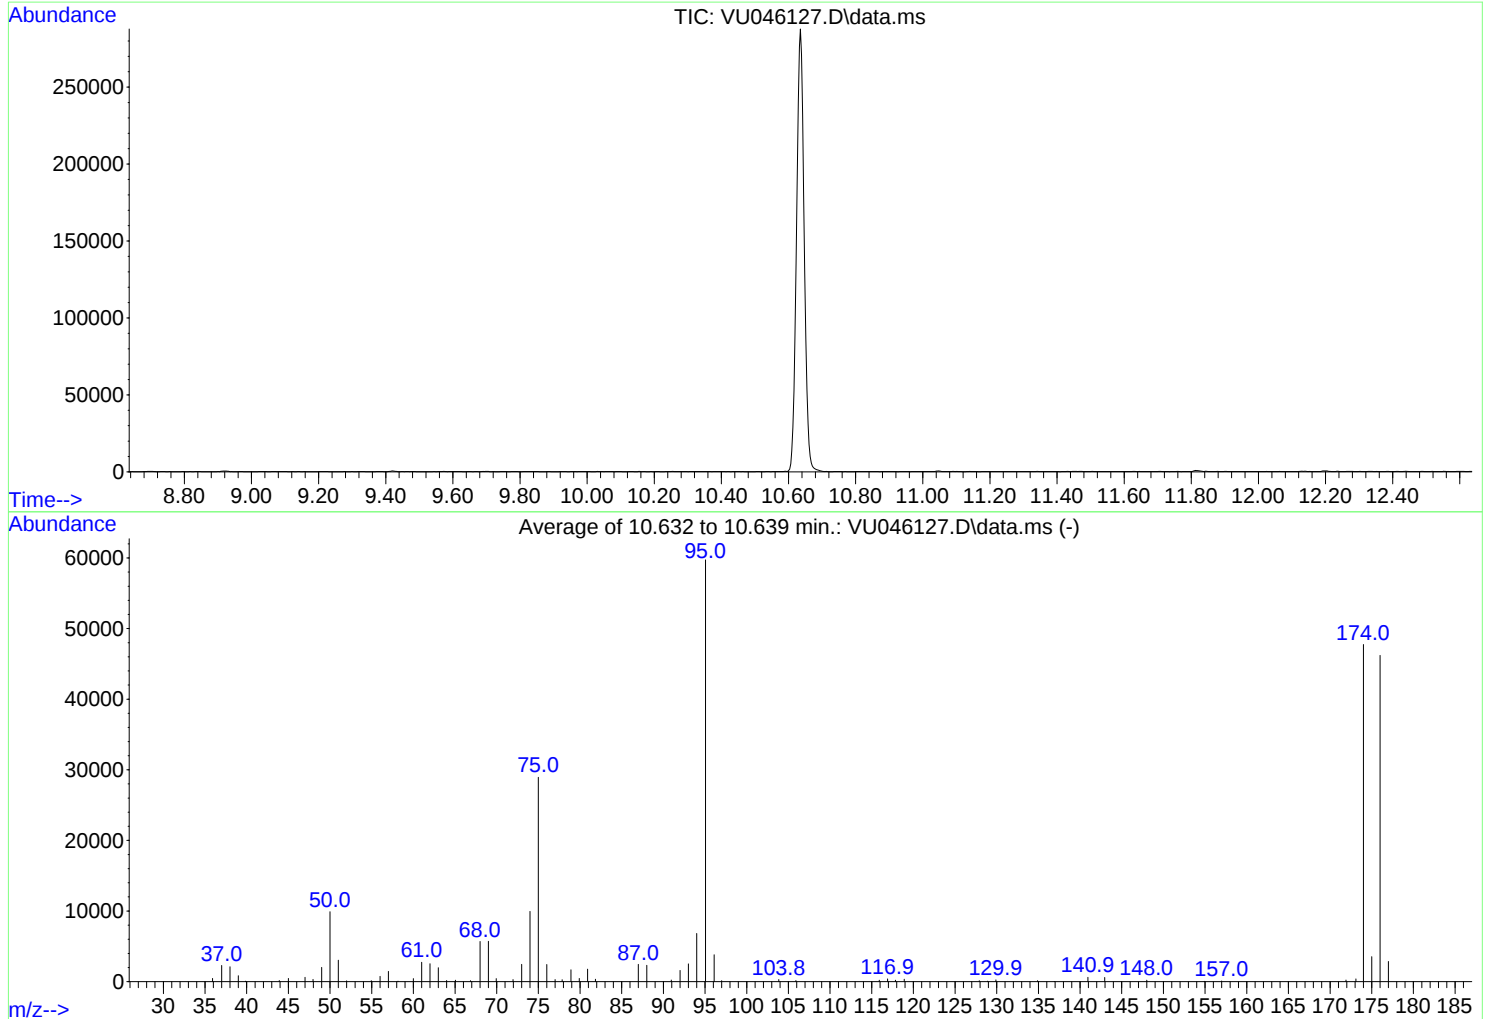

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9910	PASS
75	95	30	80	48.4	28939	PASS
95	95	100	100	100.0	59733	PASS
96	95	5	9	6.4	3813	PASS
173	174	0.00	2	0.8	383	PASS
174	95	50	120	79.9	47736	PASS
175	174	5	9	7.4	3528	PASS
176	174	95	101	96.8	46205	PASS
177	176	5	9	6.2	2846	PASS

m/z	Abundance
44.00	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	443.0
37.00	2287.0
38.00	2119.0
39.00	897.0
43.90	439.0
45.00	451.0
47.00	558.0
48.00	324.0
49.00	2051.0
50.00	9916.0
51.00	3056.0
52.10	121.0
55.00	123.0
56.00	754.0
57.00	1458.0
58.10	100.0
60.00	405.0
61.00	2723.0
62.00	2640.0
63.00	1927.0
64.00	190.0
65.10	191.0
66.80	150.0
68.00	5814.0
69.00	5802.0
69.90	454.0
72.00	286.0
73.00	2529.0
74.00	9789.0
75.00	29016.0
76.00	2529.0
77.00	278.0
77.80	331.0
78.90	1676.0
79.90	458.0
80.90	1807.0
81.80	397.0
87.00	2522.0
88.00	2349.0
90.90	196.0
92.00	1582.0
93.00	2510.0
94.00	6789.0
95.00	59664.0
96.10	3980.0
97.00	146.0
103.90	291.0
105.90	176.0
115.90	215.0
116.90	363.0
117.90	167.0
118.90	359.0
127.90	143.0
128.90	111.0
129.90	232.0
134.90	131.0
140.90	644.0
143.00	601.0
148.00	225.0
157.00	133.0
171.90	259.0
173.10	350.0
174.00	46248.0
175.00	3439.0
176.00	44904.0
177.00	2961.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	470.0
37.00	2378.0
38.00	2205.0
39.00	891.0
39.80	123.0
43.90	444.0
45.00	488.0
47.00	640.0
47.90	320.0
49.00	2044.0
50.00	10215.0
51.00	3115.0
52.00	102.0
54.90	132.0
56.00	777.0
57.00	1508.0
58.20	100.0
60.00	440.0
61.00	2847.0
62.00	2594.0
63.00	2018.0
64.00	173.0
65.00	196.0
66.80	142.0
68.00	5850.0
69.00	5833.0
70.00	436.0
71.90	318.0
73.00	2544.0
74.00	10304.0
75.00	29912.0
76.00	2486.0
77.00	304.0
77.80	299.0
78.90	1745.0
79.90	457.0
80.90	1808.0
81.90	354.0
87.00	2526.0
88.00	2379.0
90.90	227.0
92.00	1651.0
93.00	2581.0
94.00	7004.0
95.00	61824.0
96.10	3899.0
97.00	149.0
103.80	307.0
105.90	177.0
115.90	222.0
116.90	387.0
117.80	214.0
118.90	371.0
127.90	138.0
128.90	103.0
129.90	257.0
134.90	128.0
136.90	103.0
140.90	644.0
142.90	597.0
148.00	245.0
157.00	127.0
171.90	254.0
173.10	382.0
174.00	49480.0
175.00	3669.0
176.00	47768.0
177.00	2912.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	445.0
37.00	2214.0
38.00	2030.0
39.00	755.0
39.90	117.0
43.90	419.0
45.00	437.0
47.00	638.0
47.90	310.0
49.00	1942.0
50.00	9599.0
51.00	2947.0
51.90	106.0
54.90	159.0
56.00	715.0
57.00	1409.0
60.00	415.0
61.00	2683.0
62.00	2404.0
63.00	1959.0
64.00	143.0
65.00	198.0
66.90	132.0
68.00	5370.0
69.00	5471.0
70.00	402.0
71.90	316.0
73.00	2302.0
74.00	9733.0
75.00	27888.0
76.00	2293.0
77.00	293.0
77.90	219.0
78.90	1626.0
79.90	430.0
80.90	1681.0
81.90	298.0
87.00	2268.0
88.00	2236.0
91.00	241.0
92.00	1539.0
93.00	2452.0
94.00	6692.0
95.10	57712.0
96.10	3560.0
97.00	120.0
103.80	292.0
105.90	160.0
115.90	187.0
116.90	384.0
117.80	246.0
118.90	311.0
127.90	155.0
129.90	259.0
134.90	119.0
141.00	558.0
142.90	558.0
148.00	174.0
154.90	131.0
171.90	205.0
173.10	417.0
174.00	47480.0
175.00	3476.0
176.00	45944.0
177.00	2666.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025