

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052227.D
 Acq On : 08 Dec 2022 04:06
 Operator : JC/MD
 Sample : N5918-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EH5

Quant Time: Dec 08 04:35:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	213379	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	222298	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	92374	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	87696	4.225	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.600%
7) Chloroethane-d5	1.916	69	77030	4.778	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.568	65	35414	4.760	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.200%
20) 2-Butanone-d5	4.642	46	234466	62.322	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.640%
24) Chloroform-d	5.060	84	159348	5.225	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
26) 1,2-Dichloroethane-d4	5.700	65	82764	5.373	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.400%
32) Benzene-d6	5.726	84	314528	4.766	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.687	67	104263	5.105	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.896	98	232932	3.901	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.000%
43) trans-1,3-Dichloroprop...	8.176	79	30179	4.055	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.000%
46) 2-Hexanone-d5	8.636	63	161632	51.244	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.480%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	98119	5.541	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.800%
66) 1,2-Dichlorobenzene-d4	12.189	152	92039	5.204	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds					Qvalue	
13) Acetone	2.662	43	7037	2.754	ug/L	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052227.D
Acq On : 08 Dec 2022 04:06
Operator : JC/MD
Sample : N5918-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EH5

Quant Time: Dec 08 04:35:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

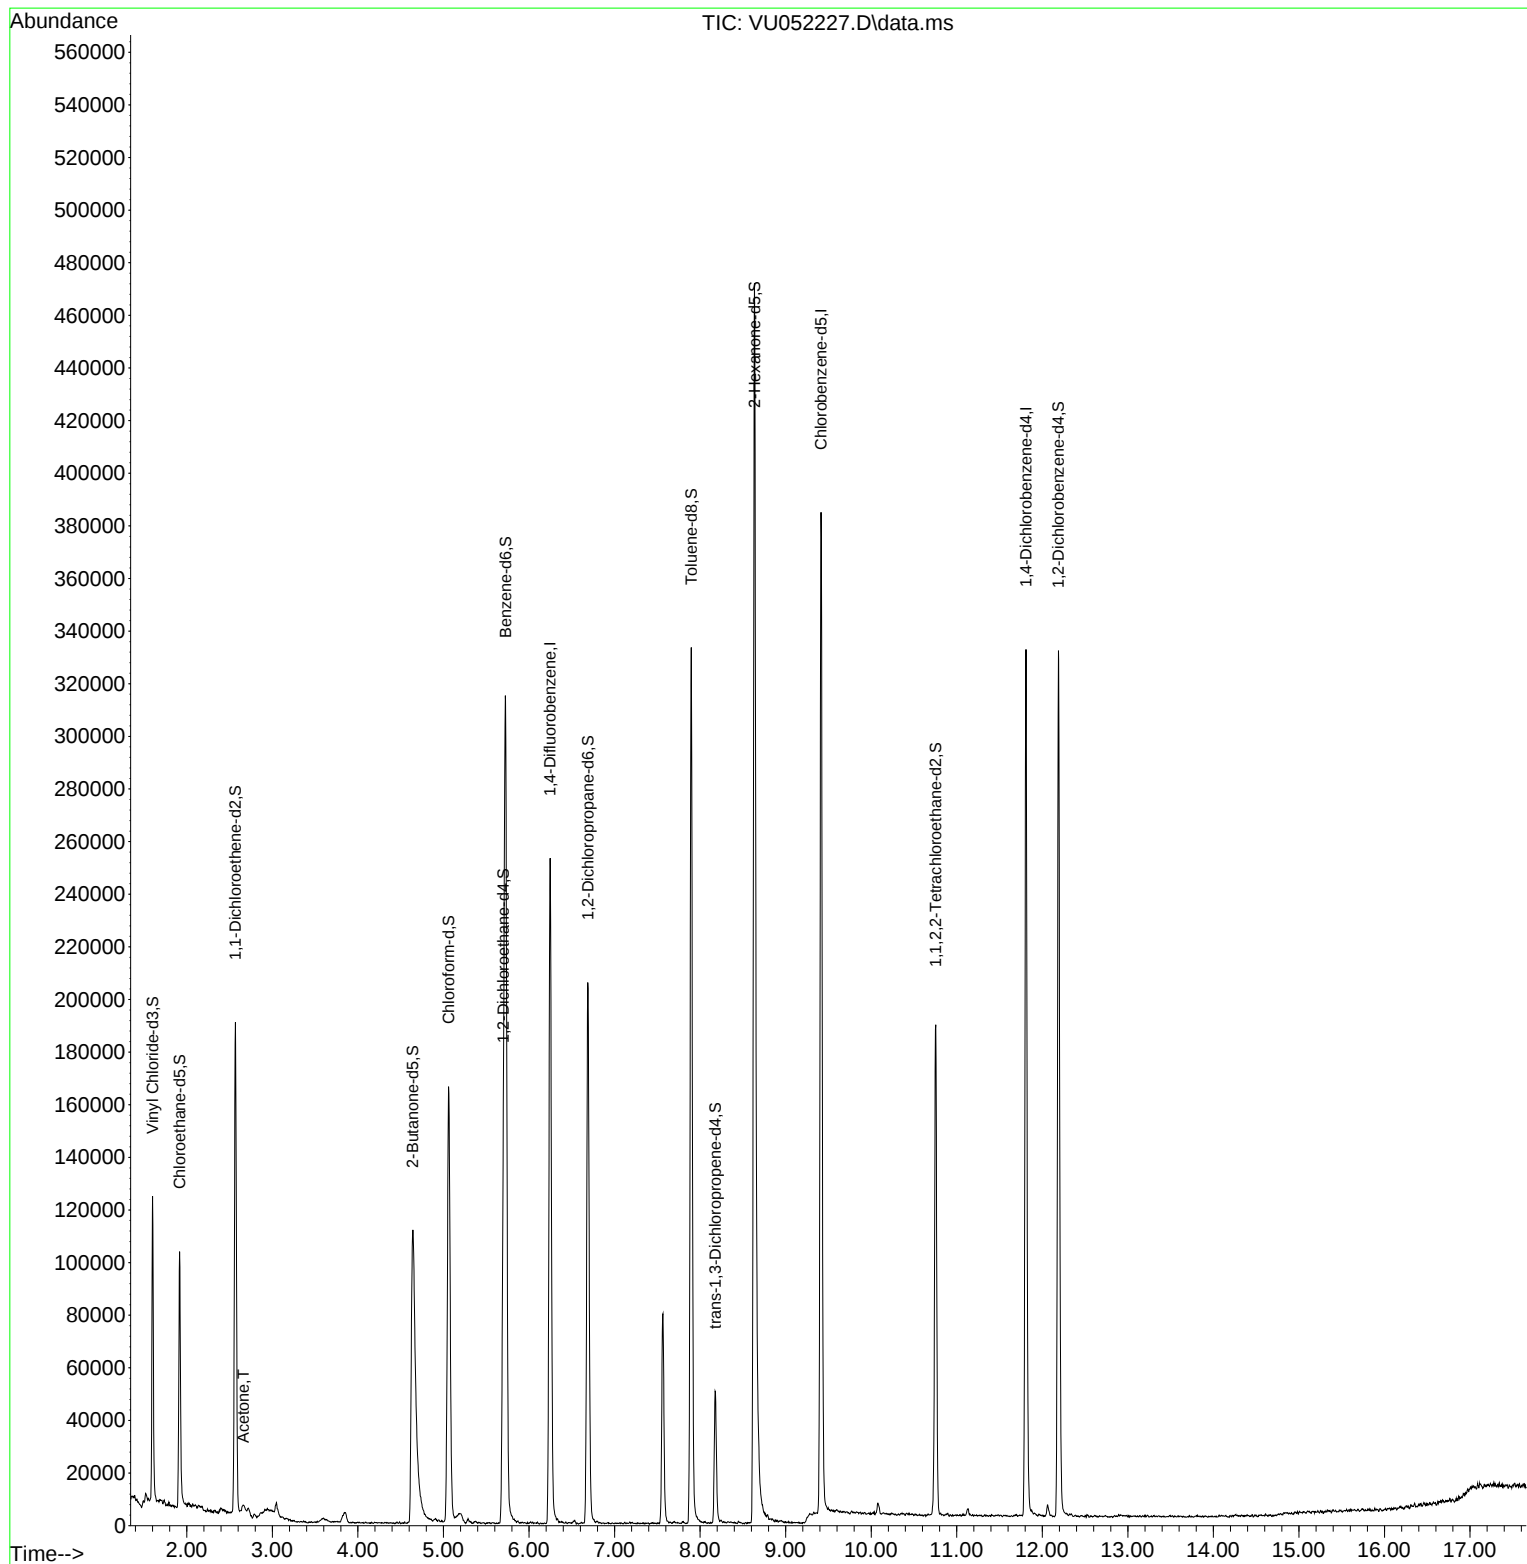

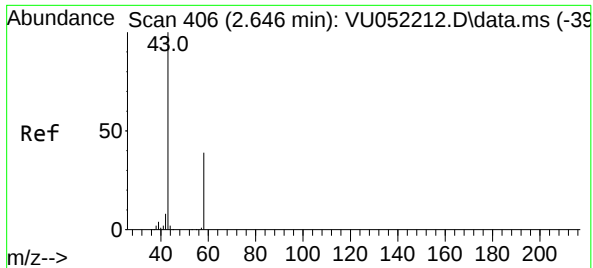

#13
 Acetone
 Concen: 2.754 ug/L
 RT: 2.662 min Scan# 411
 Delta R.T. 0.016 min
 Lab File: VU052227.D
 Acq: 08 Dec 2022 04:06

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EH5

Tgt Ion: 43 Resp: 7037
 Ion Ratio Lower Upper
 43 100
 58 14.9 0.0 76.0

