

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU120722\  
 Data File : VU052230.D  
 Acq On : 08 Dec 2022 05:20  
 Operator : JC/MD  
 Sample : N5918-12  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 42 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0EJ0

Quant Time: Dec 08 06:48:24 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Dec 08 04:19:43 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------|----------|
| -----                         |        |       |          |          |       |          |
| Internal Standards            |        |       |          |          |       |          |
| 1) 1,4-Difluorobenzene        | 6.247  | 114   | 208311   | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 9.414  | 117   | 219338   | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.809 | 152   | 90211    | 5.000    | ug/L  | 0.00     |
|                               |        |       |          |          |       |          |
| System Monitoring Compounds   |        |       |          |          |       |          |
| 4) Vinyl Chloride-d3          | 1.600  | 65    | 76114    | 3.756    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 75.200%  |
| 7) Chloroethane-d5            | 1.915  | 69    | 70764    | 4.496    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 90.000%  |
| 11) 1,1-Dichloroethene-d2     | 2.568  | 65    | 31028    | 4.272    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 85.400%  |
| 20) 2-Butanone-d5             | 4.639  | 46    | 218694   | 59.544   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 119.080% |
| 24) Chloroform-d              | 5.060  | 84    | 149311   | 5.015    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 100.400% |
| 26) 1,2-Dichloroethane-d4     | 5.700  | 65    | 78655    | 5.230    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 104.600% |
| 32) Benzene-d6                | 5.726  | 84    | 297062   | 4.562    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 91.200%  |
| 36) 1,2-Dichloropropane-d6    | 6.687  | 67    | 101675   | 5.045    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 101.000% |
| 41) Toluene-d8                | 7.896  | 98    | 220171   | 3.737    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 74.800%  |
| 43) trans-1,3-Dichloroprop... | 8.176  | 79    | 28918    | 3.938    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 78.800%  |
| 46) 2-Hexanone-d5             | 8.632  | 63    | 153364   | 49.279   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 98.560%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.751 | 84    | 93527    | 5.353    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 107.000% |
| 66) 1,2-Dichlorobenzene-d4    | 12.188 | 152   | 88714    | 5.136    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 102.800% |
|                               |        |       |          |          |       |          |
| Target Compounds              |        |       |          |          |       | Qvalue   |
| 13) Acetone                   | 2.665  | 43    | 6644     | 2.664    | ug/L  | 71       |
| -----                         |        |       |          |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU120722\  
Data File : VU052230.D  
Acq On : 08 Dec 2022 05:20  
Operator : JC/MD  
Sample : N5918-12  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 42 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
C0EJ0

Quant Time: Dec 08 06:48:24 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Dec 08 04:19:43 2022  
Response via : Initial Calibration

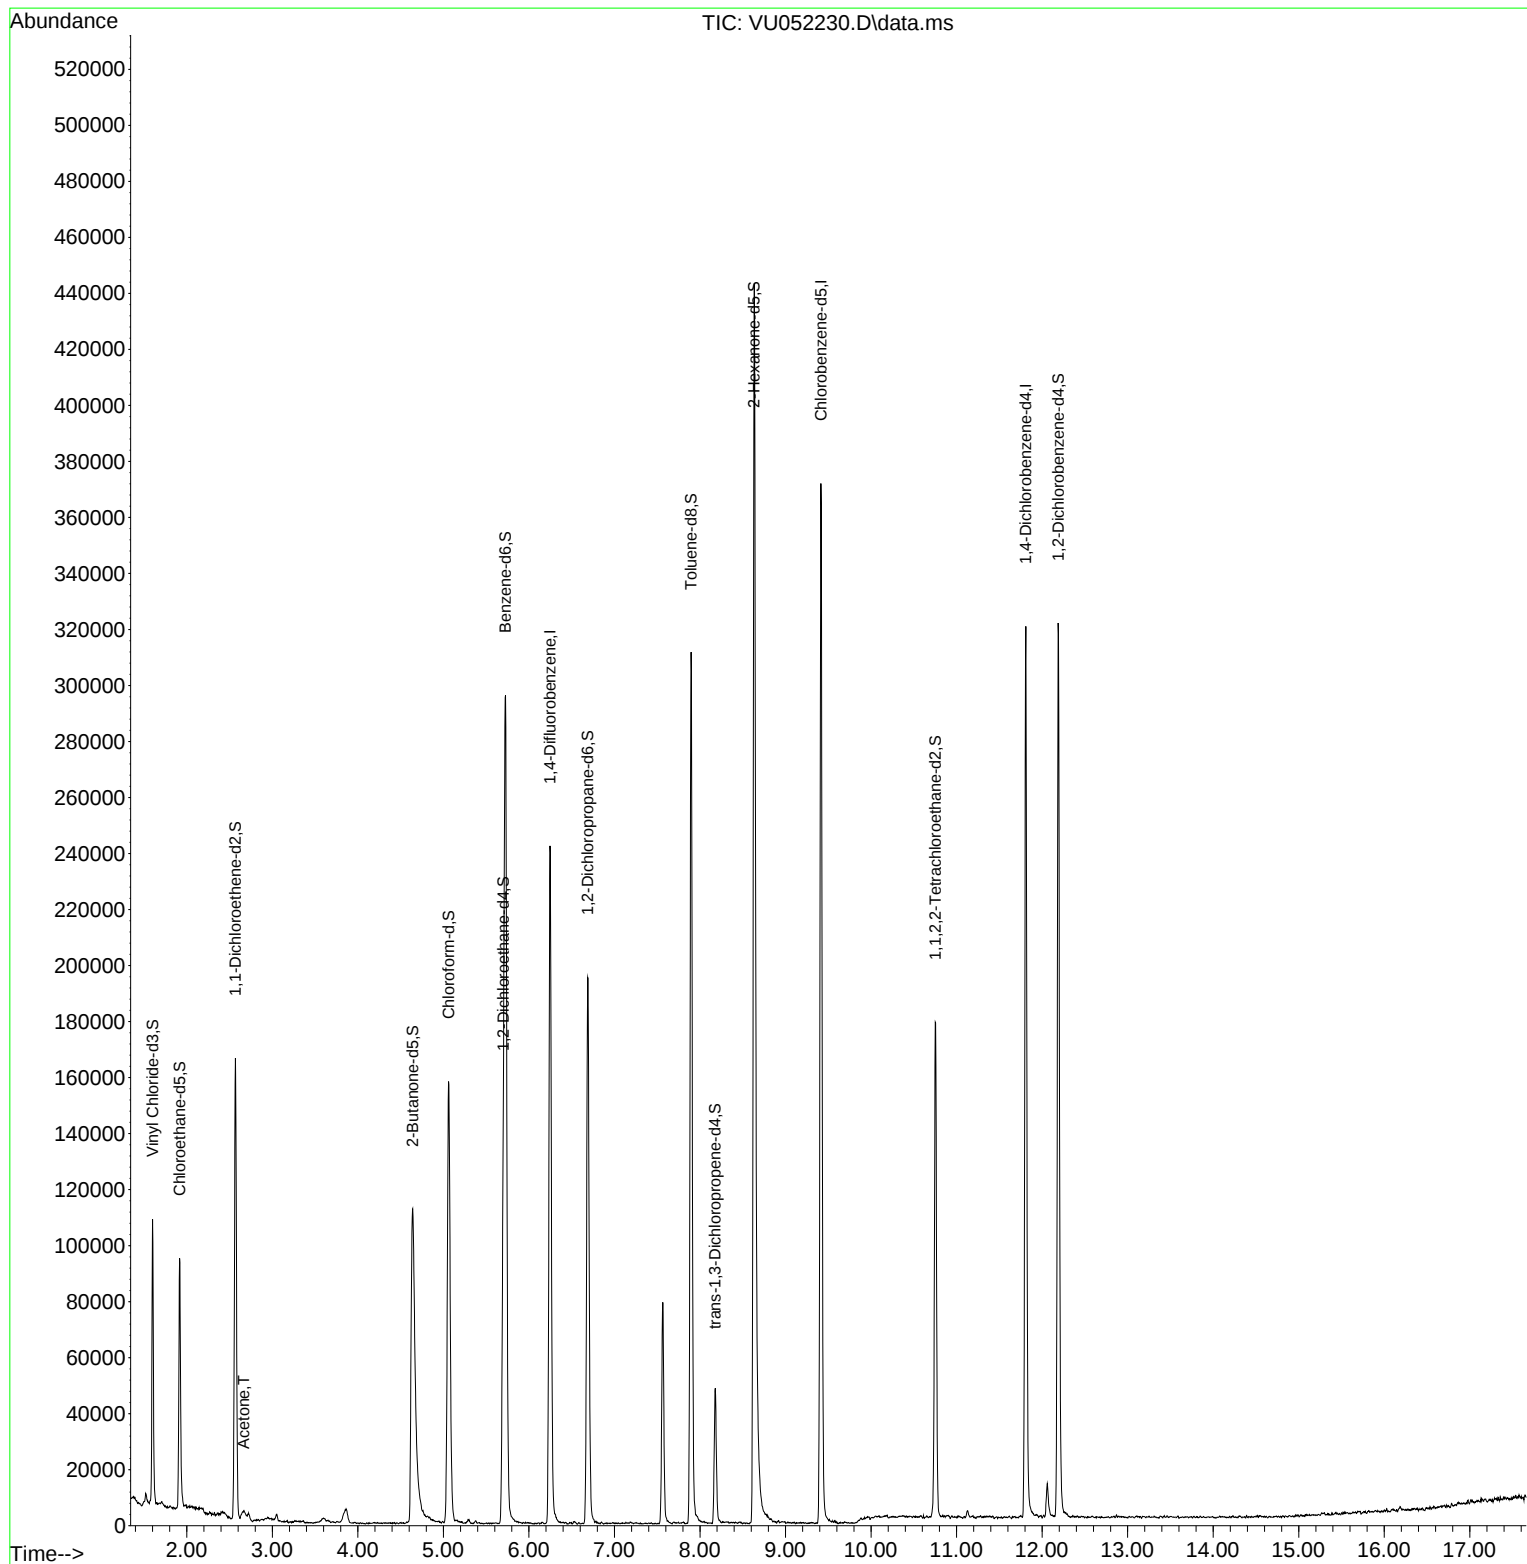

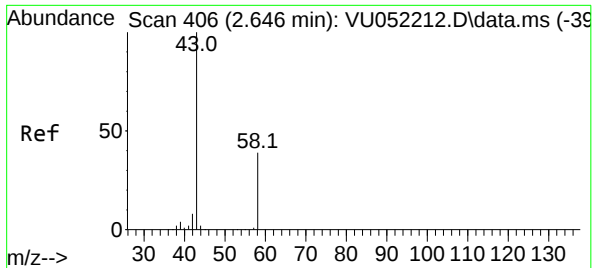

#13

Acetone

Concen: 2.664 ug/L

RT: 2.665 min Scan# 41

Delta R.T. 0.019 min

Lab File: VU052230.D

Acq: 08 Dec 2022 05:20

Instrument :

MSVOA\_U

ClientSampleId :

C0EJ0

Tgt Ion: 43 Resp: 6644

Ion Ratio Lower Upper

43 100

58 20.4 0.0 76.0

