

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052234.D
 Acq On : 08 Dec 2022 06:58
 Operator : JC/MD
 Sample : N5916-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5N40

Quant Time: Dec 08 07:46:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	220541	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	228195	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	97104	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	82010	3.823	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%
7) Chloroethane-d5	1.916	69	73120	4.388	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.568	65	31727	4.126	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	4.639	46	245558	63.150	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.300%
24) Chloroform-d	5.060	84	157828	5.007	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.700	65	83913	5.271	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	5.726	84	315780	4.661	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.687	67	106194	5.065	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.400%
41) Toluene-d8	7.896	98	240403	3.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	8.179	79	31528	4.127	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.600%
46) 2-Hexanone-d5	8.632	63	177003	54.667	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.340%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	98006	5.391	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.800%
66) 1,2-Dichlorobenzene-d4	12.189	152	92722	4.987	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						Qvalue
13) Acetone	2.668	43	21383	8.098	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052234.D
Acq On : 08 Dec 2022 06:58
Operator : JC/MD
Sample : N5916-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N40

Quant Time: Dec 08 07:46:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

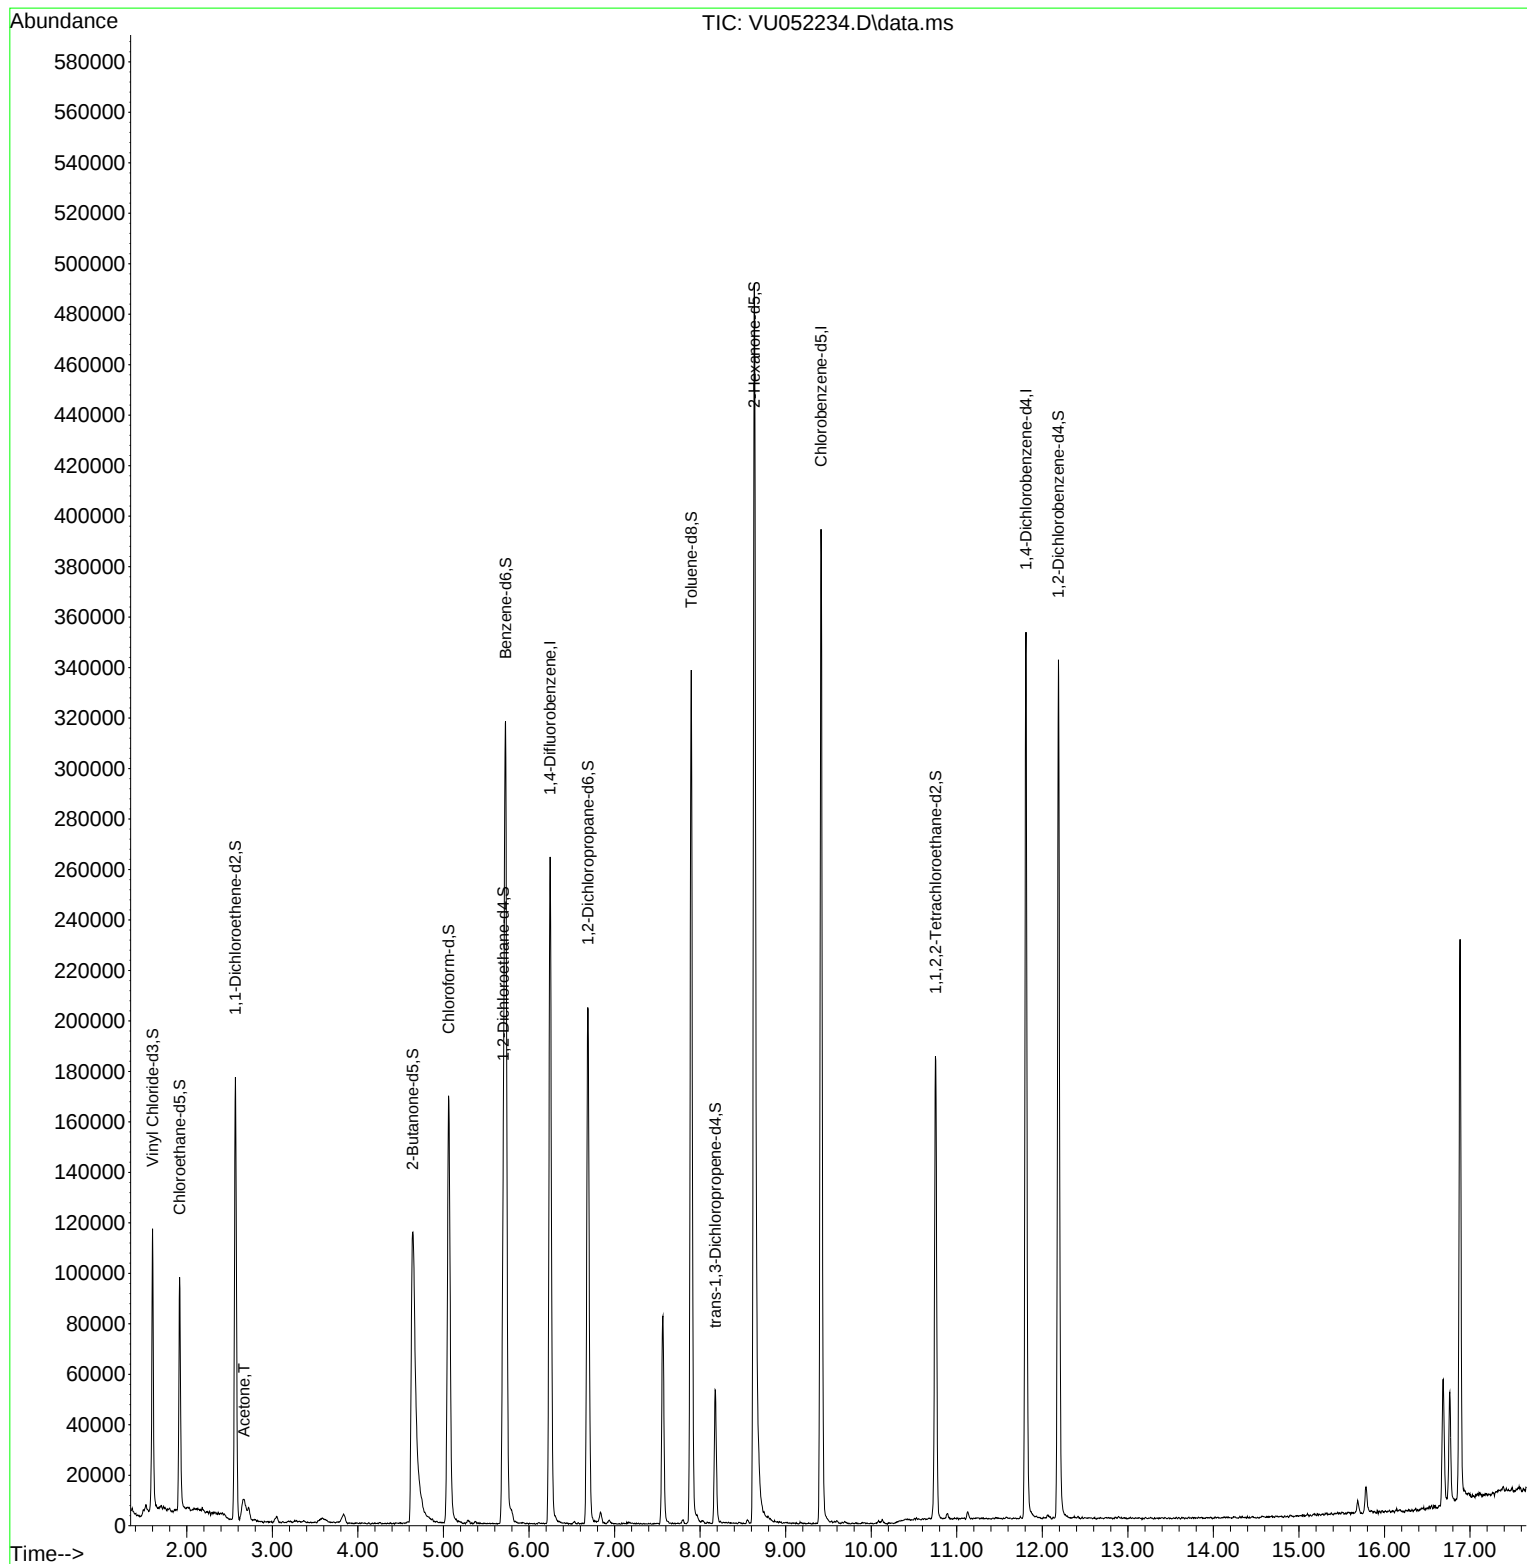

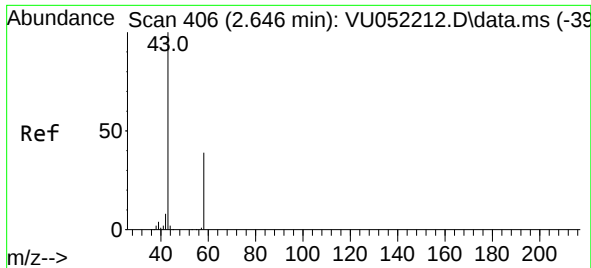

#13

Acetone

Concen: 8.098 ug/L

RT: 2.668 min Scan# 41

Delta R.T. 0.022 min

Lab File: VU052234.D


Acq: 08 Dec 2022 06:58

Instrument :

MSVOA_U

ClientSampleId :

F5N40

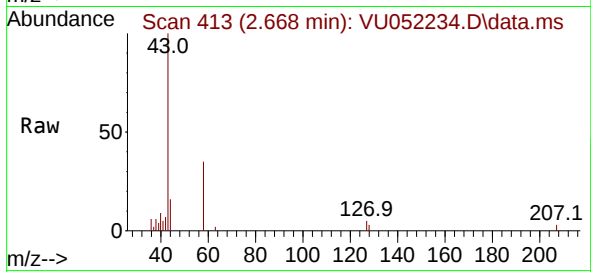

Tgt Ion: 43 Resp: 21383

Ion Ratio Lower Upper

43 100

58 35.2 0.0 76.0

