

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052201.D
 Acq On : 07 Dec 2022 17:09
 Operator : JC/MD
 Sample : N5930-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ89

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVV	111618	135031	16.68%	1.910%
2	1.912	169	178	198	rVB	95750	139262	17.20%	1.970%
3	2.568	369	382	397	rBV3	202783	366122	45.22%	5.180%
4	3.871	764	787	803	rBV2	54131	170609	21.07%	2.414%
5	4.629	1005	1023	1063	rBV2	122773	405484	50.08%	5.737%
6	5.063	1140	1158	1180	rBV	155988	352155	43.50%	4.982%
7	5.314	1215	1236	1264	rBV	168251	386283	47.71%	5.465%
8	5.726	1342	1364	1389	rBV2	301686	793269	97.98%	11.223%
9	6.250	1513	1527	1557	rBV	240804	464799	57.41%	6.576%
10	6.543	1607	1618	1635	rVB2	27437	52687	6.51%	0.745%
11	6.690	1650	1664	1682	rBV	192818	382747	47.28%	5.415%
12	7.565	1925	1936	1954	rBV	83415	148580	18.35%	2.102%
13	7.899	2022	2040	2061	rBV	313582	560568	69.24%	7.931%
14	8.179	2114	2127	2146	rBV	52164	90436	11.17%	1.279%
15	8.552	2231	2243	2256	rBV	47880	80229	9.91%	1.135%
16	8.636	2256	2269	2307	rBV2	395701	809607	100.00%	11.454%
17	9.417	2495	2512	2535	rBV	339420	578314	71.43%	8.182%
18	10.755	2916	2928	2944	rBV	160329	262595	32.43%	3.715%
19	10.893	2961	2971	2984	rBV3	5918	10057	1.24%	0.142%
20	11.812	3244	3257	3283	rBV	259267	425664	52.58%	6.022%
21	12.192	3363	3375	3398	rBV	272787	453724	56.04%	6.419%




Sum of corrected areas: 7068222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052201.D
Acq On : 07 Dec 2022 17:09
Operator : JC/MD
Sample : N5930-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

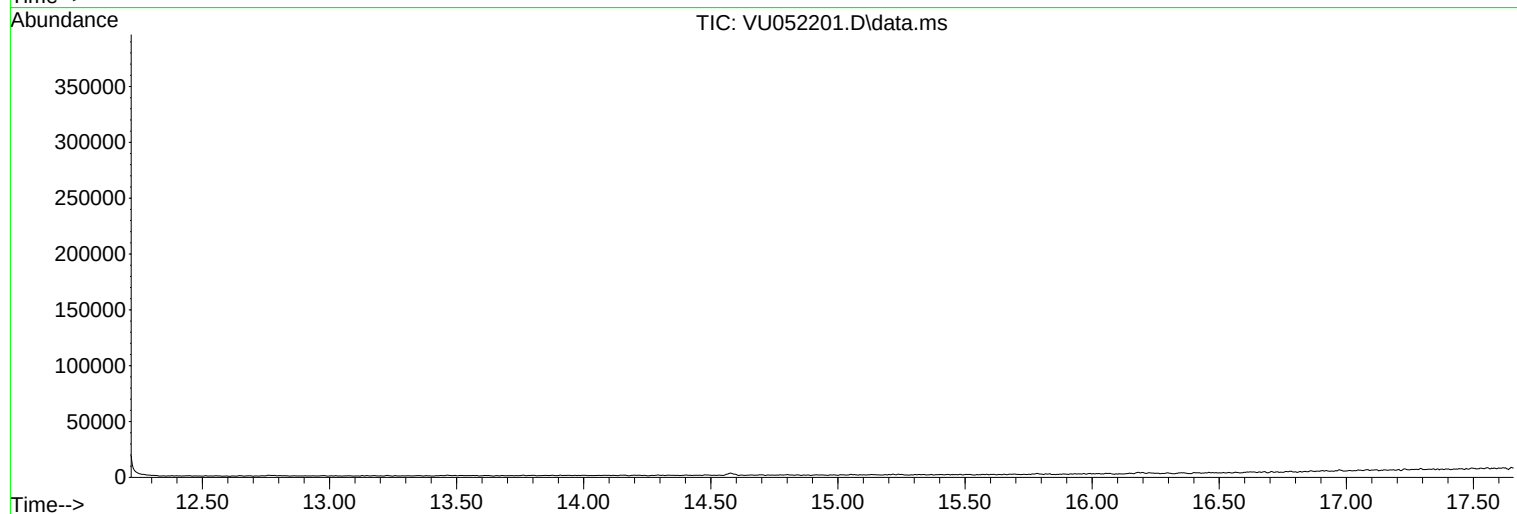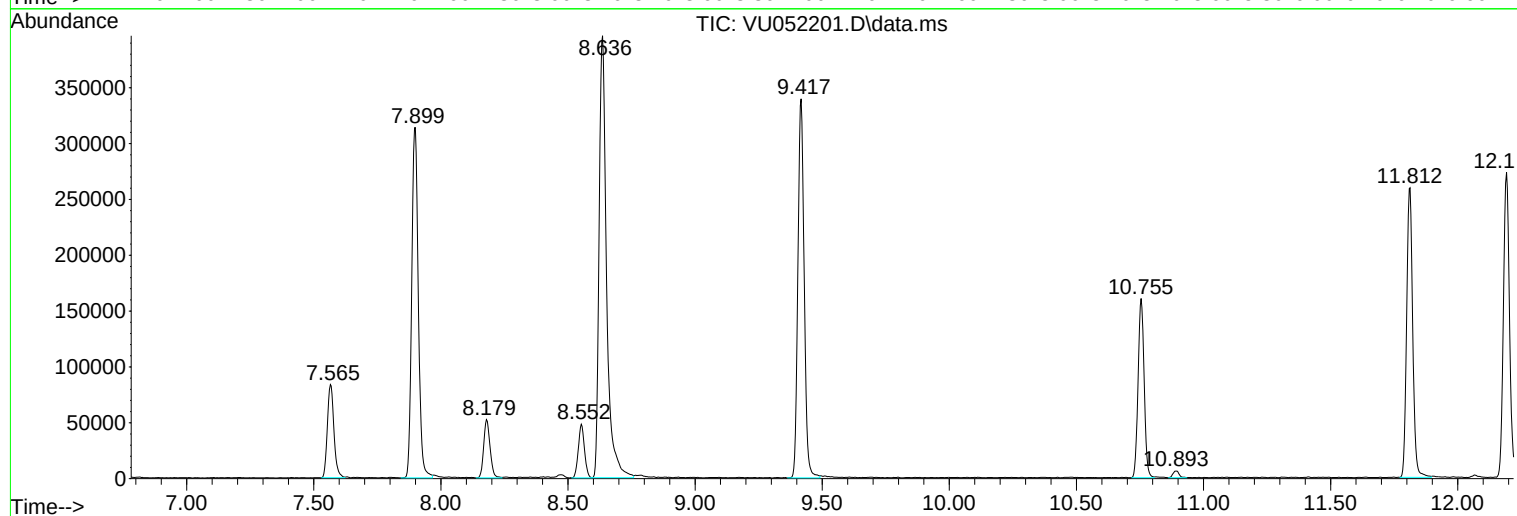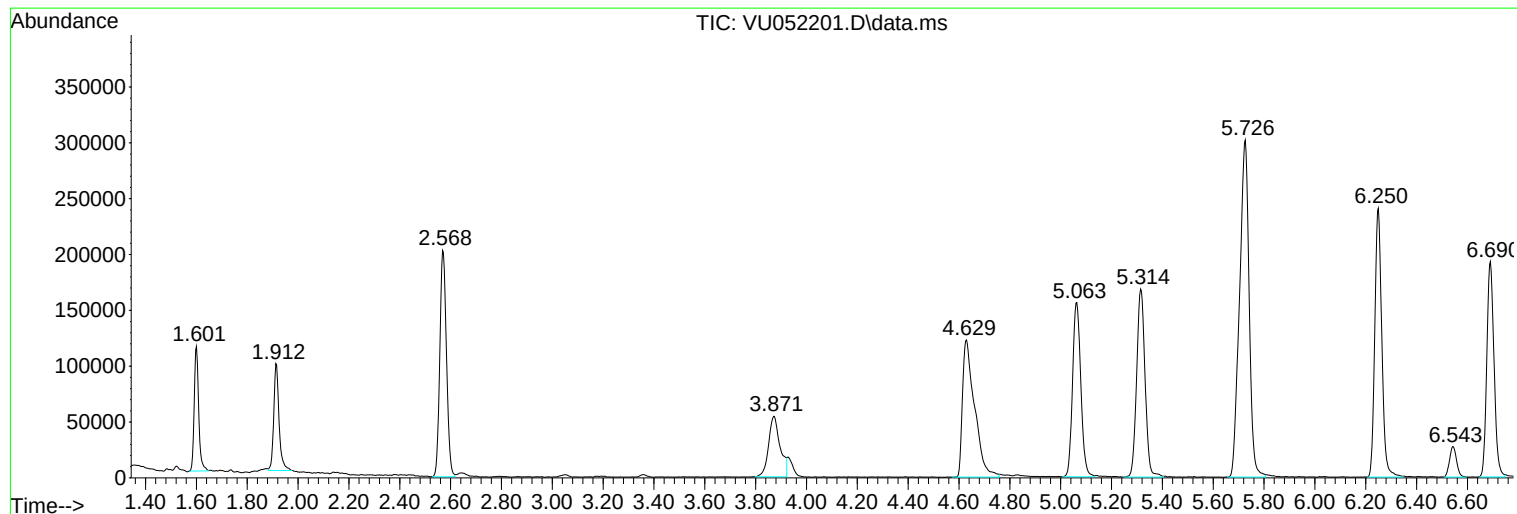

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052201.D
Acq On : 07 Dec 2022 17:09
Operator : JC/MD
Sample : N5930-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052201.D
Acq On : 07 Dec 2022 17:09
Operator : JC/MD
Sample : N5930-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc