

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052202.D
 Acq On : 07 Dec 2022 17:33
 Operator : JC/MD
 Sample : N5930-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ88

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	112662	134901	15.86%	1.962%
2	1.916	170	179	198	rBV	95769	133978	15.75%	1.949%
3	2.568	367	382	397	rBV2	182598	303033	35.62%	4.407%
4	2.649	397	407	421	rVB5	3886	9208	1.08%	0.134%
5	3.864	761	785	787	rBV	12466	34379	4.04%	0.500%
6	4.629	1011	1023	1066	rBV	120745	347854	40.89%	5.059%
7	5.060	1141	1157	1188	rBV	154050	360070	42.33%	5.237%
8	5.314	1220	1236	1253	rBV	51112	118105	13.88%	1.718%
9	5.723	1343	1363	1387	rBV2	302151	792409	93.15%	11.525%
10	6.247	1509	1526	1548	rBV	244304	471343	55.41%	6.855%
11	6.690	1646	1664	1686	rBV	194109	382983	45.02%	5.570%
12	7.565	1924	1936	1960	rBV	82650	149154	17.53%	2.169%
13	7.896	2025	2039	2060	rBV	314177	550410	64.71%	8.005%
14	8.179	2113	2127	2140	rBV	51633	88525	10.41%	1.287%
15	8.552	2230	2243	2257	rBV	215760	371224	43.64%	5.399%
16	8.636	2257	2269	2309	rVB2	421685	850637	100.00%	12.371%
17	9.414	2496	2511	2534	rBV	356271	602313	70.81%	8.760%
18	10.755	2915	2928	2944	rBV	168231	274713	32.29%	3.995%
19	11.809	3244	3256	3273	rBV	270741	443529	52.14%	6.451%
20	12.189	3359	3374	3398	rBV	275604	457096	53.74%	6.648%




Sum of corrected areas: 6875864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052202.D
Acq On : 07 Dec 2022 17:33
Operator : JC/MD
Sample : N5930-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

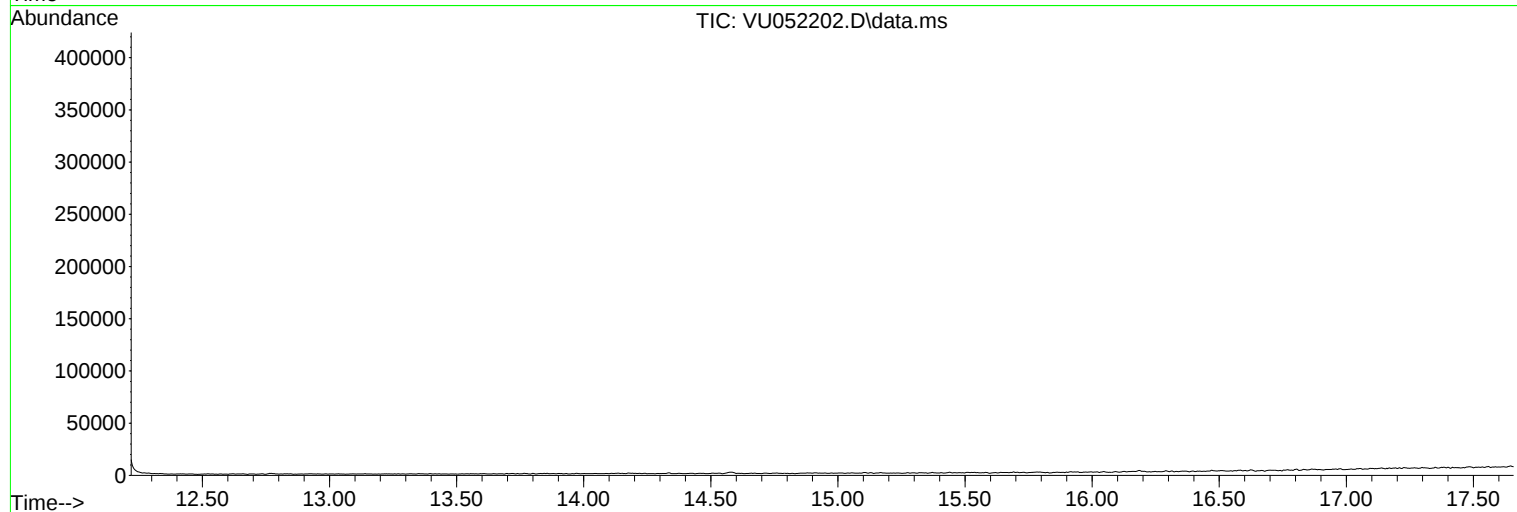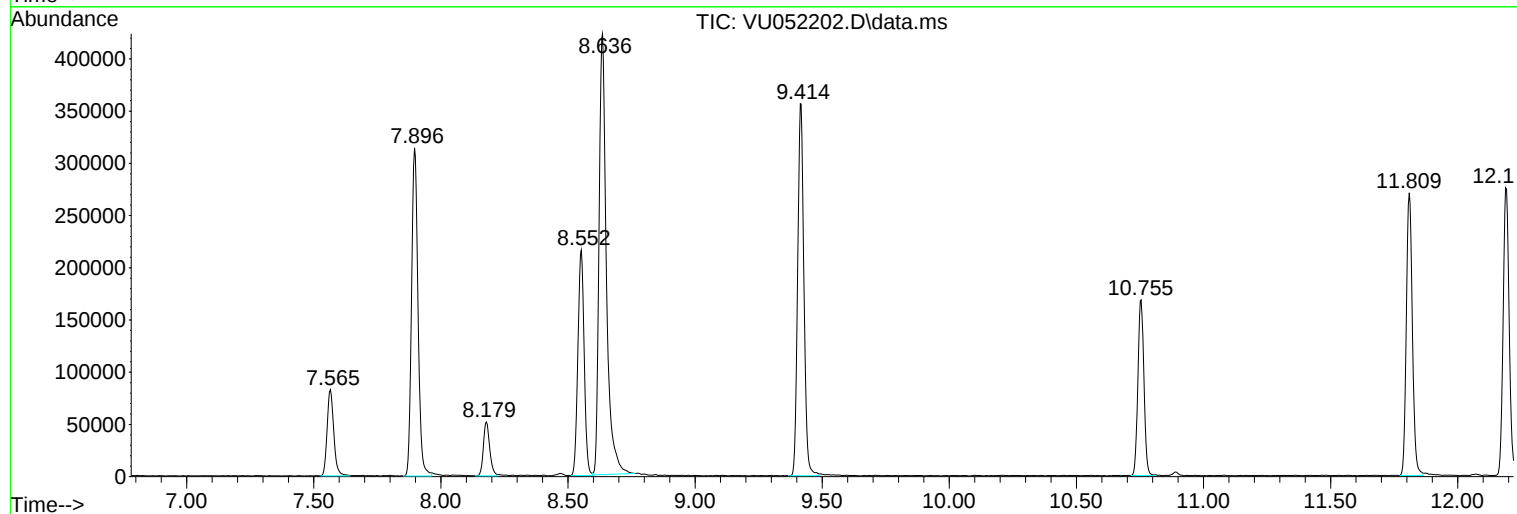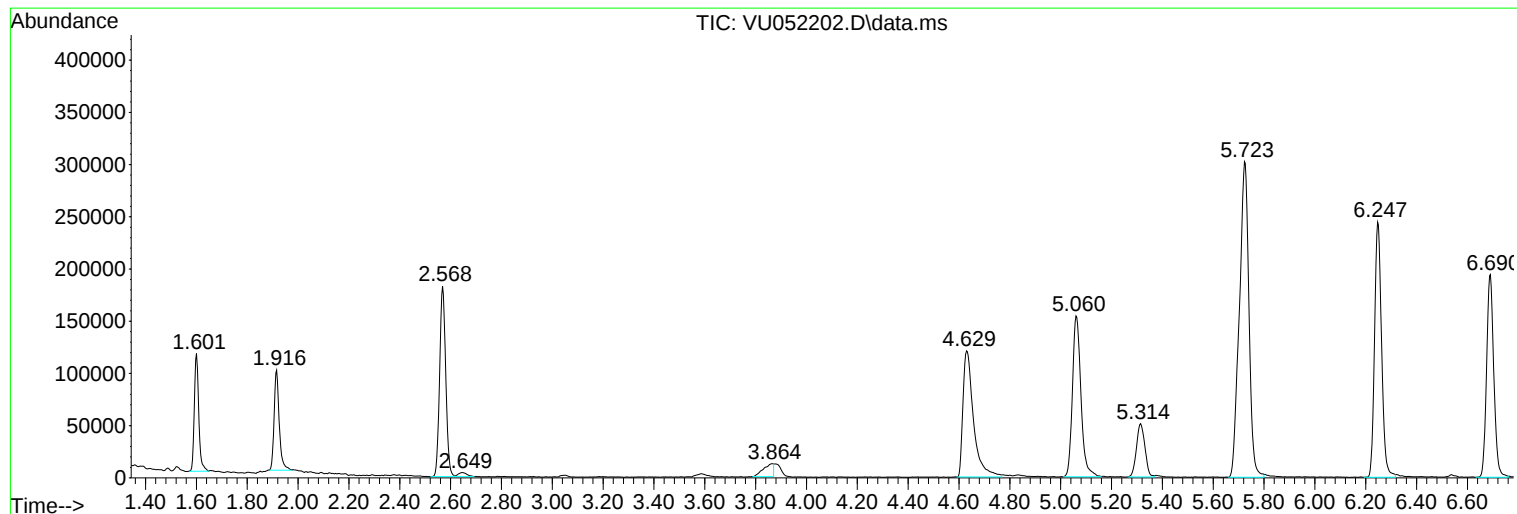

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052202.D
Acq On : 07 Dec 2022 17:33
Operator : JC/MD
Sample : N5930-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052202.D
Acq On : 07 Dec 2022 17:33
Operator : JC/MD
Sample : N5930-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc