

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052203.D
 Acq On : 07 Dec 2022 17:57
 Operator : JC/MD
 Sample : N5930-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ92

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rVB	111754	138976	15.98%	2.094%
2	1.916	170	179	202	rBV	97648	140642	16.17%	2.119%
3	2.568	369	382	396	rBV	173747	280955	32.30%	4.233%
4	3.600	682	703	723	rBV	4683	18665	2.15%	0.281%
5	3.874	763	788	790	rBV	14902	35612	4.09%	0.537%
6	4.636	1009	1025	1060	rBV	115440	358457	41.20%	5.401%
7	5.063	1142	1158	1193	rVB2	164706	390029	44.83%	5.877%
8	5.311	1224	1235	1248	rVB7	3844	9475	1.09%	0.143%
9	5.726	1341	1364	1392	rBV2	307616	815396	93.73%	12.286%
10	6.247	1513	1526	1545	rBV	235994	460687	52.96%	6.941%
11	6.690	1649	1664	1685	rBV	197821	390675	44.91%	5.886%
12	7.565	1921	1936	1958	rBV2	83779	152977	17.58%	2.305%
13	7.896	2025	2039	2061	rBV	321846	567569	65.24%	8.552%
14	8.179	2114	2127	2144	rBV	53632	93466	10.74%	1.408%
15	8.636	2255	2269	2297	rBV2	434352	869950	100.00%	13.108%
16	9.414	2499	2511	2533	rBV	350484	593137	68.18%	8.937%
17	10.755	2913	2928	2945	rBV	170308	277806	31.93%	4.186%
18	11.809	3244	3256	3278	rBV	282347	451546	51.90%	6.804%
19	12.057	3323	3333	3360	rBV2	46705	89001	10.23%	1.341%
20	12.192	3361	3375	3399	rBV	304383	501938	57.70%	7.563%




Sum of corrected areas: 6636959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052203.D
Acq On : 07 Dec 2022 17:57
Operator : JC/MD
Sample : N5930-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

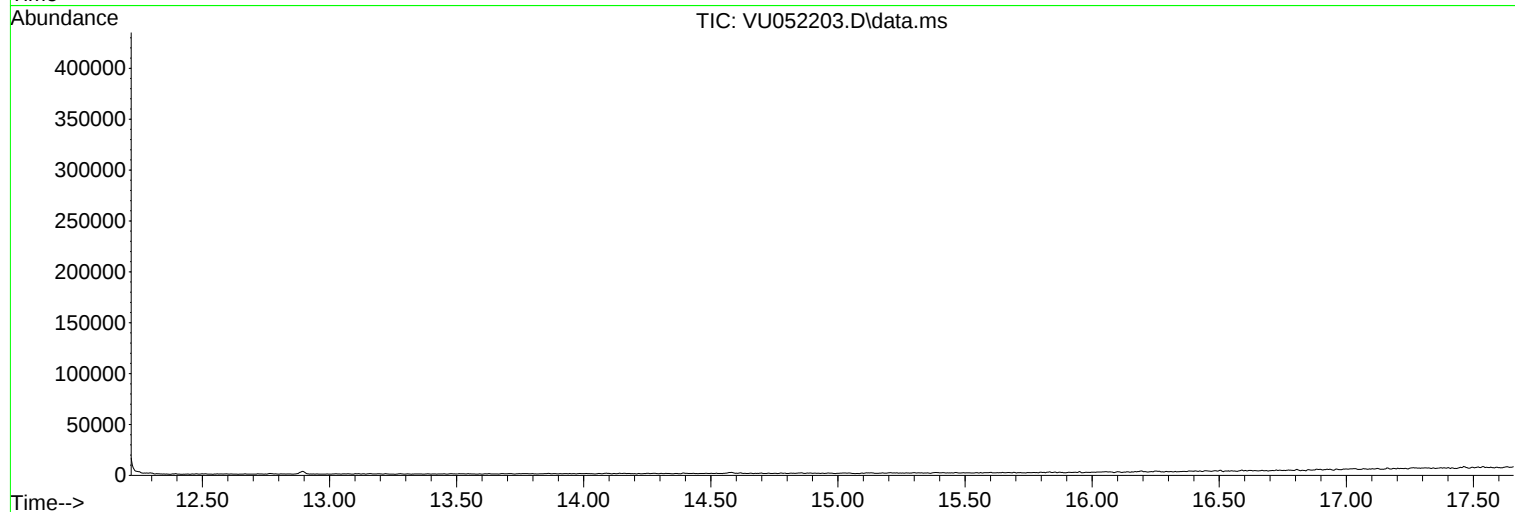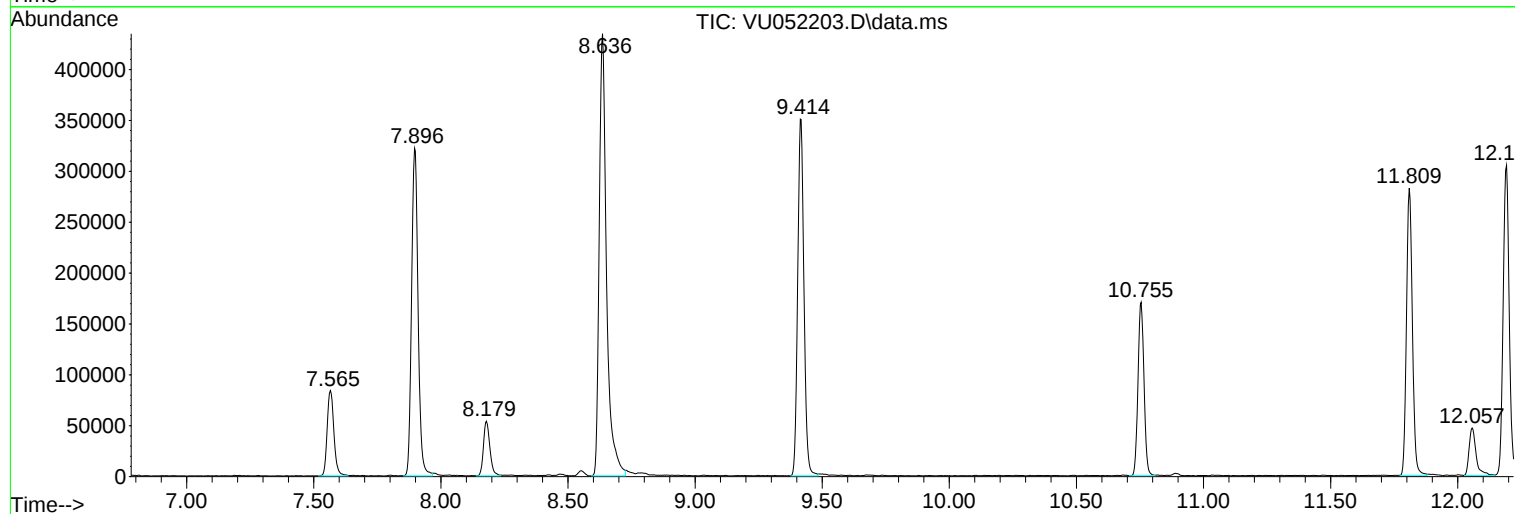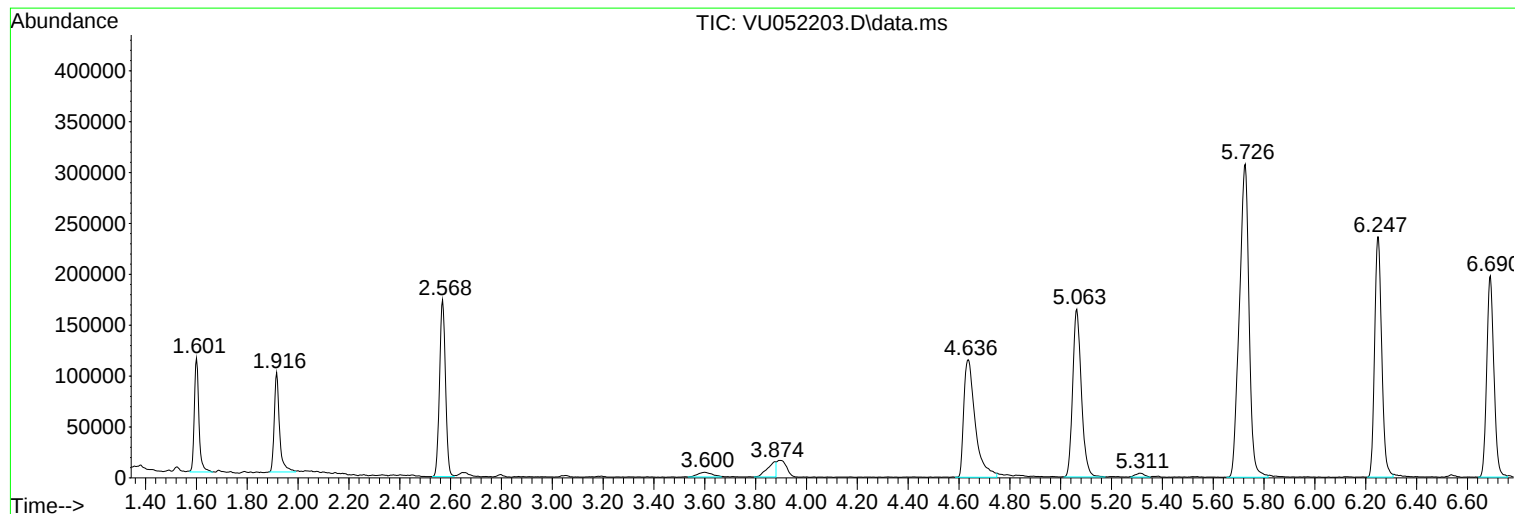

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052203.D
Acq On : 07 Dec 2022 17:57
Operator : JC/MD
Sample : N5930-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ92










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.057	0.99 ug/L	89001	1,4-Dichlorobenzene-d4	11.809

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	83
2		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	78
3		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	78
4		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	64
5		1-Hexanol, 2-ethyl-	130	C8H18O	000104-76-7	59

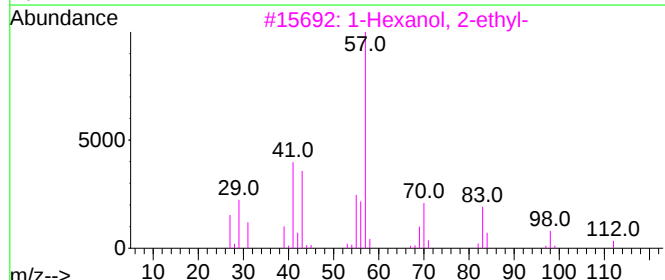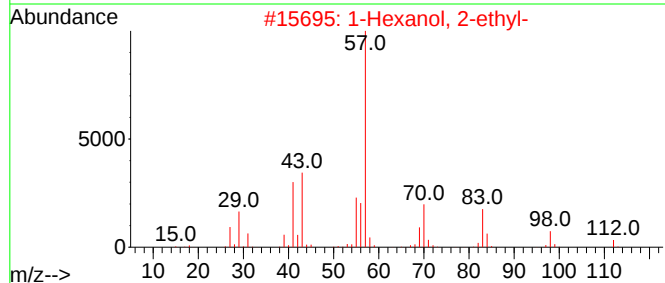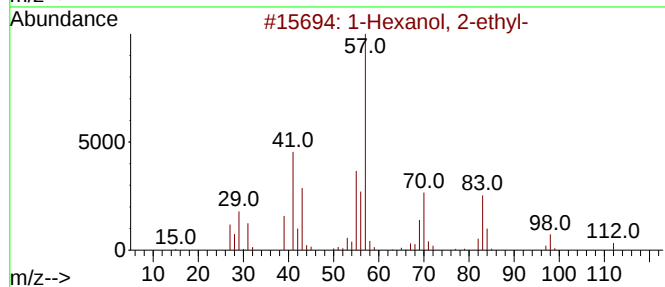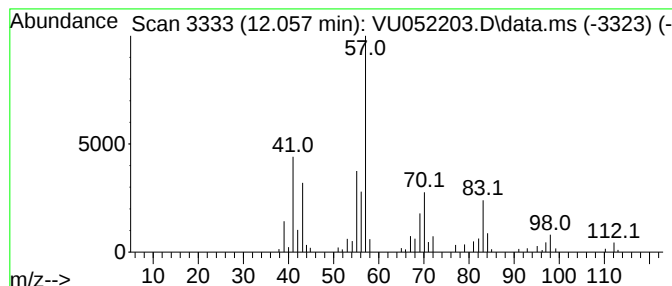

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052203.D
Acq On : 07 Dec 2022 17:57
Operator : JC/MD
Sample : N5930-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	12.057	1.0	ug/L	89001	3	11.809	451546	5.0