

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052206.D
 Acq On : 07 Dec 2022 19:09
 Operator : JC/MD
 Sample : N5916-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5N20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.385	11	14	37	rVB3	8224	14918	1.63%	0.218%
2	1.600	73	81	97	rBV	125195	147338	16.09%	2.152%
3	1.732	116	122	129	rVB	6947	9179	1.00%	0.134%
4	1.916	170	179	193	rBV	93669	130440	14.24%	1.905%
5	2.568	370	382	401	rBV3	198239	358915	39.19%	5.243%
6	3.874	752	788	814	rVB2	23193	115156	12.57%	1.682%
7	4.636	1011	1025	1060	rBV	121773	370671	40.47%	5.414%
8	5.060	1141	1157	1182	rBV	160289	365396	39.90%	5.337%
9	5.722	1342	1363	1378	rBV2	306691	818434	89.37%	11.955%
10	5.793	1380	1385	1401	rVB2	22849	46518	5.08%	0.679%
11	6.247	1512	1526	1551	rBV	244685	477555	52.14%	6.976%
12	6.690	1649	1664	1686	rBV	198260	393411	42.96%	5.747%
13	7.565	1924	1936	1955	rBV	85538	151714	16.57%	2.216%
14	7.896	2026	2039	2059	rBV	325216	574258	62.70%	8.388%
15	8.179	2116	2127	2143	rBV2	53180	91302	9.97%	1.334%
16	8.636	2255	2269	2307	rBV2	449483	915830	100.00%	13.378%
17	9.414	2499	2511	2533	rBV	360188	611719	66.79%	8.935%
18	10.754	2916	2928	2943	rBV	173291	282674	30.87%	4.129%
19	11.745	3228	3236	3244	rBV3	6672	10289	1.12%	0.150%
20	11.809	3244	3256	3275	rBV	285958	466468	50.93%	6.814%
21	12.192	3359	3375	3397	rBV	290972	493774	53.92%	7.213%




Sum of corrected areas: 6845959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052206.D
Acq On : 07 Dec 2022 19:09
Operator : JC/MD
Sample : N5916-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

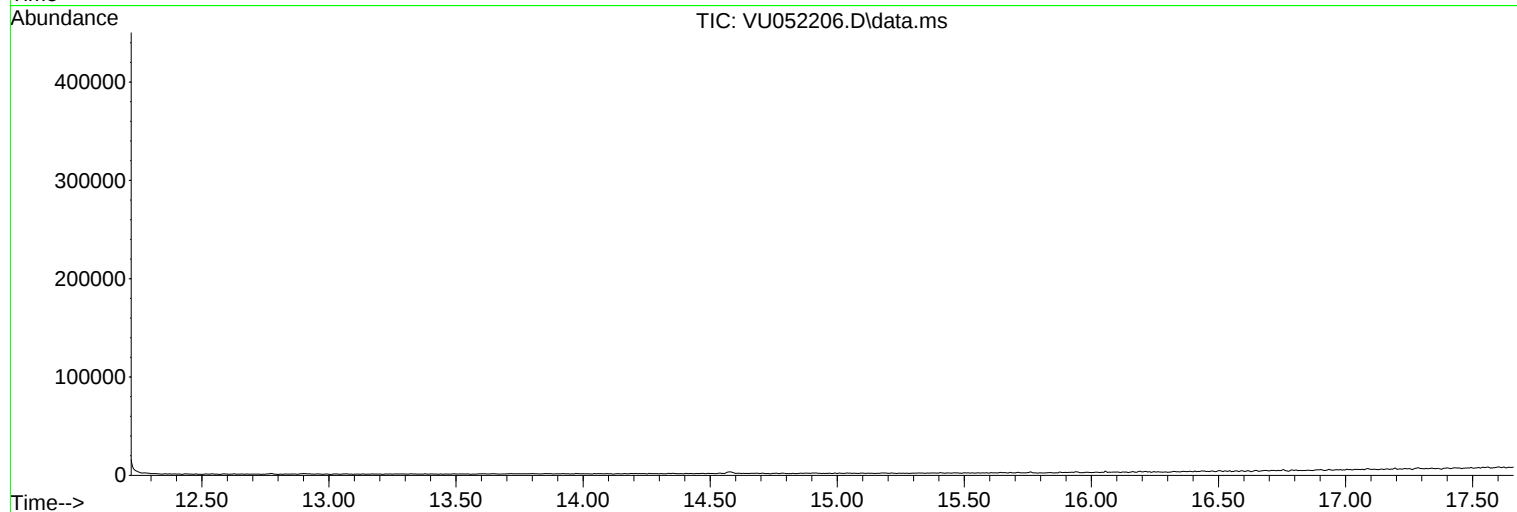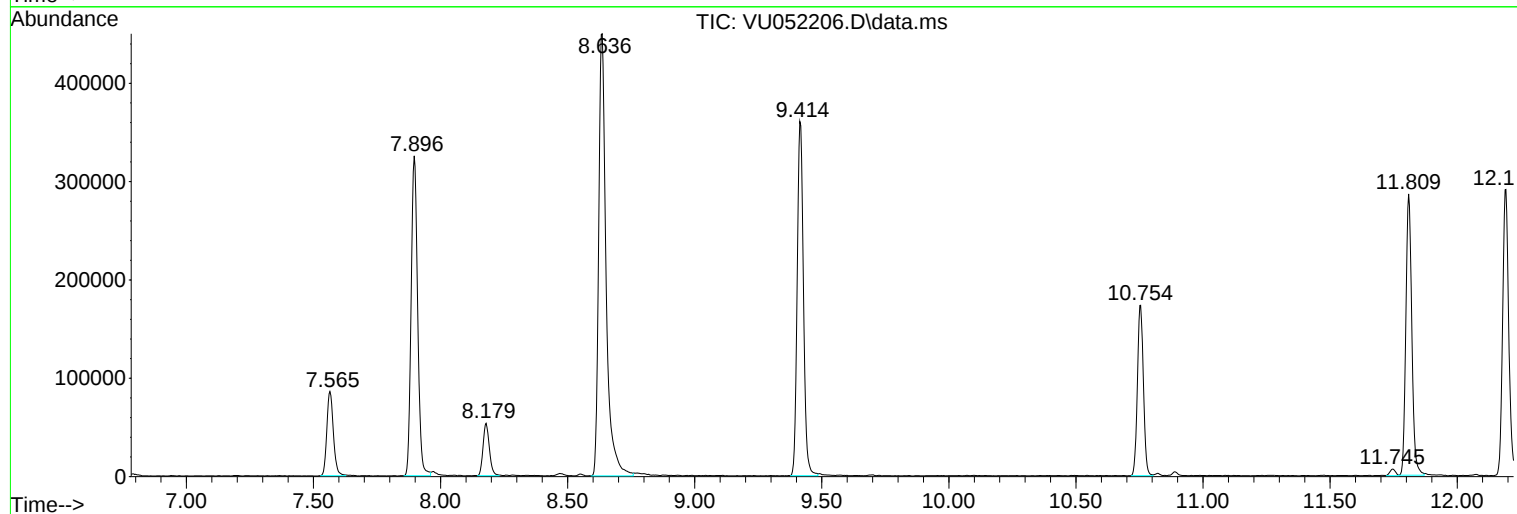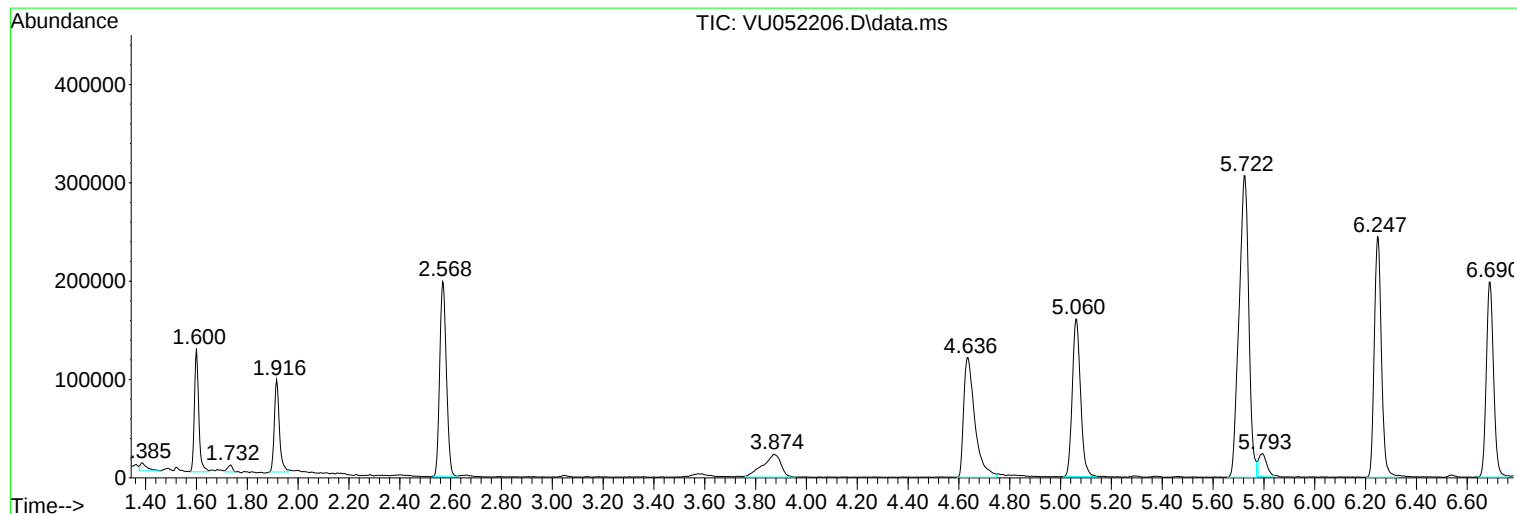

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052206.D
Acq On : 07 Dec 2022 19:09
Operator : JC/MD
Sample : N5916-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052206.D
Acq On : 07 Dec 2022 19:09
Operator : JC/MD
Sample : N5916-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc