

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052214.D
 Acq On : 07 Dec 2022 22:45
 Operator : JC/MD
 Sample : N5916-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5N26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	92	rBV	115412	145132	15.20%	2.204%
2	1.916	171	179	192	rBV	91681	125336	13.13%	1.903%
3	2.568	368	382	399	rBV	171594	279841	29.31%	4.250%
4	3.861	759	784	810	rVB4	15315	64660	6.77%	0.982%
5	4.632	1011	1024	1062	rBV	132243	390903	40.94%	5.936%
6	5.063	1142	1158	1193	rBV	153246	351710	36.84%	5.341%
7	5.726	1343	1364	1399	rBV2	300477	805030	84.31%	12.226%
8	6.250	1513	1527	1544	rBV	239953	461946	48.38%	7.015%
9	6.690	1650	1664	1684	rBV	195802	381071	39.91%	5.787%
10	7.565	1921	1936	1958	rBV	79314	144860	15.17%	2.200%
11	7.896	2024	2039	2057	rBV	308775	544524	57.03%	8.269%
12	8.179	2112	2127	2144	rBV2	51715	90860	9.52%	1.380%
13	8.636	2256	2269	2304	rBV2	472230	954799	100.00%	14.500%
14	9.417	2498	2512	2536	rBV	345289	593299	62.14%	9.010%
15	10.754	2916	2928	2947	rBV	175465	281638	29.50%	4.277%
16	11.738	3226	3234	3242	rBV6	7464	10744	1.13%	0.163%
17	11.809	3242	3256	3280	rBV	275098	455289	47.68%	6.914%
18	12.192	3362	3375	3397	rBV	279694	473059	49.55%	7.184%
19	12.976	3609	3619	3631	rBV6	19031	30051	3.15%	0.456%




Sum of corrected areas: 6584752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052214.D
Acq On : 07 Dec 2022 22:45
Operator : JC/MD
Sample : N5916-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

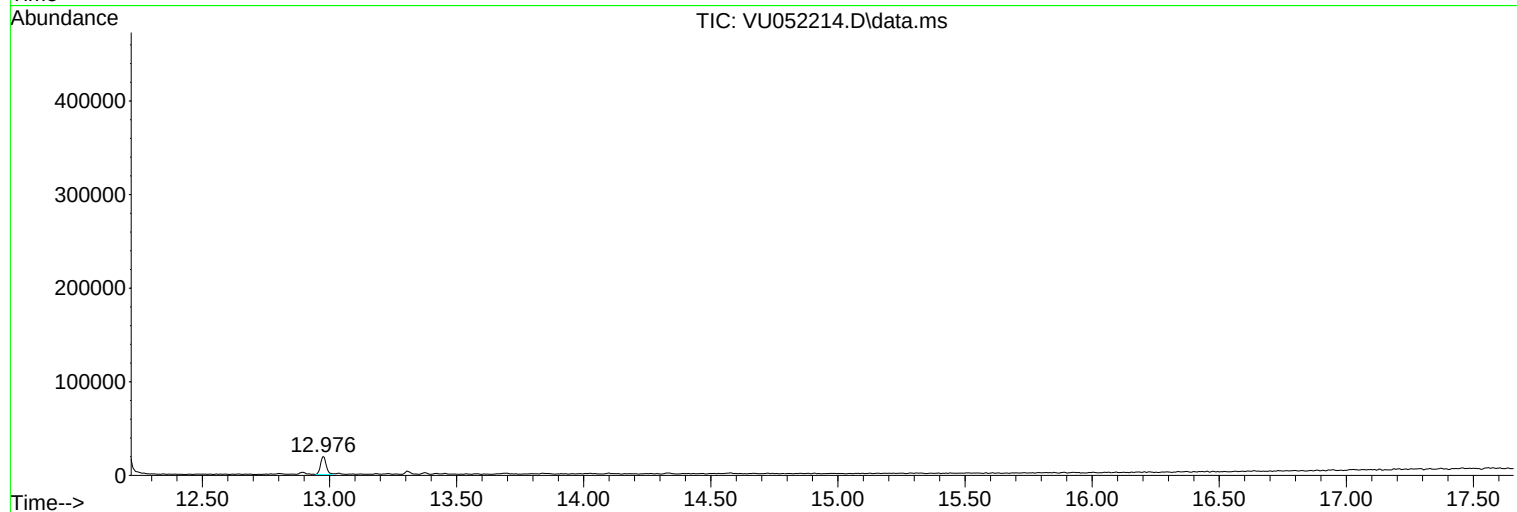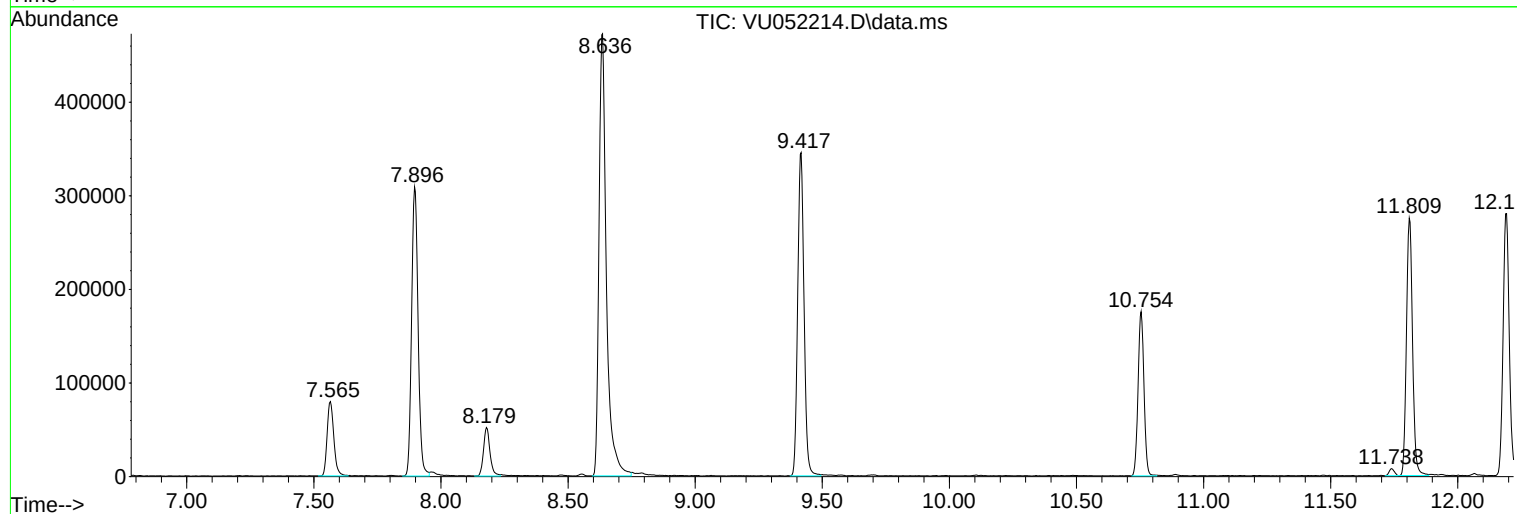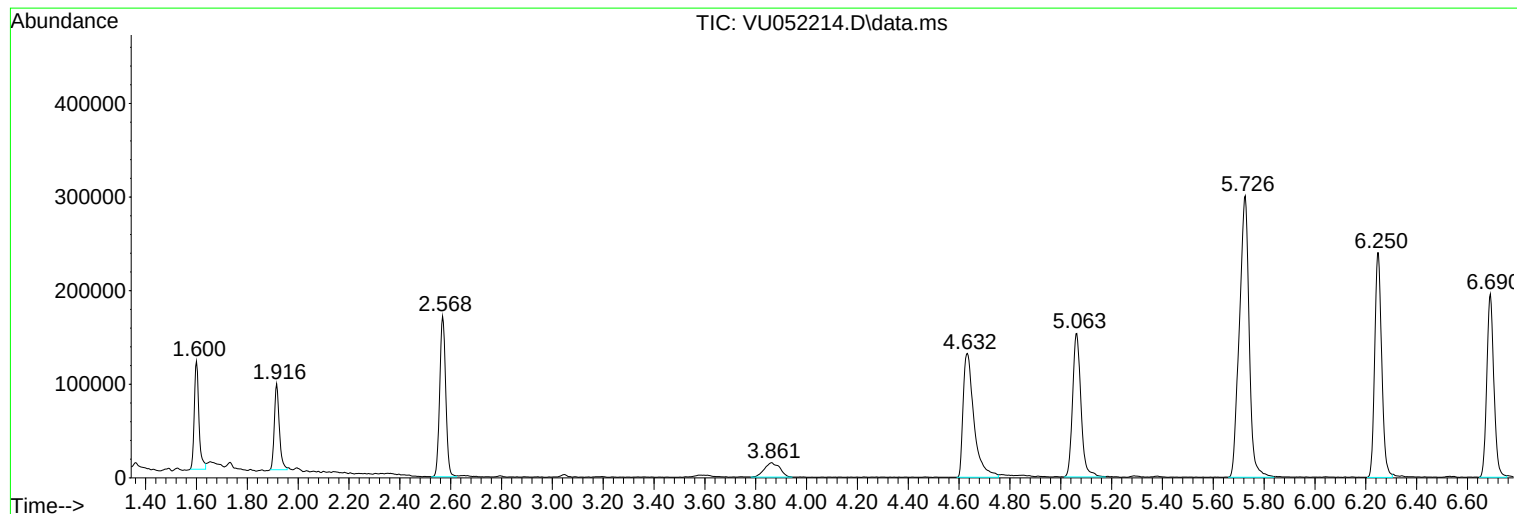

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052214.D
Acq On : 07 Dec 2022 22:45
Operator : JC/MD
Sample : N5916-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052214.D
Acq On : 07 Dec 2022 22:45
Operator : JC/MD
Sample : N5916-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc