

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052219.D
 Acq On : 08 Dec 2022 00:49
 Operator : JC/MD
 Sample : N5918-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EF1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB	114654	135625	12.31%	1.747%
2	1.916	171	179	196	rVB	98749	130623	11.86%	1.683%
3	2.568	369	382	400	rBV	175129	288639	26.20%	3.719%
4	2.723	422	430	444	rVB2	8394	15120	1.37%	0.195%
5	3.858	748	783	802	rBV	11197	53070	4.82%	0.684%
6	4.636	998	1025	1064	rBV	132842	419377	38.07%	5.403%
7	5.063	1141	1158	1182	rBV	168873	378791	34.39%	4.880%
8	5.726	1340	1364	1389	rBV2	325319	856936	77.80%	11.041%
9	6.247	1513	1526	1557	rBV	266140	515611	46.81%	6.643%
10	6.687	1648	1663	1684	rBV	211369	413832	37.57%	5.332%
11	7.565	1921	1936	1956	rBV	84062	152170	13.81%	1.961%
12	7.896	2026	2039	2067	rBV	349677	614836	55.82%	7.922%
13	8.179	2115	2127	2142	rBV2	52634	91269	8.29%	1.176%
14	8.632	2255	2268	2303	rBV2	479080	943320	85.64%	12.154%
15	9.414	2499	2511	2534	rBV	386774	683263	62.03%	8.803%
16	10.755	2913	2928	2946	rBV	182079	296368	26.91%	3.818%
17	10.893	2960	2971	2982	rVB2	6985	11709	1.06%	0.151%
18	11.809	3244	3256	3281	rBV2	337276	659324	59.86%	8.495%
19	12.198	3361	3377	3407	rBV2	441784	1101528	100.00%	14.192%




Sum of corrected areas: 7761411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052219.D
Acq On : 08 Dec 2022 00:49
Operator : JC/MD
Sample : N5918-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

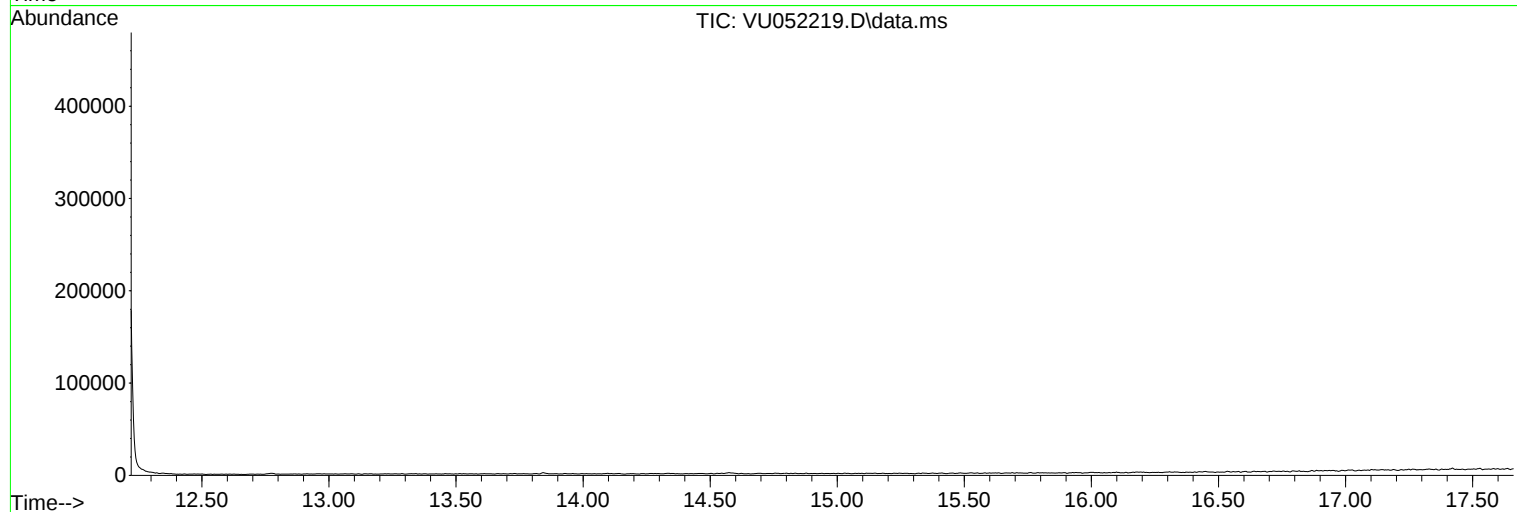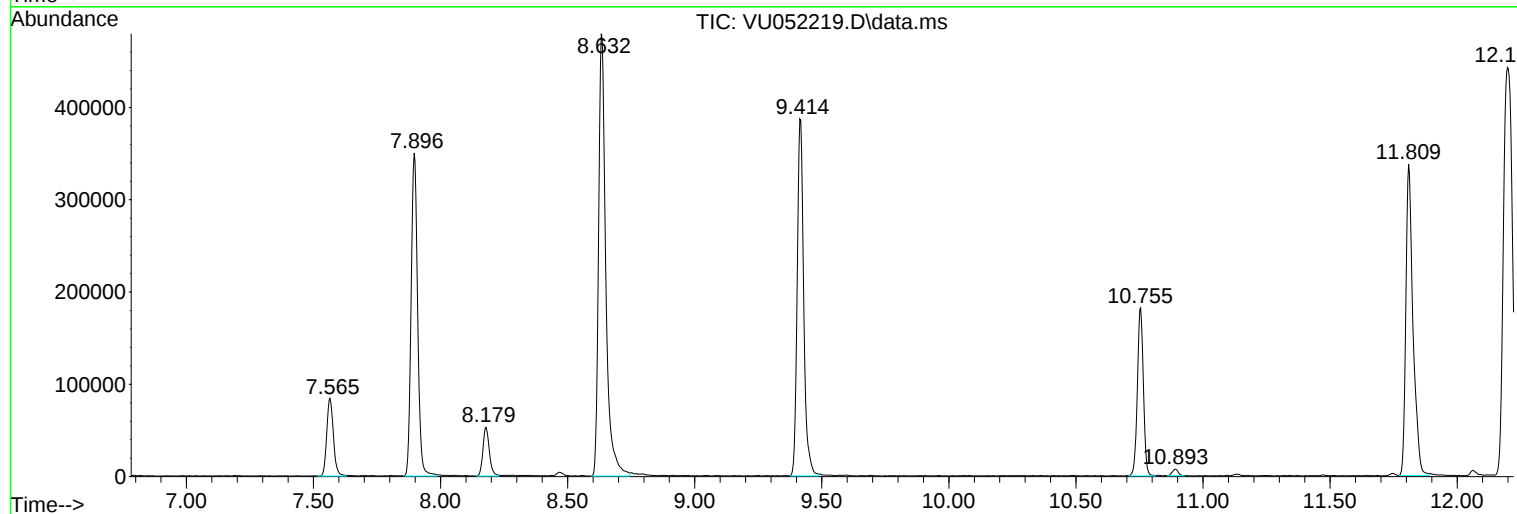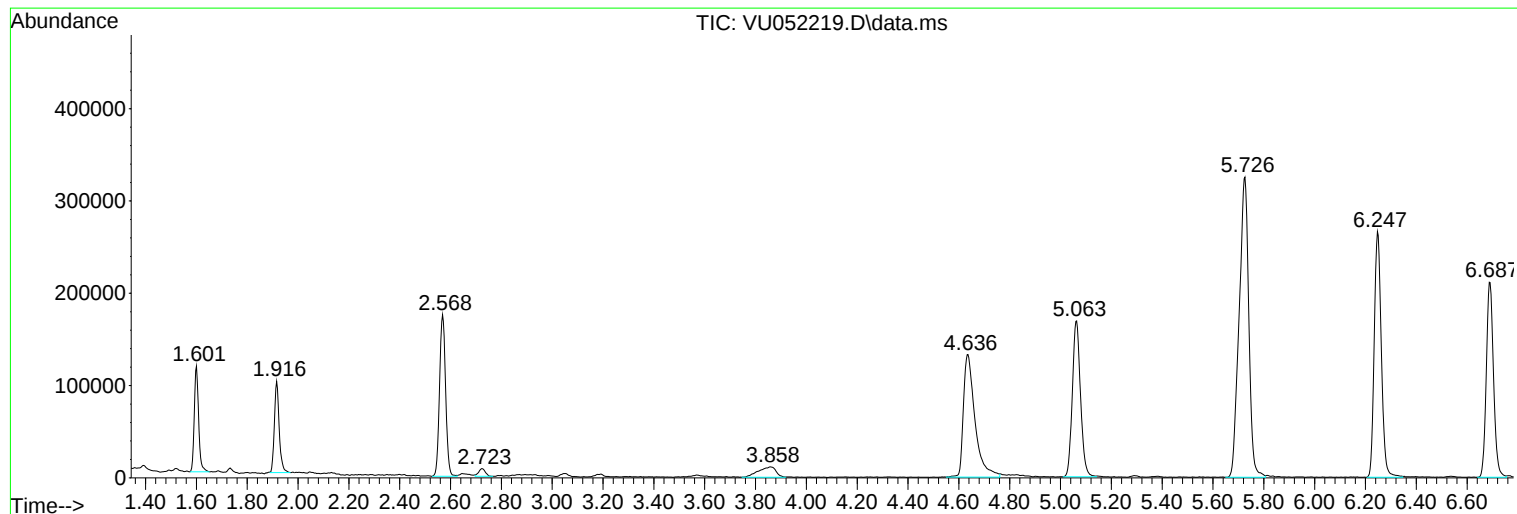

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052219.D
Acq On : 08 Dec 2022 00:49
Operator : JC/MD
Sample : N5918-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052219.D
Acq On : 08 Dec 2022 00:49
Operator : JC/MD
Sample : N5918-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc