

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052220.D
 Acq On : 08 Dec 2022 01:13
 Operator : JC/MD
 Sample : N5918-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EF4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rVB	115048	134508	14.12%	1.812%
2	1.916	171	179	196	rBV	99025	133190	13.98%	1.794%
3	2.568	369	382	395	rBV	177560	290350	30.49%	3.911%
4	2.723	422	430	446	rVB2	7830	13791	1.45%	0.186%
5	4.636	1012	1025	1064	rBV	133937	390600	41.01%	5.261%
6	5.064	1140	1158	1180	rBV	169147	380323	39.93%	5.123%
7	5.726	1343	1364	1395	rBV2	325594	869464	91.29%	11.712%
8	6.247	1509	1526	1545	rBV	264041	507883	53.33%	6.841%
9	6.691	1650	1664	1683	rBV	211010	419431	44.04%	5.650%
10	7.565	1923	1936	1962	rBV2	87643	154712	16.24%	2.084%
11	7.896	2026	2039	2070	rBV	348667	616588	64.74%	8.306%
12	8.179	2116	2127	2145	rBV2	52224	90425	9.49%	1.218%
13	8.469	2207	2217	2232	rVB2	7877	14596	1.53%	0.197%
14	8.633	2256	2268	2301	rBV2	481579	952387	100.00%	12.829%
15	9.414	2498	2511	2534	rBV	391307	667679	70.11%	8.994%
16	10.755	2913	2928	2946	rBV	180673	298202	31.31%	4.017%
17	10.893	2956	2971	2986	rVB2	17523	29810	3.13%	0.402%
18	11.809	3244	3256	3280	rBV	333894	601443	63.15%	8.102%
19	12.057	3325	3333	3349	rBV3	13837	24830	2.61%	0.334%
20	12.192	3361	3375	3406	rBV2	378269	833582	87.53%	11.229%




Sum of corrected areas: 7423794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052220.D
Acq On : 08 Dec 2022 01:13
Operator : JC/MD
Sample : N5918-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

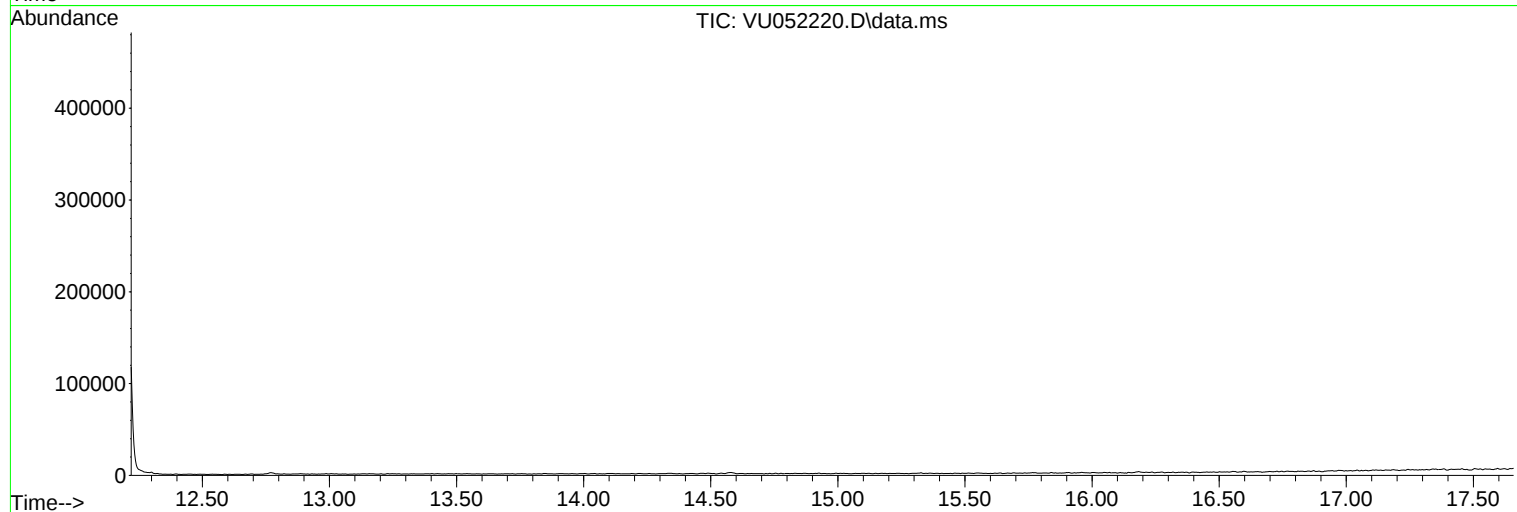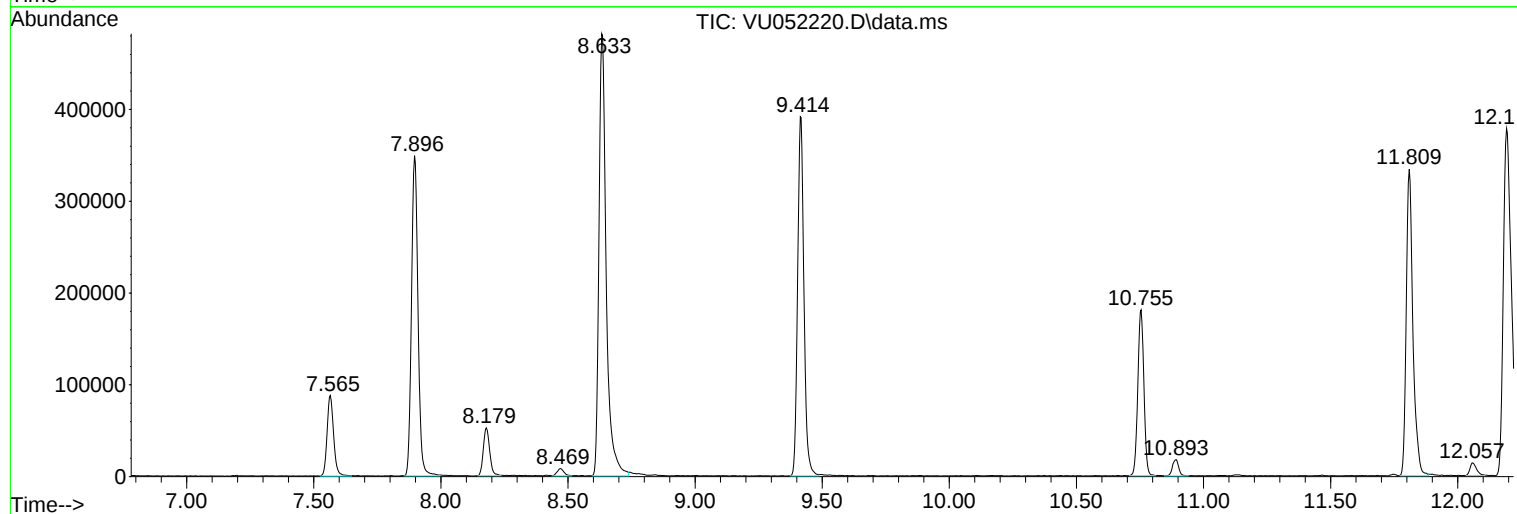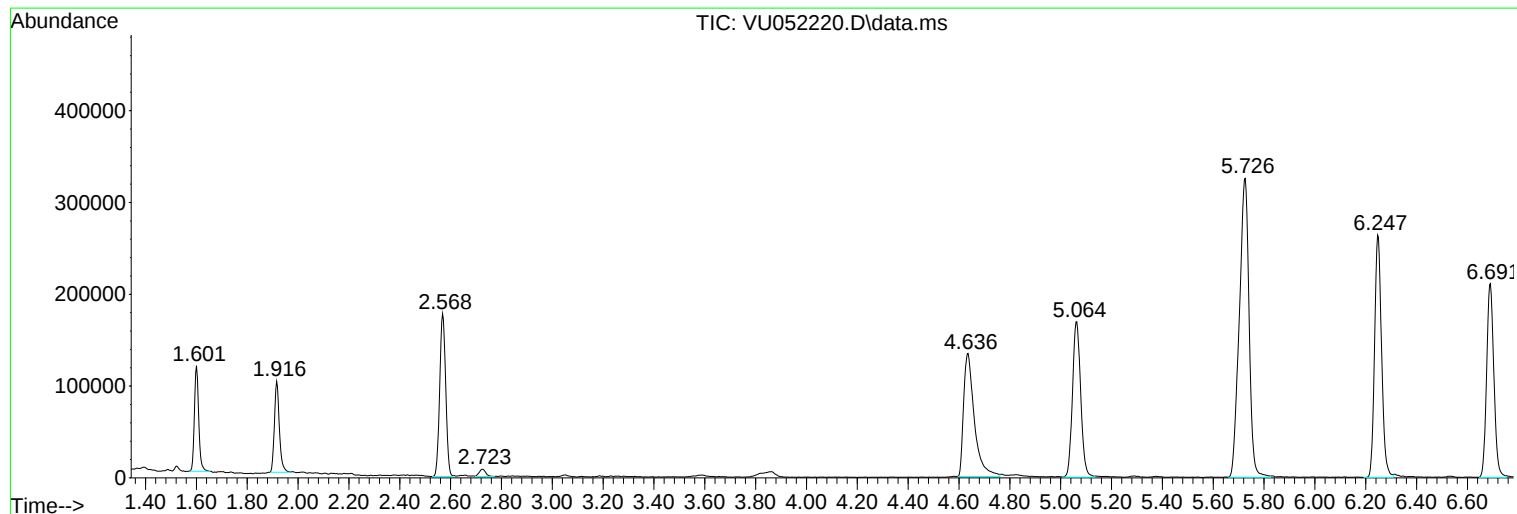

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052220.D
Acq On : 08 Dec 2022 01:13
Operator : JC/MD
Sample : N5918-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052220.D
Acq On : 08 Dec 2022 01:13
Operator : JC/MD
Sample : N5918-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EF4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc