

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
 Data File : VU052224.D
 Acq On : 08 Dec 2022 02:52
 Operator : JC/MD
 Sample : N5918-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	50	57	68	rBV	19486	24679	2.89%	0.370%
2	1.600	73	81	97	rVB	108801	132678	15.51%	1.990%
3	1.916	171	179	198	rVB	91037	127959	14.96%	1.919%
4	2.568	370	382	396	rBV	176211	281389	32.90%	4.220%
5	3.867	773	786	804	rVB3	7777	22418	2.62%	0.336%
6	4.652	1012	1030	1078	rBV2	84220	379886	44.42%	5.697%
7	5.060	1140	1157	1181	rBV	160312	367771	43.00%	5.516%
8	5.722	1342	1363	1388	rBV2	300310	802602	93.85%	12.037%
9	6.247	1509	1526	1547	rBV	241227	464951	54.37%	6.973%
10	6.690	1649	1664	1693	rBV2	194589	395628	46.26%	5.933%
11	7.565	1924	1936	1956	rBV	71414	129761	15.17%	1.946%
12	7.896	2026	2039	2058	rBV	307569	545209	63.75%	8.177%
13	8.179	2114	2127	2142	rBV	44714	78986	9.24%	1.185%
14	8.385	2182	2191	2194	rBV	7276	11243	1.31%	0.169%
15	8.639	2258	2270	2313	rBV3	358073	855227	100.00%	12.826%
16	9.414	2499	2511	2535	rBV	364154	618711	72.34%	9.279%
17	10.754	2910	2928	2941	rBV	173642	294995	34.49%	4.424%
18	11.809	3244	3256	3280	rBV	308353	522354	61.08%	7.834%
19	12.060	3324	3334	3348	rBV2	10203	19323	2.26%	0.290%
20	12.192	3363	3375	3395	rBV2	309462	567556	66.36%	8.512%
21	15.458	4375	4391	4392	rBV2	11257	24476	2.86%	0.367%




Sum of corrected areas: 6667802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052224.D
Acq On : 08 Dec 2022 02:52
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

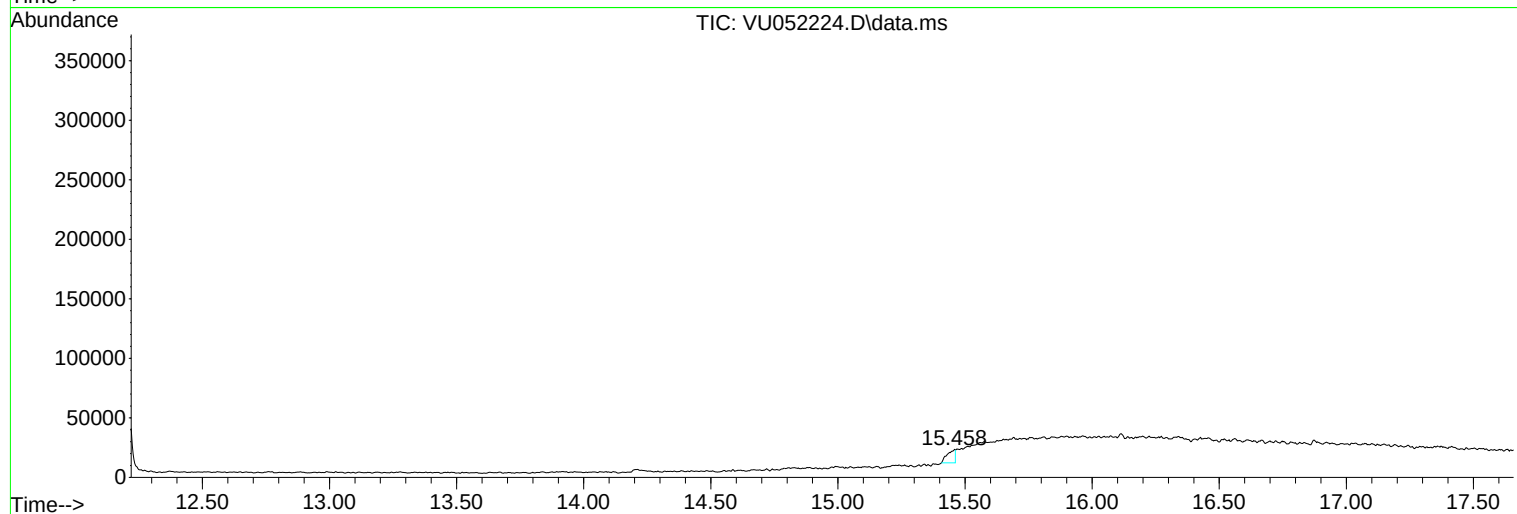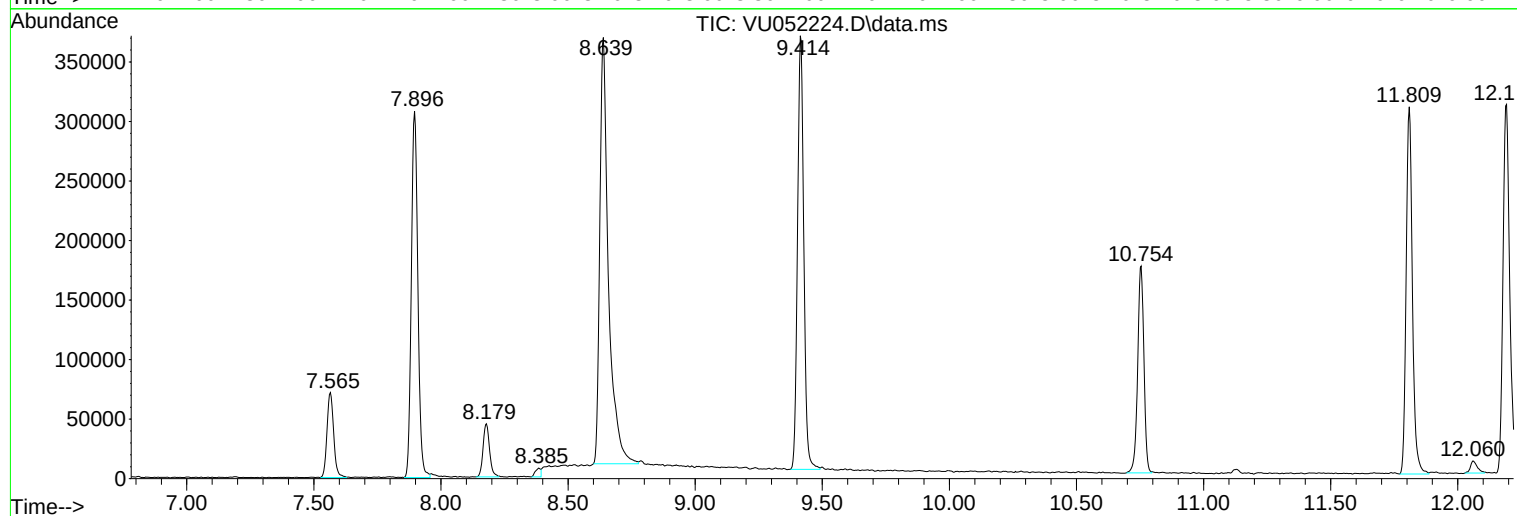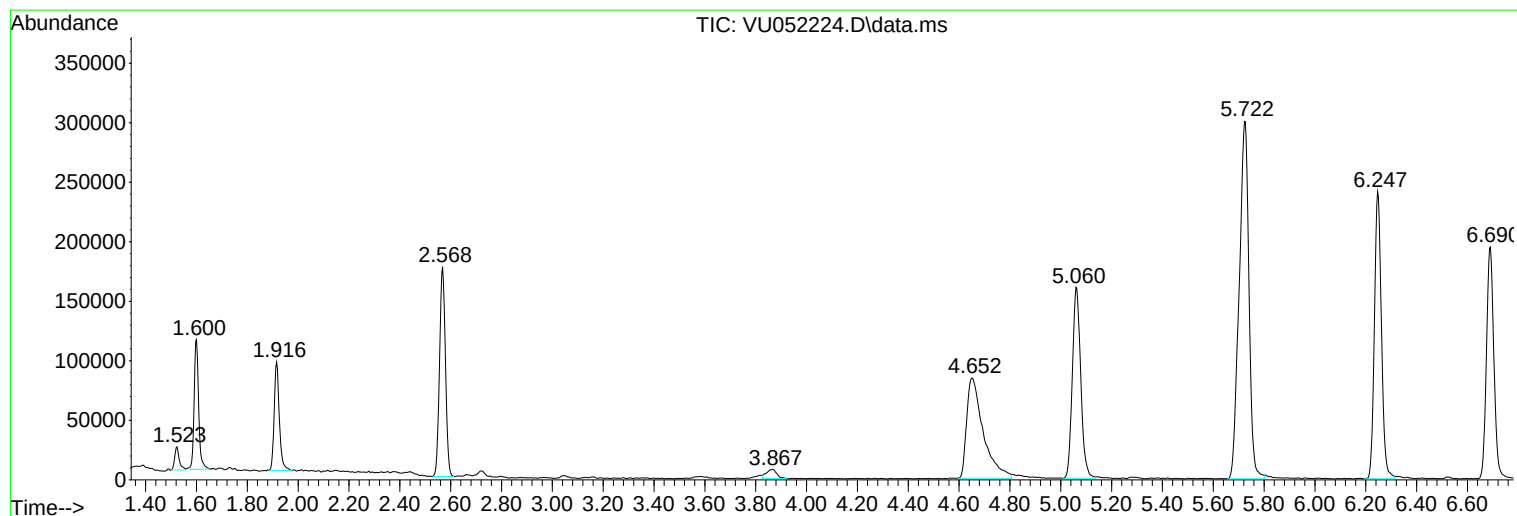

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052224.D
Acq On : 08 Dec 2022 02:52
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052224.D
Acq On : 08 Dec 2022 02:52
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc