


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120722\
Data File : VU052191.D
Acq On : 07 Dec 2022 10:02
Operator : JC/MD
Sample : BFB174
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB174

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 08 04:19:43 2022

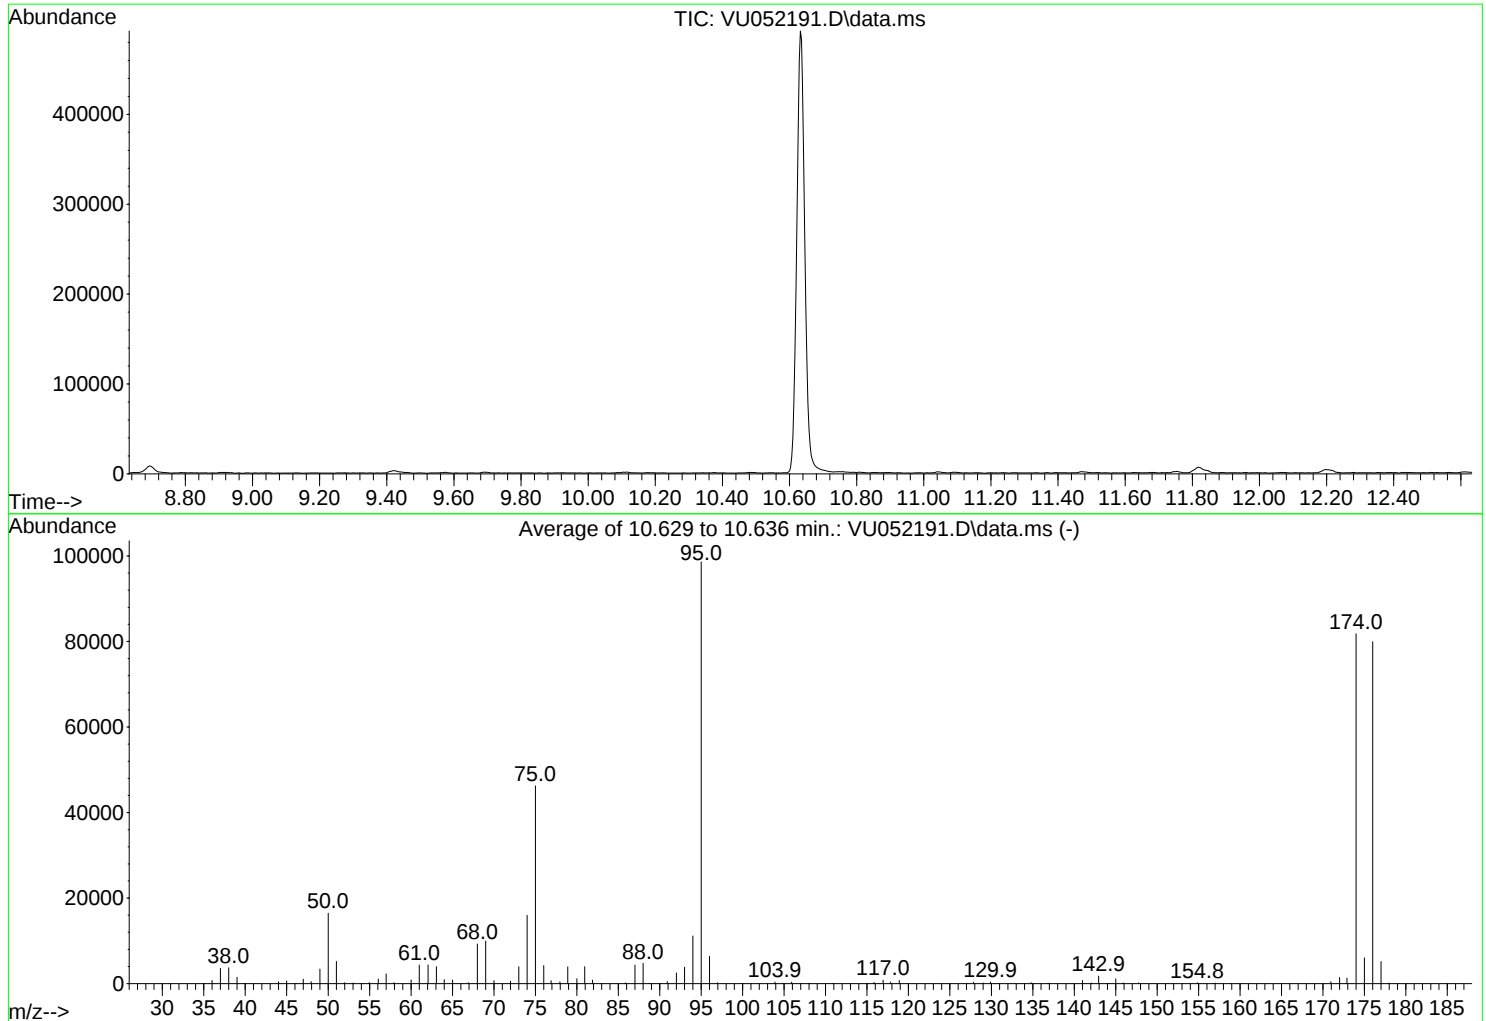

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	16445	PASS
75	95	30	80	46.9	46243	PASS
95	95	100	100	100.0	98616	PASS
96	95	5	9	6.5	6407	PASS
173	174	0.00	2	1.6	1315	PASS
174	95	50	120	83.0	81821	PASS
175	174	5	9	7.4	6018	PASS
176	174	95	101	97.7	79939	PASS
177	176	5	9	6.5	5174	PASS

m/z	Abundance
39.90	363.0
44.00	882.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	732.0
37.00	3428.0
38.00	3811.0
39.00	1510.0
40.00	411.0
44.00	1233.0
45.00	648.0
46.00	141.0
47.00	982.0
48.00	469.0
49.00	3371.0
50.00	15918.0
51.00	4909.0
52.00	196.0
54.00	115.0
54.90	251.0
56.00	1174.0
57.00	2119.0
58.00	194.0
60.00	915.0
61.00	4310.0
62.10	4261.0
63.10	3623.0
64.00	847.0
65.00	837.0
66.90	235.0
68.00	9218.0
69.00	9637.0
70.00	695.0
72.00	578.0
73.00	3952.0
74.00	15391.0
75.00	45240.0
76.00	4202.0
76.90	672.0
78.00	408.0
78.90	3929.0
80.00	1176.0
81.00	3929.0
81.90	784.0
85.80	250.0
87.00	4071.0
88.00	4480.0
90.90	479.0
92.00	2548.0
93.00	3744.0
94.00	10691.0
95.00	94536.0
96.00	6055.0
96.90	261.0
103.90	380.0
104.90	156.0
105.90	317.0
110.80	119.0
115.90	344.0
116.90	790.0
117.90	344.0
118.90	717.0
127.80	285.0
129.00	105.0
129.90	379.0
130.90	109.0
134.80	224.0
136.80	118.0
141.00	729.0
142.10	114.0
143.00	1636.0
144.10	130.0
145.00	1024.0
145.90	192.0
147.80	211.0
154.80	230.0
156.80	174.0
171.00	378.0
172.00	1204.0
172.90	1310.0
174.00	77064.0
175.00	5862.0
176.00	76392.0
177.00	4949.0
178.00	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	753.0
37.00	3717.0
38.00	3781.0
39.00	1547.0
40.00	411.0
44.00	1358.0
45.00	658.0
46.20	120.0
47.00	1061.0
48.00	505.0
49.00	3487.0
50.00	16992.0
51.00	5313.0
52.00	217.0
53.00	167.0
54.90	261.0
56.00	1123.0
57.00	2354.0
57.90	237.0
60.00	906.0
61.00	4478.0
62.10	4483.0
63.00	4104.0
64.00	986.0
65.00	874.0
66.90	235.0
68.00	9569.0
69.00	10399.0
70.00	702.0
72.00	610.0
73.00	4083.0
74.00	16576.0
75.00	47376.0
76.00	4384.0
76.90	693.0
77.90	441.0
78.90	4002.0
80.00	1218.0
81.00	4072.0
81.90	853.0
85.90	190.0
87.00	4450.0
88.00	4906.0
88.70	223.0
90.90	532.0
92.00	2600.0
93.00	3939.0
94.00	11482.0
95.00	101552.0
96.00	6600.0
97.00	226.0
103.90	398.0
104.90	129.0
105.90	363.0
107.90	134.0
110.80	126.0
115.90	316.0
117.00	853.0
117.80	376.0
118.90	796.0
127.90	356.0
129.00	166.0
129.90	392.0
134.80	235.0
136.90	117.0
141.00	735.0
142.10	163.0
143.00	1816.0
145.00	1168.0
145.90	193.0
147.70	221.0
154.80	227.0
157.00	168.0
170.90	456.0
172.00	1451.0
172.90	1388.0
174.00	84168.0
175.00	6178.0
176.00	82288.0
177.00	5347.0
178.00	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174

m/z	Abundance
36.00	754.0
37.00	3576.0
38.00	3534.0
39.00	1485.0
40.00	361.0
44.00	1304.0
45.00	580.0
47.00	1118.0
47.90	484.0
49.00	3321.0
50.00	16424.0
51.00	5416.0
51.90	250.0
53.00	250.0
55.00	238.0
56.10	988.0
57.00	2374.0
57.90	230.0
60.00	782.0
61.00	4219.0
62.00	4422.0
63.00	4147.0
64.00	978.0
65.00	860.0
66.10	117.0
66.90	210.0
68.00	9063.0
69.00	9802.0
70.00	702.0
72.00	531.0
73.00	3839.0
74.00	15924.0
75.00	46112.0
76.00	4096.0
76.90	641.0
77.90	417.0
78.90	3881.0
80.00	1116.0
80.90	3954.0
81.90	799.0
82.90	109.0
85.90	106.0
87.00	4457.0
88.00	4854.0
90.90	455.0
92.00	2379.0
93.00	3925.0
94.00	11237.0
95.00	99760.0
96.00	6566.0
97.00	176.0
103.90	364.0
104.80	114.0
105.90	392.0
107.00	160.0
108.00	152.0
115.00	107.0
115.80	249.0
117.00	841.0
117.80	389.0
118.90	694.0
127.90	394.0
129.00	213.0
129.90	344.0
134.80	232.0
136.90	145.0
141.00	755.0
142.10	155.0
142.90	1812.0
145.00	1159.0
145.90	161.0
147.70	170.0
154.90	237.0
157.00	132.0
158.90	130.0
170.90	475.0
172.00	1565.0
172.90	1248.0
174.00	84232.0
175.00	6013.0
176.00	81136.0
177.00	5225.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB174