


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120820\
 Data File : VU041493.D
 Acq On : 08 Dec 2020 09:21
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB203

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUSIM120820.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Dec 10 02:42:14 2020

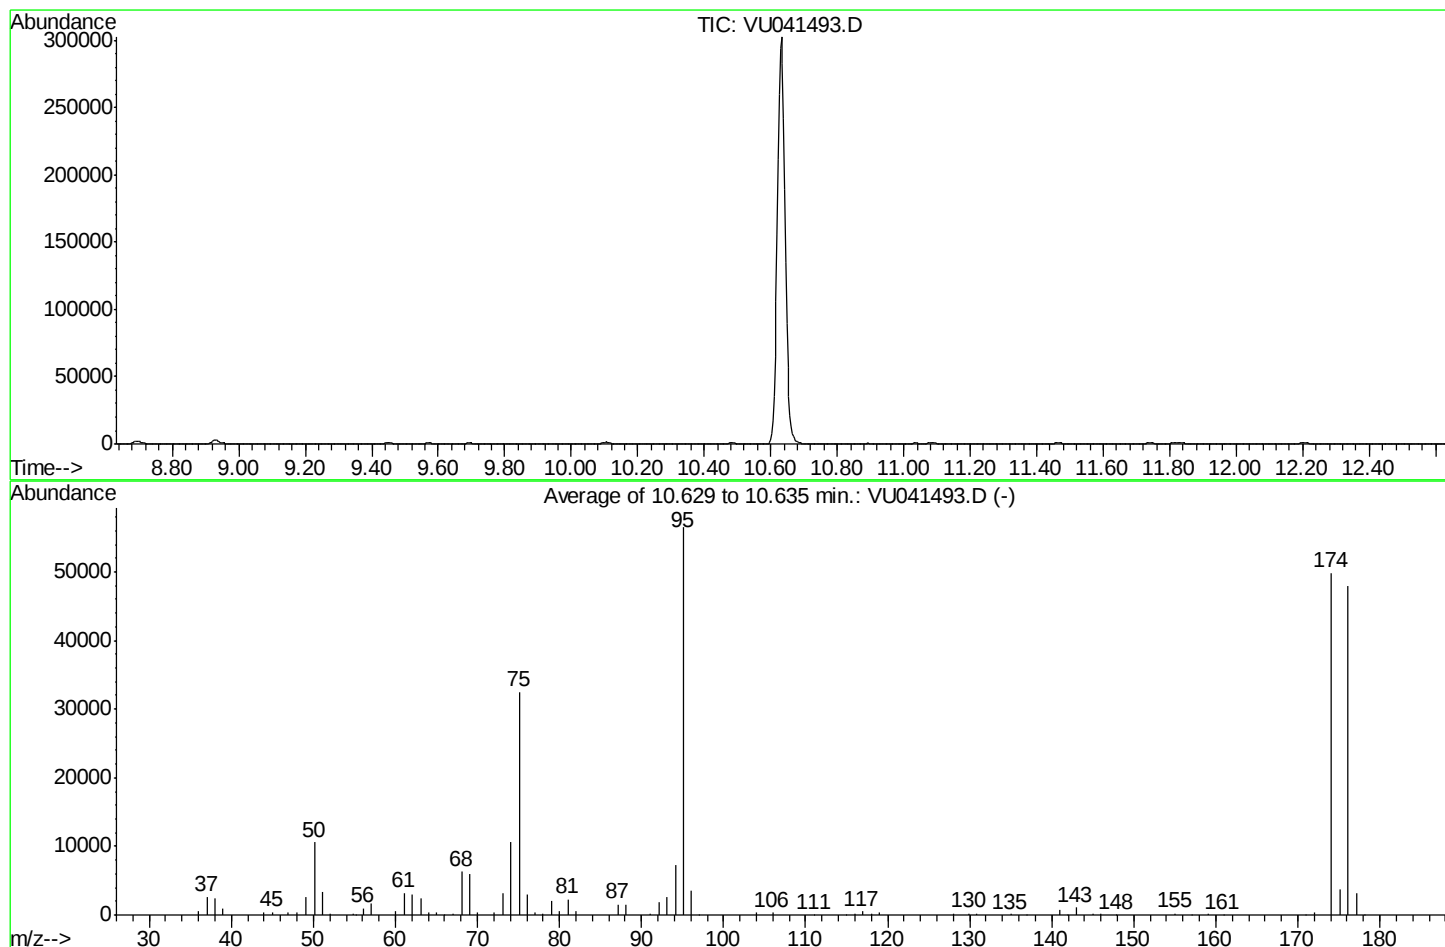

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	10619	PASS
75	95	30	80	57.6	32546	PASS
95	95	100	100	100.0	56490	PASS
96	95	5	9	6.2	3498	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	49877	PASS
175	174	5	9	7.4	3700	PASS
176	174	95	101	96.0	47858	PASS
177	176	5	9	6.6	3179	PASS

m/z	Abundance
36.00	544.0
37.00	2812.0
38.10	2536.0
39.00	937.0
44.00	458.0
45.00	450.0
46.90	329.0
48.00	432.0
49.00	2663.0
50.10	11002.0
51.00	3501.0
52.00	190.0
54.90	200.0
56.00	950.0
57.00	1622.0
60.00	576.0
61.10	3414.0
62.10	3115.0
63.10	2539.0
64.00	327.0
65.00	404.0
67.10	191.0
68.10	6485.0
69.10	5943.0
70.00	431.0
72.00	393.0
73.10	3200.0
74.10	10629.0
75.10	32960.0
76.10	2929.0
77.00	306.0
77.90	204.0
79.00	2113.0
79.90	619.0
81.00	2171.0
82.00	494.0
87.10	1597.0
88.10	1669.0
91.00	262.0
92.10	1959.0
93.10	2721.0
94.10	7314.0
95.10	57096.0
96.10	3551.0
104.00	337.0
106.00	335.0
115.90	219.0
117.00	506.0
118.00	236.0
119.00	368.0
128.00	239.0
129.90	210.0
130.70	107.0
135.10	128.0
141.00	819.0
143.00	1028.0
145.00	239.0
145.90	113.0
147.90	142.0
155.10	183.0
157.10	117.0
159.10	109.0
161.00	100.0
172.10	464.0
174.10	49016.0
175.10	3740.0
176.10	47408.0
177.10	3074.0
178.10	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

m/z	Abundance
36.00	598.0
37.00	2773.0
38.00	2568.0
39.00	1031.0
44.00	404.0
45.00	462.0
46.90	362.0
48.00	393.0
49.00	2768.0
50.10	10908.0
51.00	3481.0
52.00	186.0
54.90	161.0
56.10	976.0
57.00	1673.0
60.00	593.0
61.10	3396.0
62.10	3131.0
63.10	2603.0
64.10	343.0
65.00	406.0
66.00	113.0
67.10	190.0
68.10	6526.0
69.10	6187.0
70.10	439.0
72.10	424.0
73.10	3204.0
74.10	10869.0
75.10	33568.0
76.10	3041.0
77.00	291.0
77.90	196.0
79.00	2119.0
79.90	608.0
81.00	2374.0
82.00	492.0
87.10	1609.0
88.10	1673.0
91.10	261.0
92.10	1962.0
93.10	2787.0
94.10	7461.0
95.10	58336.0
96.10	3607.0
97.00	104.0
104.00	334.0
106.00	380.0
111.10	120.0
114.90	107.0
115.90	212.0
116.90	545.0
118.00	285.0
119.00	380.0
128.00	221.0
130.00	240.0
130.80	113.0
135.00	144.0
141.00	835.0
141.90	107.0
143.00	1103.0
145.00	233.0
146.00	122.0
147.90	115.0
155.00	206.0
157.00	112.0
159.00	120.0
160.90	108.0
170.90	102.0
172.10	451.0
174.10	51352.0
175.10	3829.0
176.10	49368.0
177.10	3280.0
178.10	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

m/z	Abundance
36.00	539.0
37.00	2459.0
38.00	2349.0
39.00	995.0
44.00	346.0
45.00	451.0
46.90	351.0
47.90	334.0
49.10	2558.0
50.10	9948.0
51.10	3170.0
52.00	156.0
55.10	116.0
56.10	916.0
57.00	1656.0
60.00	601.0
61.10	2934.0
62.10	2973.0
63.10	2415.0
64.00	351.0
65.00	363.0
67.10	206.0
68.10	5810.0
69.10	5982.0
70.10	421.0
72.10	367.0
73.10	2891.0
74.10	10372.0
75.10	31112.0
76.10	2961.0
77.00	267.0
79.00	1969.0
80.00	563.0
81.00	2361.0
82.00	449.0
87.10	1558.0
88.10	1414.0
91.20	272.0
92.10	1743.0
93.10	2553.0
94.10	6912.0
95.10	54040.0
96.10	3338.0
97.00	101.0
104.00	332.0
106.00	375.0
111.10	109.0
114.90	100.0
116.00	232.0
117.00	483.0
118.00	278.0
119.00	383.0
128.00	180.0
130.00	278.0
130.90	112.0
135.00	121.0
137.00	125.0
141.00	823.0
141.90	132.0
143.00	1068.0
145.00	233.0
146.10	131.0
155.00	186.0
159.00	113.0
172.00	410.0
174.10	49264.0
175.10	3533.0
176.10	46800.0
177.10	3184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

m/z

Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB203