

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046175.D
 Acq On : 08 Dec 2021 15:05
 Operator : SY/MD
 Sample : VIBLK007
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	90375	100823	11.90%	1.491%
2	1.919	172	180	195	rVB	76510	96978	11.45%	1.434%
3	2.572	371	383	409	rBV	164598	278474	32.87%	4.118%
4	3.051	519	532	540	rBV4	1996	3885	0.46%	0.057%
5	3.109	545	550	557	rBV2	422	587	0.07%	0.009%
6	3.395	635	639	640	rBV2	424	296	0.03%	0.004%
7	3.543	677	685	687	rBV	304	420	0.05%	0.006%
8	3.623	707	710	711	rBV	256	138	0.02%	0.002%
9	3.691	727	731	734	rBV	283	267	0.03%	0.004%
10	3.848	777	780	785	rBV	380	347	0.04%	0.005%
11	4.009	828	830	832	rBV	243	143	0.02%	0.002%
12	4.041	837	840	845	rVB2	639	531	0.06%	0.008%
13	4.080	849	852	855	rVB	253	152	0.02%	0.002%
14	4.160	874	877	880	rBV2	312	223	0.03%	0.003%
15	4.269	908	911	915	rBV2	341	337	0.04%	0.005%
16	4.478	974	976	981	rVB2	290	224	0.03%	0.003%
17	4.504	982	984	988	rBV2	214	202	0.02%	0.003%
18	4.562	999	1002	1005	rBV	307	195	0.02%	0.003%
19	4.639	1011	1026	1062	rBV2	65317	194695	22.98%	2.879%
20	4.999	1134	1138	1143	rBV	423	344	0.04%	0.005%
21	5.067	1143	1159	1180	rBV	146331	334332	39.47%	4.944%
22	5.289	1225	1228	1233	rVB3	382	290	0.03%	0.004%
23	5.366	1248	1252	1257	rBV2	306	290	0.03%	0.004%
24	5.623	1328	1332	1335	rBV2	364	253	0.03%	0.004%
25	5.729	1342	1365	1386	rBV2	314732	847083	100.00%	12.526%
26	6.063	1467	1469	1471	rBV	277	162	0.02%	0.002%
27	6.112	1481	1484	1490	rBV3	446	322	0.04%	0.005%
28	6.250	1514	1527	1545	rBV	296072	551871	65.15%	8.160%
29	6.533	1605	1615	1626	rBV3	5421	10608	1.25%	0.157%
30	6.610	1636	1639	1643	rBV	411	318	0.04%	0.005%
31	6.633	1643	1646	1650	rBV2	315	209	0.02%	0.003%
32	6.694	1650	1665	1681	rBV	196931	381660	45.06%	5.644%
33	6.842	1708	1711	1713	rBV	383	270	0.03%	0.004%
34	6.941	1737	1742	1746	rBV2	389	454	0.05%	0.007%
35	6.989	1752	1757	1761	rVB2	169	182	0.02%	0.003%
36	7.015	1761	1765	1768	rBV	330	231	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046175.D
 Acq On : 08 Dec 2021 15:05
 Operator : SY/MD
 Sample : VIBLK007
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.047	1768	1775	1780	rBV3	369	580	0.07%	0.009%
38	7.105	1791	1793	1796	rBB	256	139	0.02%	0.002%
39	7.125	1796	1799	1801	rVB	217	129	0.02%	0.002%
40	7.182	1809	1817	1827	rBV3	2401	4191	0.49%	0.062%
41	7.288	1846	1850	1851	rBV	180	124	0.01%	0.002%
42	7.375	1873	1877	1879	rBV2	265	219	0.03%	0.003%
43	7.411	1885	1888	1891	rBV	209	153	0.02%	0.002%
44	7.449	1895	1900	1901	rBV	276	224	0.03%	0.003%
45	7.568	1923	1937	1952	rBV	86399	148361	17.51%	2.194%
46	7.684	1968	1973	1987	rVB2	1534	2578	0.30%	0.038%
47	7.739	1987	1990	1995	rVB	423	272	0.03%	0.004%
48	7.790	2001	2006	2012	rBV3	298	378	0.04%	0.006%
49	7.842	2018	2022	2026	rBV	314	259	0.03%	0.004%
50	7.899	2026	2040	2057	rBV	390567	687194	81.12%	10.161%
51	8.089	2096	2099	2101	rBV2	294	140	0.02%	0.002%
52	8.179	2116	2127	2146	rBV	59964	98400	11.62%	1.455%
53	8.372	2184	2187	2189	rBV2	225	143	0.02%	0.002%
54	8.475	2218	2219	2227	rBV3	214	195	0.02%	0.003%
55	8.552	2237	2243	2249	rBV5	1538	2286	0.27%	0.034%
56	8.632	2256	2268	2302	rBV	249247	456524	53.89%	6.751%
57	8.835	2328	2331	2336	rBV2	384	268	0.03%	0.004%
58	8.874	2340	2343	2344	rBV	240	152	0.02%	0.002%
59	8.948	2363	2366	2371	rBV	235	172	0.02%	0.003%
60	9.153	2428	2430	2433	rBV2	269	193	0.02%	0.003%
61	9.195	2440	2443	2445	rBV	249	170	0.02%	0.003%
62	9.240	2452	2457	2459	rBV2	263	236	0.03%	0.003%
63	9.417	2499	2512	2536	rBV	408687	686234	81.01%	10.147%
64	9.575	2558	2561	2570	rVV2	484	569	0.07%	0.008%
65	9.613	2570	2573	2578	rVB	439	366	0.04%	0.005%
66	9.645	2578	2583	2586	rBV2	235	291	0.03%	0.004%
67	9.694	2592	2598	2608	rBV2	752	1144	0.14%	0.017%
68	9.854	2645	2648	2654	rBV2	315	301	0.04%	0.004%
69	9.928	2664	2671	2677	rBV2	327	498	0.06%	0.007%
70	9.960	2677	2681	2683	rBV	222	190	0.02%	0.003%
71	10.092	2718	2722	2723	rBV2	227	159	0.02%	0.002%
72	10.208	2754	2758	2761	rBV2	288	269	0.03%	0.004%
73	10.324	2788	2794	2797	rBV2	464	527	0.06%	0.008%
74	10.433	2824	2828	2835	rVB2	539	484	0.06%	0.007%
75	10.758	2916	2929	2943	rBV	297372	477684	56.39%	7.063%
76	10.829	2948	2951	2956	rVB2	356	244	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046175.D
 Acq On : 08 Dec 2021 15:05
 Operator : SY/MD
 Sample : VIBLK007
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	10.983	2996	2999	3002	rBV	371	271	0.03%	0.004%
78	11.009	3005	3007	3013	rVB	267	262	0.03%	0.004%
79	11.111	3037	3039	3043	rVB2	468	299	0.04%	0.004%
80	11.369	3115	3119	3123	rVB2	336	325	0.04%	0.005%
81	11.391	3123	3126	3129	rBV2	414	333	0.04%	0.005%
82	11.555	3173	3177	3183	rBV	275	337	0.04%	0.005%
83	11.710	3223	3225	3229	rVB2	524	297	0.04%	0.004%
84	11.812	3245	3257	3275	rVB	445091	701945	82.87%	10.379%
85	11.880	3276	3278	3284	rBV2	231	230	0.03%	0.003%
86	12.150	3357	3362	3363	rBV2	401	309	0.04%	0.005%
87	12.192	3363	3375	3392	rVB	413336	669007	78.98%	9.892%
88	12.327	3410	3417	3423	rBV3	1522	1892	0.22%	0.028%
89	12.427	3444	3448	3455	rBV	391	515	0.06%	0.008%
90	12.500	3467	3471	3480	rVB2	265	426	0.05%	0.006%
91	12.623	3506	3509	3513	rBV2	216	142	0.02%	0.002%
92	12.755	3547	3550	3556	rBV2	261	294	0.03%	0.004%
93	12.861	3581	3583	3587	rBV3	240	167	0.02%	0.002%
94	13.012	3628	3630	3634	rVB	223	157	0.02%	0.002%
95	13.037	3634	3638	3639	rBV	299	196	0.02%	0.003%
96	13.150	3669	3673	3676	rBV	440	305	0.04%	0.005%
97	13.433	3755	3761	3768	rVB5	1464	1724	0.20%	0.025%
98	14.092	3959	3966	3969	rBV2	1061	1358	0.16%	0.020%
99	14.870	4199	4208	4211	rBV3	824	1169	0.14%	0.017%
100	14.992	4242	4246	4249	rBV2	430	419	0.05%	0.006%




Sum of corrected areas: 6762815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046175.D
Acq On : 08 Dec 2021 15:05
Operator : SY/MD
Sample : VIBLK007
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

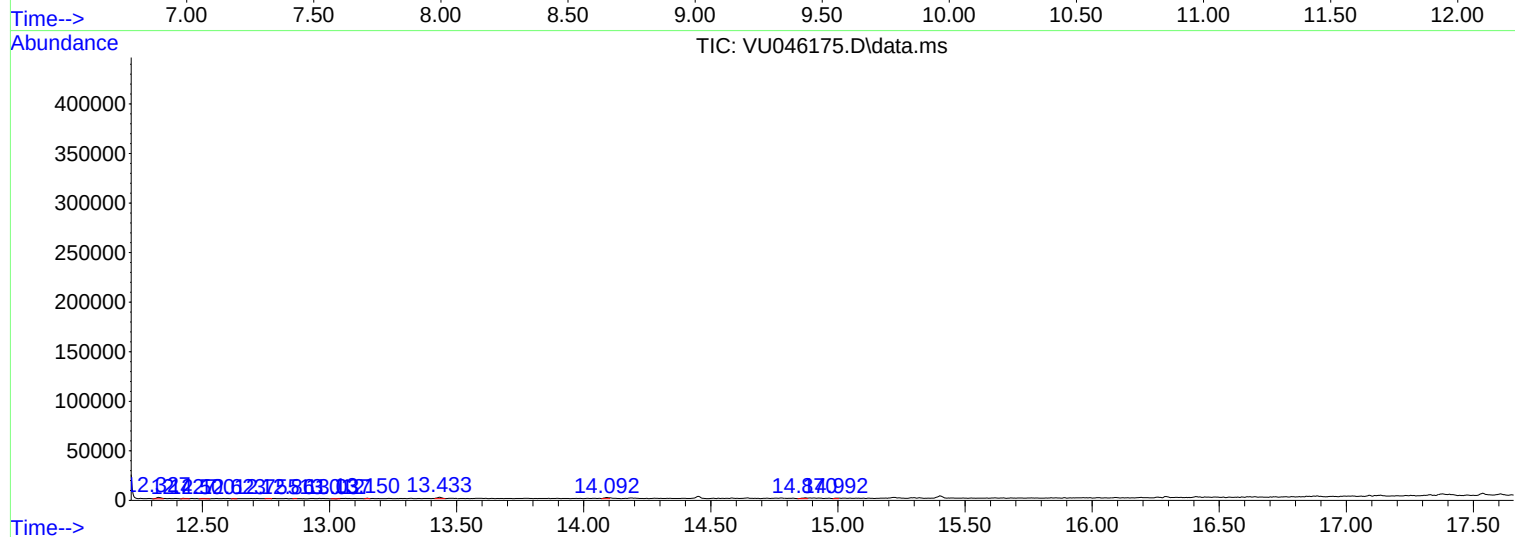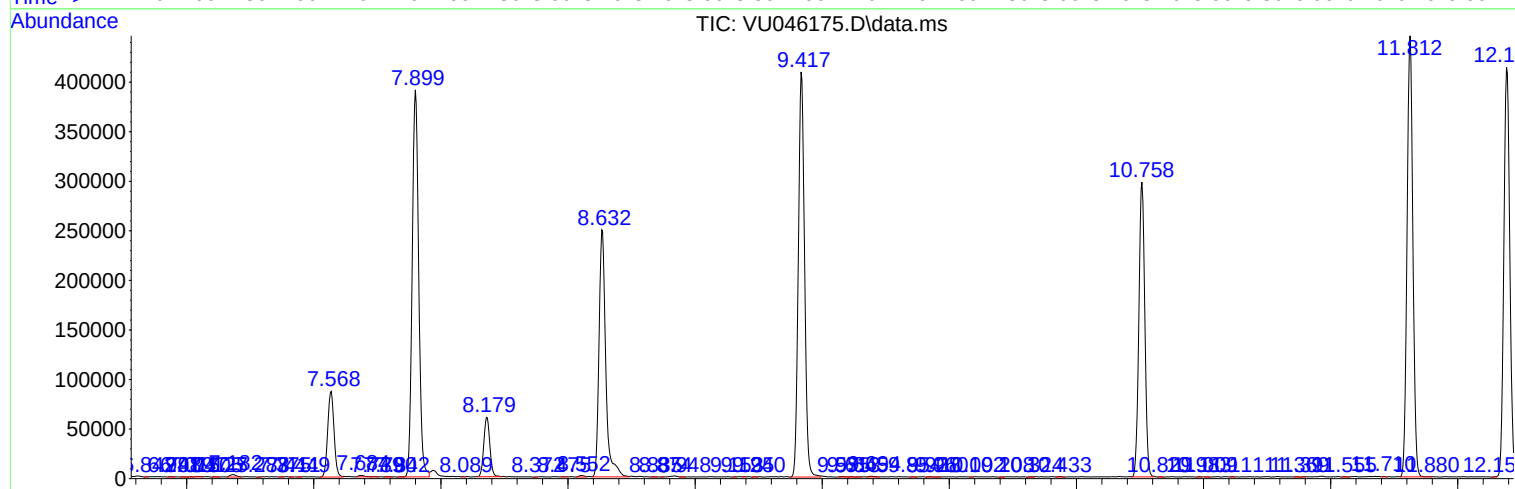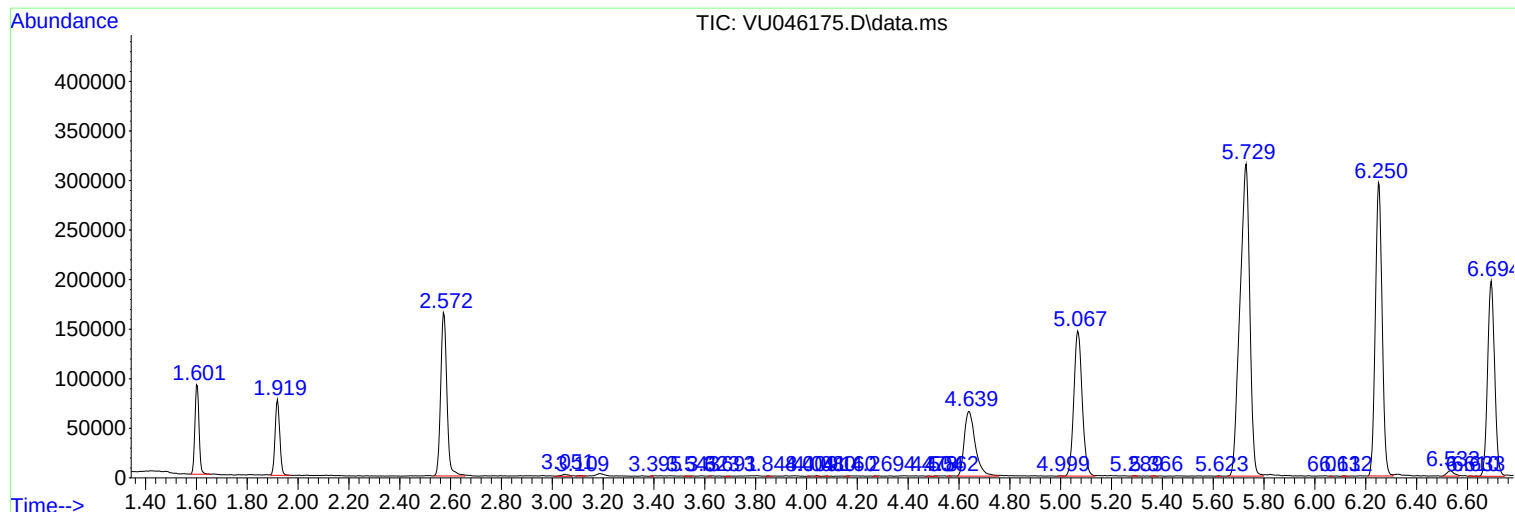

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046175.D
Acq On : 08 Dec 2021 15:05
Operator : SY/MD
Sample : VIBLK007
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046175.D
Acq On : 08 Dec 2021 15:05
Operator : SY/MD
Sample : VIBLK007
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------