

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046188.D
 Acq On : 08 Dec 2021 20:21
 Operator : SY/MD
 Sample : M4971-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	98	rVB	84739	95407	12.84%	1.555%
2	1.919	171	180	192	rBV	64152	82968	11.17%	1.352%
3	2.420	331	336	338	rBV	153	137	0.02%	0.002%
4	2.440	338	342	346	rVB2	684	542	0.07%	0.009%
5	2.462	346	349	353	rBV2	367	391	0.05%	0.006%
6	2.572	371	383	399	rBV	144339	242303	32.61%	3.949%
7	3.109	548	550	555	rBV	251	193	0.03%	0.003%
8	3.269	598	600	603	rVB	199	104	0.01%	0.002%
9	3.285	603	605	607	rBV	270	122	0.02%	0.002%
10	3.298	607	609	611	rBV	335	192	0.03%	0.003%
11	3.475	662	664	669	rVB	222	165	0.02%	0.003%
12	3.507	671	674	681	rVB	456	397	0.05%	0.006%
13	3.533	681	682	683	rBV	157	52	0.01%	0.001%
14	3.575	690	695	697	rBV	374	381	0.05%	0.006%
15	3.626	708	711	714	rBV	437	252	0.03%	0.004%
16	3.646	714	717	720	rBV	422	382	0.05%	0.006%
17	3.678	723	727	729	rBV2	510	348	0.05%	0.006%
18	3.710	735	737	742	rBV2	271	244	0.03%	0.004%
19	3.835	772	776	778	rBV	402	294	0.04%	0.005%
20	4.028	830	836	839	rVB	329	232	0.03%	0.004%
21	4.060	839	846	849	rBV	285	326	0.04%	0.005%
22	4.080	849	852	854	rBV	165	108	0.01%	0.002%
23	4.109	858	861	863	rBV	250	149	0.02%	0.002%
24	4.154	873	875	879	rVB2	306	196	0.03%	0.003%
25	4.176	879	882	885	rBV2	291	186	0.03%	0.003%
26	4.199	885	889	890	rBV	406	252	0.03%	0.004%
27	4.273	908	912	913	rBV	308	219	0.03%	0.004%
28	4.314	918	925	928	rBV2	363	363	0.05%	0.006%
29	4.330	928	930	932	rVB	182	63	0.01%	0.001%
30	4.353	932	937	938	rBV	280	240	0.03%	0.004%
31	4.408	952	954	957	rBV	129	79	0.01%	0.001%
32	4.427	957	960	963	rBV	431	281	0.04%	0.005%
33	4.472	971	974	976	rBV	213	140	0.02%	0.002%
34	4.491	976	980	983	rVB	402	281	0.04%	0.005%
35	4.520	983	989	992	rBV2	415	472	0.06%	0.008%
36	4.539	992	995	999	rBV	391	281	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046188.D
 Acq On : 08 Dec 2021 20:21
 Operator : SY/MD
 Sample : M4971-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	4.639	1012	1026	1058	rBV2	74716	216958	29.20%	3.536%
38	5.067	1142	1159	1183	rBV	140283	317846	42.78%	5.180%
39	5.237	1208	1212	1218	rVB3	437	493	0.07%	0.008%
40	5.292	1226	1229	1235	rBV2	597	464	0.06%	0.008%
41	5.362	1248	1251	1255	rBV2	351	232	0.03%	0.004%
42	5.388	1255	1259	1262	rBV3	541	552	0.07%	0.009%
43	5.488	1285	1290	1294	rBV2	477	503	0.07%	0.008%
44	5.539	1302	1306	1312	rBV	407	511	0.07%	0.008%
45	5.623	1330	1332	1334	rBV	238	136	0.02%	0.002%
46	5.729	1343	1365	1389	rBV2	271135	742936	100.00%	12.109%
47	6.025	1452	1457	1458	rBV2	500	385	0.05%	0.006%
48	6.105	1477	1482	1483	rBV	552	416	0.06%	0.007%
49	6.144	1492	1494	1502	rVB	383	448	0.06%	0.007%
50	6.179	1502	1505	1507	rBV	412	272	0.04%	0.004%
51	6.250	1513	1527	1549	rBV	248655	471768	63.50%	7.689%
52	6.430	1580	1583	1585	rBV	312	240	0.03%	0.004%
53	6.633	1641	1646	1648	rBV	396	366	0.05%	0.006%
54	6.694	1651	1665	1684	rVV	168447	324068	43.62%	5.282%
55	6.854	1711	1715	1717	rBV	558	403	0.05%	0.007%
56	7.086	1783	1787	1792	rBV	438	535	0.07%	0.009%
57	7.224	1827	1830	1836	rBV	401	330	0.04%	0.005%
58	7.256	1836	1840	1843	rBV2	296	321	0.04%	0.005%
59	7.346	1862	1868	1871	rBV2	476	520	0.07%	0.008%
60	7.440	1894	1897	1899	rBV	398	235	0.03%	0.004%
61	7.568	1924	1937	1958	rBV	96907	168408	22.67%	2.745%
62	7.899	2027	2040	2054	rBV	339390	592798	79.79%	9.662%
63	8.179	2116	2127	2145	rBV2	64292	110625	14.89%	1.803%
64	8.472	2210	2218	2234	rVB3	6573	11822	1.59%	0.193%
65	8.594	2253	2256	2257	rBV	295	144	0.02%	0.002%
66	8.636	2257	2269	2300	rVV	240494	430114	57.89%	7.010%
67	8.922	2356	2358	2363	rBV	369	273	0.04%	0.004%
68	9.202	2442	2445	2447	rBV	379	280	0.04%	0.005%
69	9.417	2500	2512	2538	rBV	353889	596497	80.29%	9.722%
70	9.947	2673	2677	2679	rBV	343	275	0.04%	0.004%
71	10.674	2898	2903	2909	rVB4	1290	1432	0.19%	0.023%
72	10.758	2915	2929	2945	rBV	261638	420807	56.64%	6.859%
73	10.893	2964	2971	2980	rVB2	8118	11900	1.60%	0.194%
74	11.089	3027	3032	3033	rBV2	645	545	0.07%	0.009%
75	11.812	3244	3257	3273	rVB	413175	645933	86.94%	10.528%
76	12.060	3327	3334	3344	rBV4	4816	9026	1.21%	0.147%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046188.D
Acq On : 08 Dec 2021 20:21
Operator : SY/MD
Sample : M4971-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3D8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	12.192	3364	3375	3395	rVB	379787	611026	82.24%	9.959%
78	12.295	3404	3407	3411	rBV2	539	449	0.06%	0.007%
79	12.642	3511	3515	3519	rBV2	630	590	0.08%	0.010%
80	12.774	3547	3556	3566	rBV2	4819	7819	1.05%	0.127%
81	12.890	3586	3592	3601	rVB3	3562	4017	0.54%	0.065%
82	12.960	3611	3614	3617	rBV	431	387	0.05%	0.006%
83	13.381	3741	3745	3750	rBV2	533	632	0.09%	0.010%




Sum of corrected areas: 6135479

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046188.D
Acq On : 08 Dec 2021 20:21
Operator : SY/MD
Sample : M4971-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

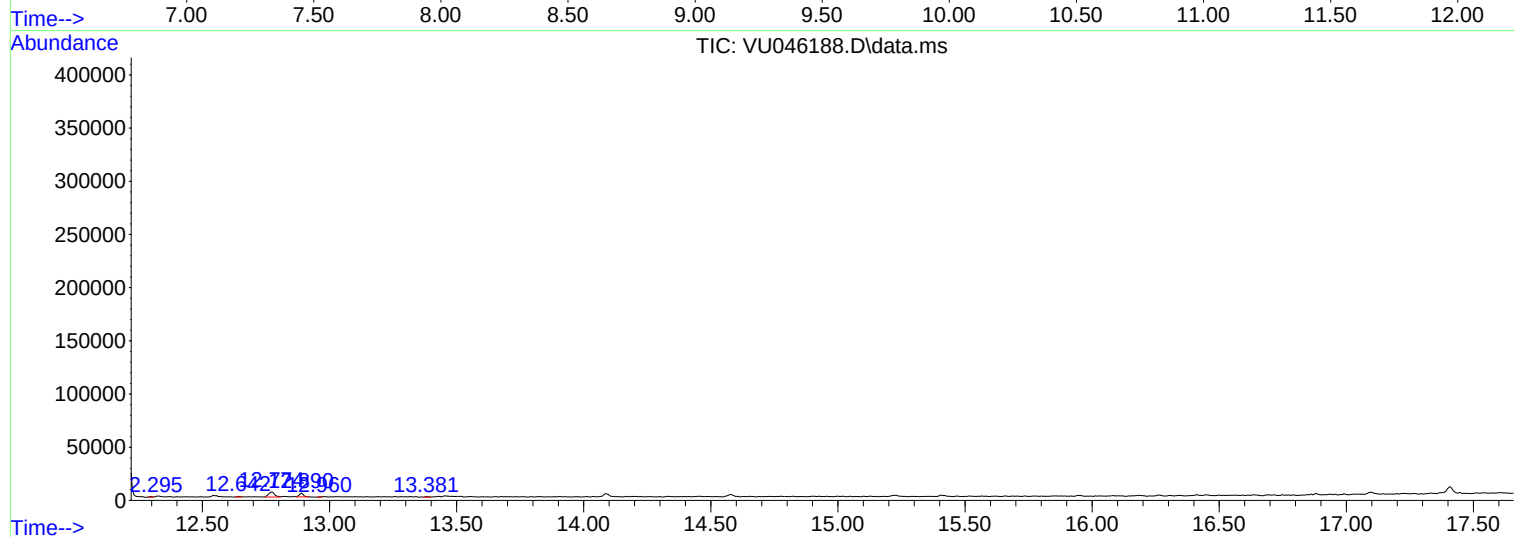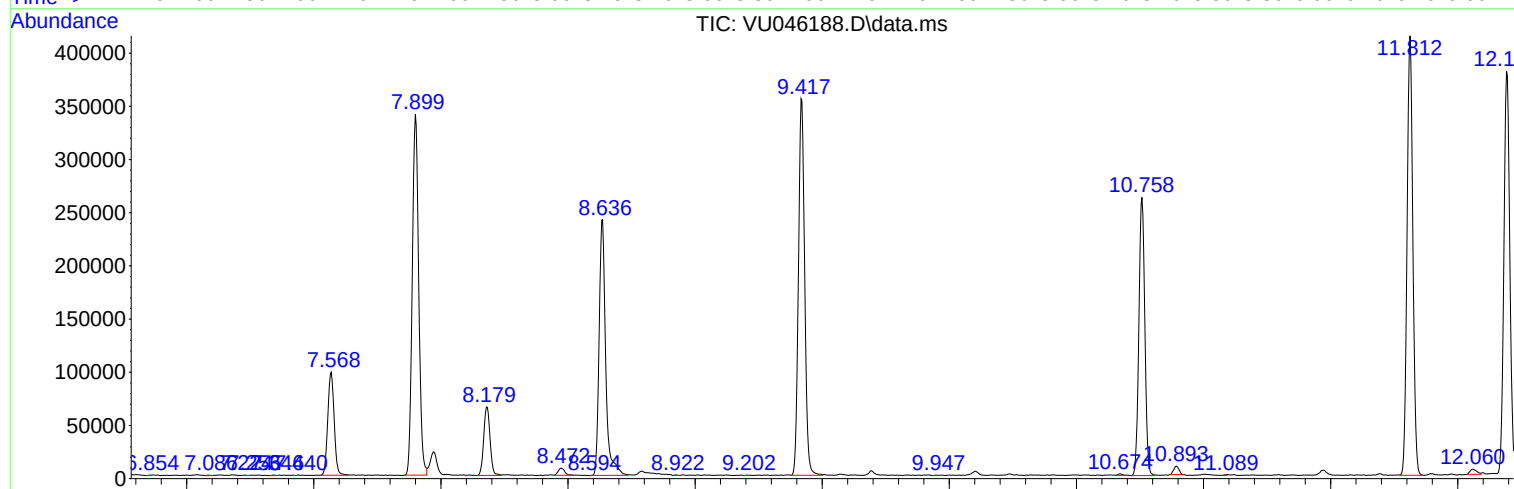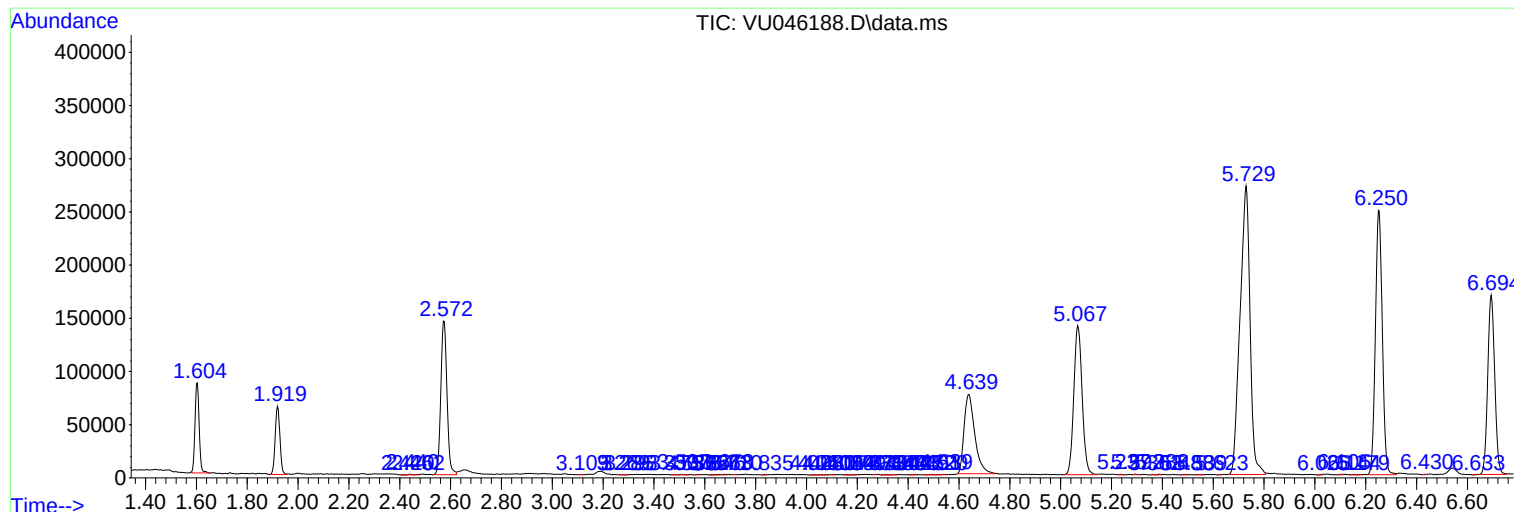

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046188.D
Acq On : 08 Dec 2021 20:21
Operator : SY/MD
Sample : M4971-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046188.D
Acq On : 08 Dec 2021 20:21
Operator : SY/MD
Sample : M4971-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3D8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc