

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046189.D
 Acq On : 08 Dec 2021 20:44
 Operator : SY/MD
 Sample : M4971-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	90	rBV	84737	94900	12.66%	1.507%
2	1.919	171	180	193	rBV	65743	82757	11.04%	1.315%
3	2.253	280	284	287	rBV3	444	336	0.04%	0.005%
4	2.404	327	331	333	rBV2	381	301	0.04%	0.005%
5	2.446	341	344	347	rBV2	526	386	0.05%	0.006%
6	2.572	372	383	398	rBV	144986	242506	32.36%	3.852%
7	3.189	562	575	593	rVB2	6635	14902	1.99%	0.237%
8	3.362	624	629	631	rBV3	464	501	0.07%	0.008%
9	3.469	659	662	666	rVB2	467	354	0.05%	0.006%
10	3.514	673	676	678	rBV	413	300	0.04%	0.005%
11	3.700	730	734	740	rVB2	504	518	0.07%	0.008%
12	3.822	769	772	778	rVB2	423	373	0.05%	0.006%
13	3.864	778	785	786	rBV	438	411	0.05%	0.007%
14	4.002	820	828	834	rBV2	487	760	0.10%	0.012%
15	4.031	835	837	844	rVB2	423	408	0.05%	0.006%
16	4.105	853	860	861	rBV	293	305	0.04%	0.005%
17	4.192	883	887	893	rVV2	355	417	0.06%	0.007%
18	4.231	896	899	903	rVB	575	411	0.05%	0.007%
19	4.256	903	907	911	rBV	471	350	0.05%	0.006%
20	4.639	1009	1026	1062	rVV2	76997	236062	31.50%	3.750%
21	4.806	1075	1078	1084	rBV2	678	632	0.08%	0.010%
22	5.067	1143	1159	1183	rVV2	144035	322930	43.10%	5.130%
23	5.169	1188	1191	1198	rVV	611	766	0.10%	0.012%
24	5.295	1224	1230	1235	rBV3	495	684	0.09%	0.011%
25	5.356	1243	1249	1252	rBV2	521	546	0.07%	0.009%
26	5.443	1269	1276	1282	rBV	534	807	0.11%	0.013%
27	5.520	1295	1300	1302	rBV2	508	411	0.05%	0.007%
28	5.591	1319	1322	1325	rVB	448	313	0.04%	0.005%
29	5.729	1343	1365	1394	rBV2	272444	749317	100.00%	11.903%
30	6.150	1491	1496	1498	rBV2	410	372	0.05%	0.006%
31	6.166	1498	1501	1506	rVB3	422	328	0.04%	0.005%
32	6.253	1513	1528	1546	rBV	245674	466039	62.20%	7.403%
33	6.536	1605	1616	1633	rBV6	5033	11436	1.53%	0.182%
34	6.626	1640	1644	1651	rBV2	588	678	0.09%	0.011%
35	6.694	1651	1665	1683	rBV	171060	331168	44.20%	5.261%
36	6.977	1747	1753	1758	rBV2	422	513	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046189.D
 Acq On : 08 Dec 2021 20:44
 Operator : SY/MD
 Sample : M4971-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.079	1782	1785	1791	rBV	374	362	0.05%	0.006%
38	7.343	1860	1867	1870	rBV2	554	572	0.08%	0.009%
39	7.378	1875	1878	1886	rBV2	406	574	0.08%	0.009%
40	7.411	1886	1888	1895	rVB	524	584	0.08%	0.009%
41	7.443	1895	1898	1902	rBV	330	354	0.05%	0.006%
42	7.568	1923	1937	1961	rBV	96377	169744	22.65%	2.696%
43	7.739	1986	1990	1996	rVB2	512	540	0.07%	0.009%
44	7.793	2002	2007	2009	rBV2	638	513	0.07%	0.008%
45	7.899	2026	2040	2055	rBV	339262	597773	79.78%	9.496%
46	7.970	2056	2062	2076	rVB2	21555	36997	4.94%	0.588%
47	8.179	2115	2127	2142	rBV	66422	111228	14.84%	1.767%
48	8.240	2144	2146	2149	rVV	701	493	0.07%	0.008%
49	8.269	2153	2155	2158	rVV	421	336	0.04%	0.005%
50	8.304	2162	2166	2171	rBV3	508	599	0.08%	0.010%
51	8.472	2210	2218	2231	rVB2	7698	12668	1.69%	0.201%
52	8.526	2231	2235	2238	rBV2	389	319	0.04%	0.005%
53	8.591	2251	2255	2257	rBV2	402	318	0.04%	0.005%
54	8.632	2257	2268	2297	rVV	236527	429109	57.27%	6.816%
55	8.793	2308	2318	2326	rBV6	3747	7698	1.03%	0.122%
56	8.957	2366	2369	2375	rVB	334	305	0.04%	0.005%
57	9.034	2389	2393	2396	rBV2	410	317	0.04%	0.005%
58	9.198	2441	2444	2448	rVV	393	348	0.05%	0.006%
59	9.417	2500	2512	2534	rVV	350688	588320	78.51%	9.346%
60	9.697	2589	2599	2609	rVB	4528	6763	0.90%	0.107%
61	9.890	2656	2659	2664	rBV	373	372	0.05%	0.006%
62	10.102	2713	2725	2735	rVB4	4391	7579	1.01%	0.120%
63	10.147	2735	2739	2744	rBV	413	348	0.05%	0.006%
64	10.240	2760	2768	2773	rBV4	879	1373	0.18%	0.022%
65	10.404	2815	2819	2821	rBV	469	407	0.05%	0.006%
66	10.481	2838	2843	2847	rBV3	518	594	0.08%	0.009%
67	10.568	2867	2870	2876	rVV2	270	319	0.04%	0.005%
68	10.671	2895	2902	2912	rVV3	1453	2020	0.27%	0.032%
69	10.758	2917	2929	2952	rVB	267242	424649	56.67%	6.746%
70	10.893	2958	2971	2986	rBV	10604	17424	2.33%	0.277%
71	11.079	3025	3029	3032	rBV2	878	868	0.12%	0.014%
72	11.127	3040	3044	3048	rBV2	386	368	0.05%	0.006%
73	11.230	3071	3076	3079	rBV	491	426	0.06%	0.007%
74	11.288	3090	3094	3097	rBV2	634	542	0.07%	0.009%
75	11.471	3142	3151	3165	rVB4	5483	9911	1.32%	0.157%
76	11.648	3202	3206	3212	rVB2	509	597	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046189.D
 Acq On : 08 Dec 2021 20:44
 Operator : SY/MD
 Sample : M4971-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.687	3212	3218	3221	rBV4	1384	1456	0.19%	0.023%
78	11.812	3245	3257	3276	rVB	393854	636557	84.95%	10.112%
79	11.889	3276	3281	3282	rBV2	994	781	0.10%	0.012%
80	11.967	3302	3305	3311	rVB2	723	697	0.09%	0.011%
81	12.060	3322	3334	3344	rBV4	5839	10916	1.46%	0.173%
82	12.195	3363	3376	3394	rVB	382667	619037	82.61%	9.833%
83	12.324	3412	3416	3420	rBV	682	675	0.09%	0.011%
84	12.449	3452	3455	3463	rVV2	406	484	0.06%	0.008%
85	12.484	3463	3466	3473	rVB2	349	433	0.06%	0.007%
86	12.545	3480	3485	3493	rVB5	1238	1798	0.24%	0.029%
87	12.774	3549	3556	3565	rVB2	4417	6836	0.91%	0.109%
88	12.889	3585	3592	3602	rBV5	3359	4316	0.58%	0.069%
89	12.947	3607	3610	3614	rBV2	302	312	0.04%	0.005%
90	13.195	3683	3687	3693	rBV	390	451	0.06%	0.007%
91	13.224	3693	3696	3701	rVB	379	319	0.04%	0.005%
92	13.333	3723	3730	3734	rBV2	302	416	0.06%	0.007%
93	13.751	3855	3860	3863	rBV2	560	530	0.07%	0.008%
94	13.915	3906	3911	3914	rBV	469	383	0.05%	0.006%
95	13.938	3914	3918	3922	rBV	432	505	0.07%	0.008%
96	14.086	3956	3964	3976	rVB4	2547	4324	0.58%	0.069%
97	14.205	3993	4001	4008	rBV2	564	1012	0.14%	0.016%
98	14.581	4110	4118	4126	rVB3	1496	2753	0.37%	0.044%
99	15.053	4262	4265	4269	rBV3	347	309	0.04%	0.005%
100	15.217	4312	4316	4319	rBV4	1003	1067	0.14%	0.017%



Sum of corrected areas: 6295196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046189.D
Acq On : 08 Dec 2021 20:44
Operator : SY/MD
Sample : M4971-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

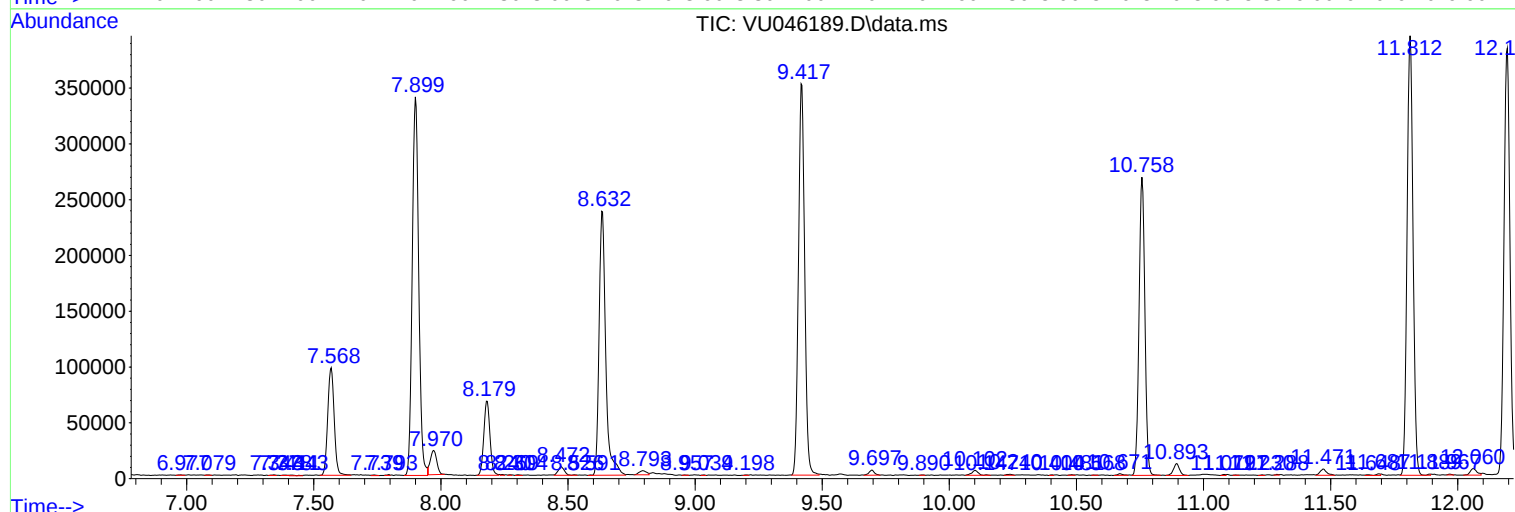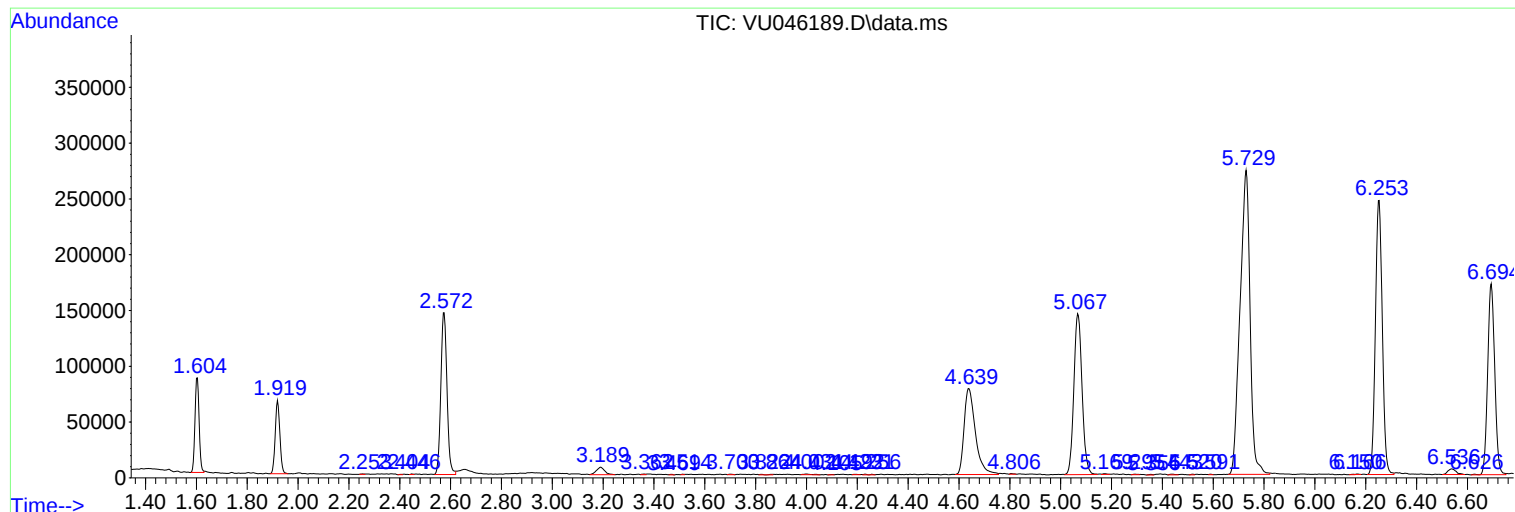

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046189.D
Acq On : 08 Dec 2021 20:44
Operator : SY/MD
Sample : M4971-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046189.D
Acq On : 08 Dec 2021 20:44
Operator : SY/MD
Sample : M4971-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------