

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046190.D
 Acq On : 08 Dec 2021 21:06
 Operator : SY/MD
 Sample : M4983-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	92	rBV	85475	93483	12.72%	1.497%
2	1.919	172	180	193	rVB	64924	82049	11.17%	1.314%
3	2.459	343	348	350	rBV2	546	478	0.07%	0.008%
4	2.572	372	383	409	rBV	144492	241466	32.86%	3.866%
5	2.761	439	442	445	rBV3	377	229	0.03%	0.004%
6	3.044	524	530	533	rBV3	722	914	0.12%	0.015%
7	3.292	604	607	609	rBV	335	197	0.03%	0.003%
8	3.366	627	630	631	rBV	130	61	0.01%	0.001%
9	3.385	631	636	646	rVV2	618	1029	0.14%	0.016%
10	3.449	653	656	659	rBV	444	325	0.04%	0.005%
11	3.748	746	749	751	rBV	372	246	0.03%	0.004%
12	3.800	763	765	769	rVB	325	191	0.03%	0.003%
13	3.822	769	772	777	rBV	373	345	0.05%	0.006%
14	3.864	782	785	788	rBV2	503	340	0.05%	0.005%
15	4.038	836	839	842	rBV	500	391	0.05%	0.006%
16	4.240	899	902	907	rVB2	315	321	0.04%	0.005%
17	4.266	907	910	912	rBV	422	276	0.04%	0.004%
18	4.382	942	946	951	rBV	576	707	0.10%	0.011%
19	4.642	1011	1027	1064	rBV	66963	221379	30.13%	3.544%
20	4.915	1108	1112	1117	rBV2	581	556	0.08%	0.009%
21	4.970	1125	1129	1131	rBV2	335	341	0.05%	0.005%
22	5.067	1145	1159	1180	rVB	129517	292056	39.74%	4.676%
23	5.433	1269	1273	1274	rBV	295	191	0.03%	0.003%
24	5.507	1294	1296	1297	rBV	271	111	0.02%	0.002%
25	5.729	1343	1365	1382	rBV2	271883	734826	100.00%	11.765%
26	6.099	1475	1480	1482	rBV2	486	483	0.07%	0.008%
27	6.250	1514	1527	1547	rBV	264292	500141	68.06%	8.008%
28	6.501	1603	1605	1607	rBV2	360	220	0.03%	0.004%
29	6.536	1607	1616	1632	rVV6	3906	8883	1.21%	0.142%
30	6.694	1651	1665	1687	rBV	169611	328993	44.77%	5.267%
31	6.806	1698	1700	1702	rBV	344	207	0.03%	0.003%
32	6.858	1712	1716	1721	rBV2	516	555	0.08%	0.009%
33	6.880	1721	1723	1726	rVV2	152	101	0.01%	0.002%
34	7.018	1762	1766	1769	rBV	408	326	0.04%	0.005%
35	7.163	1808	1811	1813	rBV	252	137	0.02%	0.002%
36	7.211	1823	1826	1830	rBV2	423	290	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046190.D
 Acq On : 08 Dec 2021 21:06
 Operator : SY/MD
 Sample : M4983-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.234	1830	1833	1834	rBV	187	91	0.01%	0.001%
38	7.282	1846	1848	1853	rBV2	233	284	0.04%	0.005%
39	7.404	1882	1886	1889	rBV	237	220	0.03%	0.004%
40	7.468	1904	1906	1907	rBV	148	62	0.01%	0.001%
41	7.510	1915	1919	1921	rBV2	295	192	0.03%	0.003%
42	7.568	1921	1937	1955	rBV	98531	170689	23.23%	2.733%
43	7.761	1993	1997	2003	rVB	459	354	0.05%	0.006%
44	7.796	2003	2008	2013	rBV3	640	813	0.11%	0.013%
45	7.819	2013	2015	2018	rVB	312	153	0.02%	0.002%
46	7.832	2018	2019	2021	rBV2	153	57	0.01%	0.001%
47	7.899	2026	2040	2057	rBV	341630	595908	81.10%	9.541%
48	8.063	2089	2091	2092	rBV	165	80	0.01%	0.001%
49	8.102	2099	2103	2109	rBV2	365	379	0.05%	0.006%
50	8.131	2109	2112	2113	rBV2	258	150	0.02%	0.002%
51	8.179	2115	2127	2141	rVV2	72258	128117	17.44%	2.051%
52	8.382	2186	2190	2194	rBV	211	171	0.02%	0.003%
53	8.404	2194	2197	2200	rVV	335	212	0.03%	0.003%
54	8.475	2211	2219	2232	rVB2	4291	7907	1.08%	0.127%
55	8.539	2233	2239	2243	rVB2	500	556	0.08%	0.009%
56	8.562	2243	2246	2248	rBV2	408	288	0.04%	0.005%
57	8.636	2256	2269	2301	rBV	241910	437341	59.52%	7.002%
58	8.771	2308	2311	2313	rBV	336	220	0.03%	0.004%
59	8.829	2326	2329	2333	rBV	341	254	0.03%	0.004%
60	8.899	2348	2351	2355	rBV2	328	267	0.04%	0.004%
61	8.989	2370	2379	2383	rVB2	517	543	0.07%	0.009%
62	9.012	2383	2386	2390	rBV2	476	450	0.06%	0.007%
63	9.144	2425	2427	2431	rVB	426	252	0.03%	0.004%
64	9.176	2431	2437	2440	rBV	431	570	0.08%	0.009%
65	9.275	2464	2468	2469	rBV	434	334	0.05%	0.005%
66	9.343	2485	2489	2492	rBV	360	294	0.04%	0.005%
67	9.417	2499	2512	2530	rBV	372740	631415	85.93%	10.109%
68	9.610	2569	2572	2575	rVB2	425	229	0.03%	0.004%
69	9.986	2684	2689	2693	rBV	425	495	0.07%	0.008%
70	10.095	2720	2723	2725	rBV	419	242	0.03%	0.004%
71	10.150	2737	2740	2743	rVB	368	186	0.03%	0.003%
72	10.234	2760	2766	2769	rVB	421	480	0.07%	0.008%
73	10.266	2769	2776	2783	rBV2	491	778	0.11%	0.012%
74	10.414	2819	2822	2827	rBV	430	472	0.06%	0.008%
75	10.555	2863	2866	2872	rBV2	419	482	0.07%	0.008%
76	10.610	2881	2883	2886	rVB	412	222	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046190.D
 Acq On : 08 Dec 2021 21:06
 Operator : SY/MD
 Sample : M4983-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	10.668	2896	2901	2910	rVB4	1686	2625	0.36%	0.042%
78	10.758	2916	2929	2945	rVB	264600	424873	57.82%	6.802%
79	10.835	2951	2953	2958	rBV	241	194	0.03%	0.003%
80	10.893	2962	2971	2984	rVB2	7019	11582	1.58%	0.185%
81	10.960	2989	2992	2994	rBV	287	167	0.02%	0.003%
82	11.108	3036	3038	3039	rBV2	402	177	0.02%	0.003%
83	11.240	3076	3079	3080	rBV	250	136	0.02%	0.002%
84	11.693	3217	3220	3226	rBV3	964	1049	0.14%	0.017%
85	11.812	3245	3257	3271	rBV	438671	685463	93.28%	10.975%
86	12.195	3364	3376	3391	rVB	382097	620320	84.42%	9.932%
87	12.327	3413	3417	3423	rBV4	1517	1589	0.22%	0.025%
88	13.433	3756	3761	3768	rBV6	987	1159	0.16%	0.019%
89	14.192	3991	3997	4003	rVB5	1079	1470	0.20%	0.024%




Sum of corrected areas: 6245857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046190.D
Acq On : 08 Dec 2021 21:06
Operator : SY/MD
Sample : M4983-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

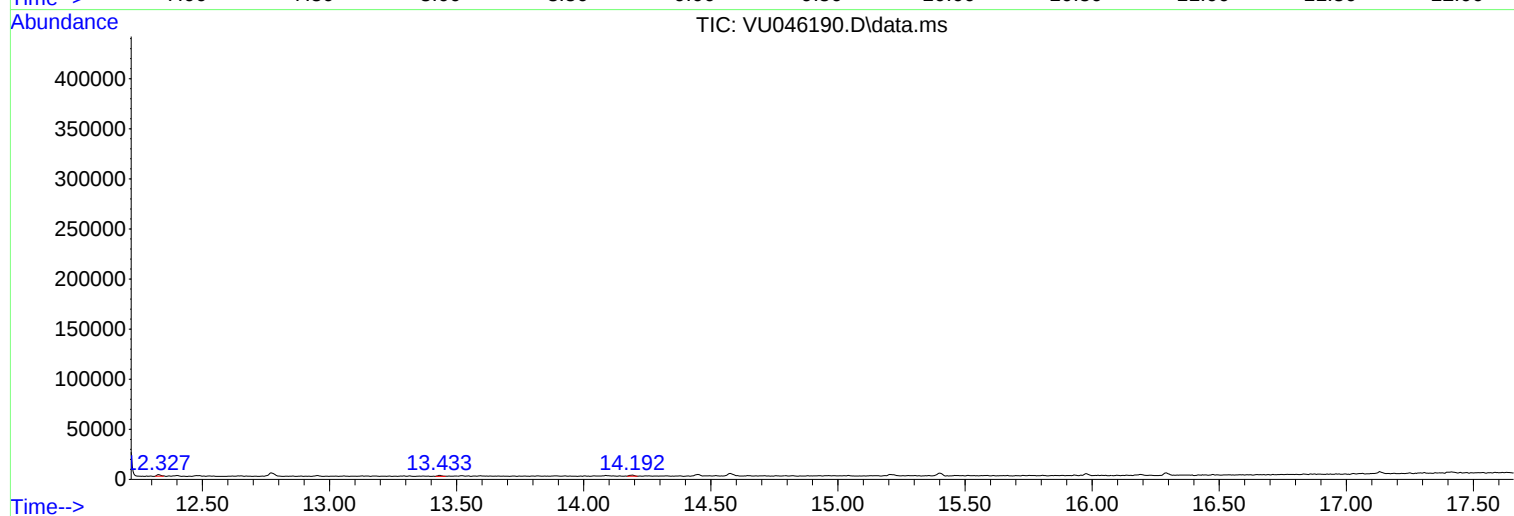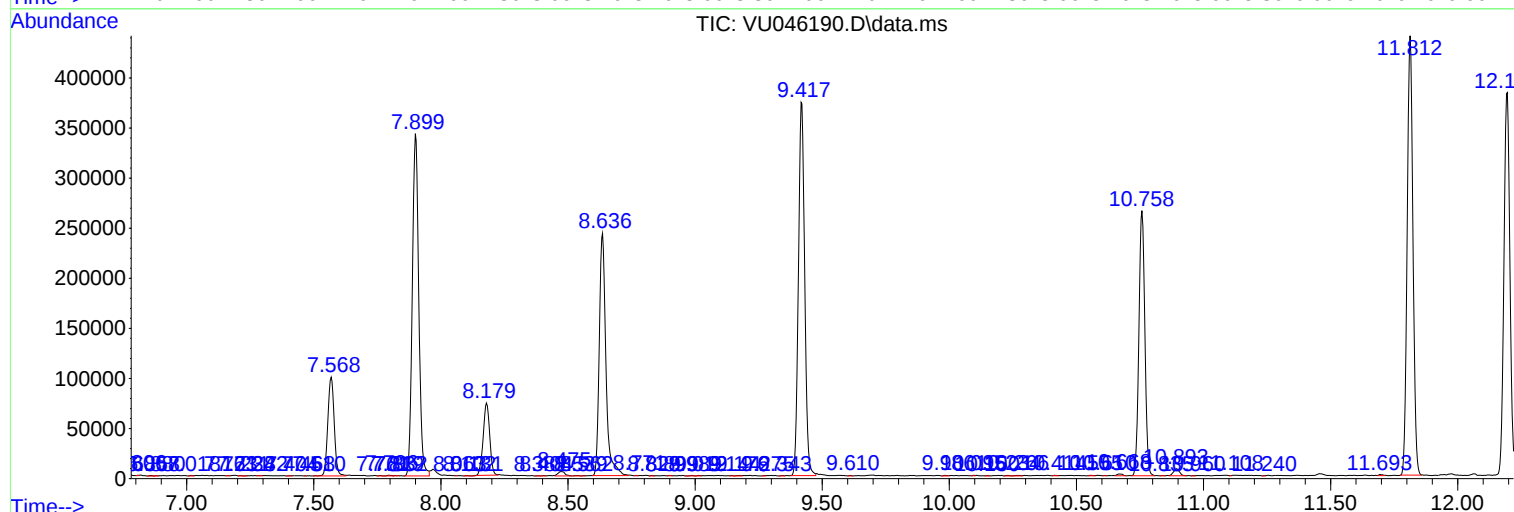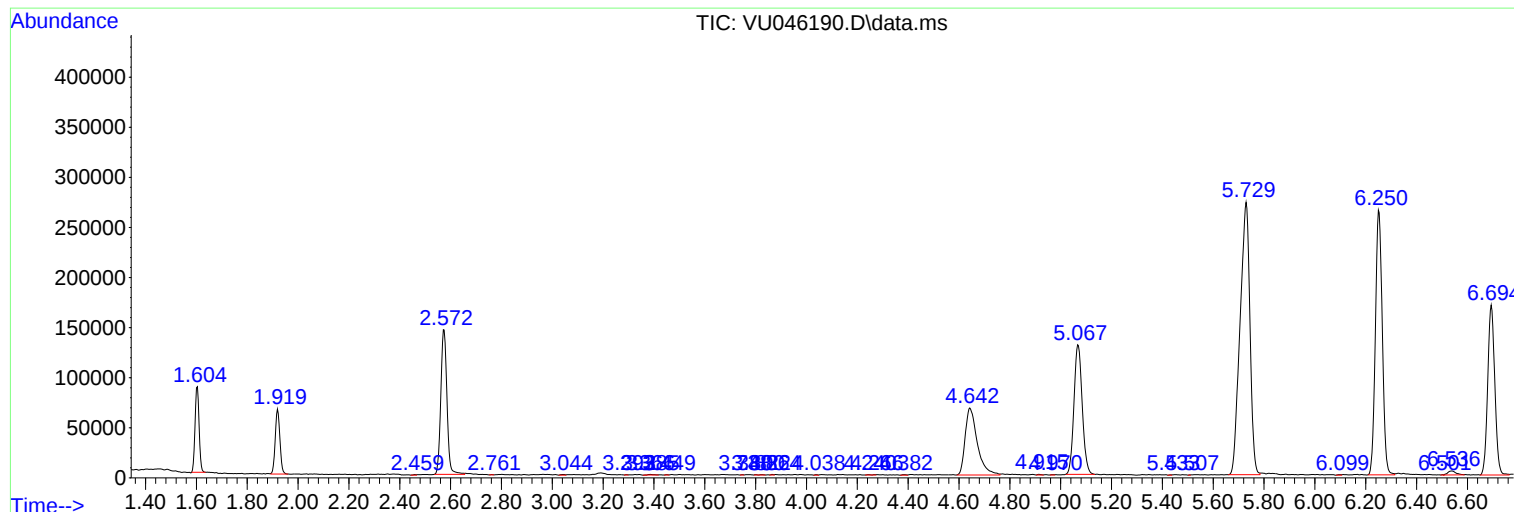

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046190.D
Acq On : 08 Dec 2021 21:06
Operator : SY/MD
Sample : M4983-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046190.D
Acq On : 08 Dec 2021 21:06
Operator : SY/MD
Sample : M4983-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------