

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046194.D
 Acq On : 08 Dec 2021 22:35
 Operator : SY/MD
 Sample : M4983-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	78861	88699	10.27%	1.241%
2	1.919	172	180	191	rVB	62642	79676	9.22%	1.114%
3	2.076	226	229	234	rBV3	532	575	0.07%	0.008%
4	2.147	245	251	257	rVB	1023	1148	0.13%	0.016%
5	2.392	322	327	329	rBV2	543	365	0.04%	0.005%
6	2.575	371	384	403	rBV2	147412	264149	30.57%	3.695%
7	2.826	459	462	467	rBV2	284	260	0.03%	0.004%
8	2.967	502	506	511	rVB2	473	419	0.05%	0.006%
9	3.054	529	533	536	rBV4	421	321	0.04%	0.004%
10	3.083	539	542	546	rBV2	326	337	0.04%	0.005%
11	3.141	556	560	564	rBV2	281	298	0.03%	0.004%
12	3.163	564	567	568	rVV	536	296	0.03%	0.004%
13	3.186	569	574	589	rVB2	1750	3299	0.38%	0.046%
14	3.295	605	608	613	rBV2	309	268	0.03%	0.004%
15	3.366	618	630	637	rBV6	2952	5645	0.65%	0.079%
16	3.536	680	683	689	rVB2	417	468	0.05%	0.007%
17	3.581	693	697	700	rBV2	574	520	0.06%	0.007%
18	3.633	709	713	715	rBV	402	257	0.03%	0.004%
19	3.649	715	718	723	rBV	394	349	0.04%	0.005%
20	3.874	769	788	807	rBV	60572	142991	16.55%	2.000%
21	4.298	918	920	926	rVB2	331	339	0.04%	0.005%
22	4.327	926	929	933	rBV2	377	314	0.04%	0.004%
23	4.639	1011	1026	1059	rVV2	73427	263109	30.45%	3.680%
24	4.858	1091	1094	1097	rVB	501	344	0.04%	0.005%
25	4.967	1124	1128	1131	rBV2	382	381	0.04%	0.005%
26	5.067	1143	1159	1180	rBV	128549	287142	33.23%	4.016%
27	5.321	1220	1238	1262	rBV	382313	864067	100.00%	12.086%
28	5.626	1329	1333	1336	rVV2	399	300	0.03%	0.004%
29	5.729	1343	1365	1386	rBV2	259494	705956	81.70%	9.874%
30	5.986	1443	1445	1450	rVB2	486	357	0.04%	0.005%
31	6.012	1450	1453	1458	rBV2	477	399	0.05%	0.006%
32	6.044	1458	1463	1466	rBV2	379	408	0.05%	0.006%
33	6.166	1497	1501	1503	rBV	416	328	0.04%	0.005%
34	6.202	1508	1512	1513	rBV	429	283	0.03%	0.004%
35	6.250	1514	1527	1543	rBV	243202	453186	52.45%	6.339%
36	6.543	1606	1618	1633	rVB4	15084	29711	3.44%	0.416%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046194.D
 Acq On : 08 Dec 2021 22:35
 Operator : SY/MD
 Sample : M4983-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1680	rBV	166477	316176	36.59%	4.422%
38	6.980	1751	1754	1758	rVV	313	279	0.03%	0.004%
39	7.009	1761	1763	1767	rVV2	369	253	0.03%	0.004%
40	7.038	1769	1772	1779	rVB2	380	380	0.04%	0.005%
41	7.240	1832	1835	1837	rBV2	387	251	0.03%	0.004%
42	7.317	1857	1859	1866	rVB2	777	820	0.09%	0.011%
43	7.359	1866	1872	1875	rBV2	721	987	0.11%	0.014%
44	7.436	1891	1896	1899	rBV2	432	363	0.04%	0.005%
45	7.472	1904	1907	1913	rVB2	531	519	0.06%	0.007%
46	7.514	1913	1920	1922	rBV2	491	428	0.05%	0.006%
47	7.568	1922	1937	1952	rBV	96091	165867	19.20%	2.320%
48	7.655	1961	1964	1967	rBV2	337	288	0.03%	0.004%
49	7.713	1979	1982	1986	rBV	458	348	0.04%	0.005%
50	7.813	2010	2013	2018	rBV2	452	447	0.05%	0.006%
51	7.899	2027	2040	2055	rBV	327194	569054	65.86%	7.959%
52	8.179	2115	2127	2144	rBV	65331	110161	12.75%	1.541%
53	8.375	2185	2188	2191	rVB	464	288	0.03%	0.004%
54	8.401	2191	2196	2201	rBV3	704	832	0.10%	0.012%
55	8.427	2201	2204	2207	rVV	362	281	0.03%	0.004%
56	8.475	2211	2219	2232	rVB4	5128	9515	1.10%	0.133%
57	8.555	2232	2244	2256	rBV3	38344	65666	7.60%	0.918%
58	8.636	2256	2269	2298	rBV	240458	434863	50.33%	6.082%
59	8.787	2312	2316	2319	rBV	372	303	0.04%	0.004%
60	8.861	2333	2339	2341	rBV	367	414	0.05%	0.006%
61	8.989	2376	2379	2383	rBV	387	305	0.04%	0.004%
62	9.086	2405	2409	2413	rBV2	398	385	0.04%	0.005%
63	9.208	2443	2447	2451	rBV	494	464	0.05%	0.006%
64	9.279	2461	2469	2475	rBV2	705	1168	0.14%	0.016%
65	9.417	2499	2512	2539	rBV	336316	569786	65.94%	7.970%
66	9.571	2556	2560	2567	rVB2	1285	1481	0.17%	0.021%
67	9.694	2590	2598	2607	rVB4	3794	6133	0.71%	0.086%
68	9.999	2691	2693	2697	rBV2	347	279	0.03%	0.004%
69	10.234	2761	2766	2770	rVB2	310	318	0.04%	0.004%
70	10.449	2829	2833	2840	rBV2	321	374	0.04%	0.005%
71	10.671	2896	2902	2905	rBV3	1362	1329	0.15%	0.019%
72	10.758	2916	2929	2946	rVB	261676	416276	48.18%	5.822%
73	10.893	2961	2971	2986	rVB2	6753	11787	1.36%	0.165%
74	10.996	2997	3003	3009	rBV3	2222	3295	0.38%	0.046%
75	11.089	3020	3032	3038	rBV3	1872	2894	0.33%	0.040%
76	11.144	3045	3049	3053	rBV	376	334	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046194.D
 Acq On : 08 Dec 2021 22:35
 Operator : SY/MD
 Sample : M4983-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5N6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.288	3090	3094	3105	rVB3	1757	2486	0.29%	0.035%
78	11.468	3139	3150	3161	rVB	9172	13721	1.59%	0.192%
79	11.812	3245	3257	3274	rBV	396116	622327	72.02%	8.704%
80	11.899	3277	3284	3292	rVB3	2517	3856	0.45%	0.054%
81	11.935	3292	3295	3299	rBV	568	616	0.07%	0.009%
82	11.973	3303	3307	3315	rBV3	693	817	0.09%	0.011%
83	12.092	3340	3344	3347	rBV3	837	891	0.10%	0.012%
84	12.192	3362	3375	3394	rBV	362098	589619	68.24%	8.247%
85	12.484	3457	3466	3480	rVB4	4691	7945	0.92%	0.111%
86	12.771	3549	3555	3564	rVB	2667	3424	0.40%	0.048%
87	12.973	3615	3618	3621	rVB3	448	316	0.04%	0.004%
88	13.031	3632	3636	3641	rBV2	666	699	0.08%	0.010%
89	13.102	3654	3658	3662	rBV2	352	362	0.04%	0.005%
90	13.324	3721	3727	3730	rBV	352	331	0.04%	0.005%
91	13.767	3861	3865	3868	rBV	397	417	0.05%	0.006%
92	13.806	3874	3877	3880	rBV	440	339	0.04%	0.005%
93	14.089	3961	3965	3975	rVB3	1951	2800	0.32%	0.039%
94	14.581	4111	4118	4126	rVB2	2127	3154	0.37%	0.044%
95	14.716	4155	4160	4167	rBV2	467	654	0.08%	0.009%
96	15.005	4247	4250	4254	rVB2	516	353	0.04%	0.005%
97	15.066	4265	4269	4272	rBV2	467	405	0.05%	0.006%
98	15.224	4314	4318	4320	rBV3	760	685	0.08%	0.010%
99	15.555	4418	4421	4425	rBV3	594	602	0.07%	0.008%
100	15.597	4431	4434	4437	rBV	451	326	0.04%	0.005%




Sum of corrected areas: 7149500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046194.D
Acq On : 08 Dec 2021 22:35
Operator : SY/MD
Sample : M4983-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

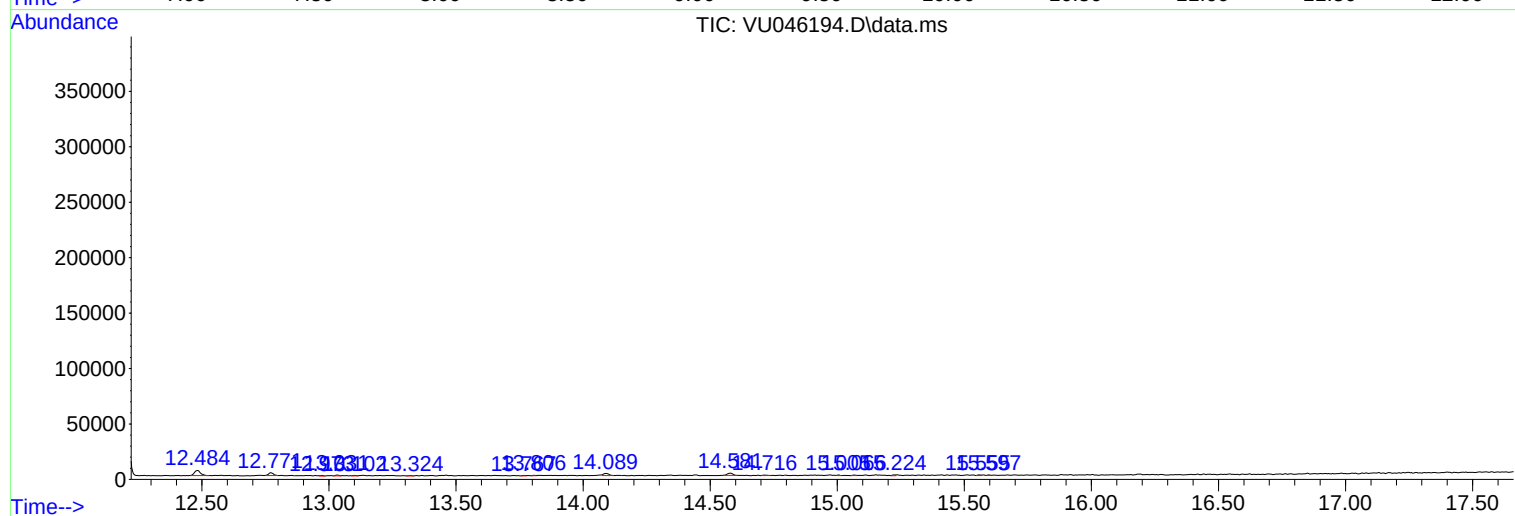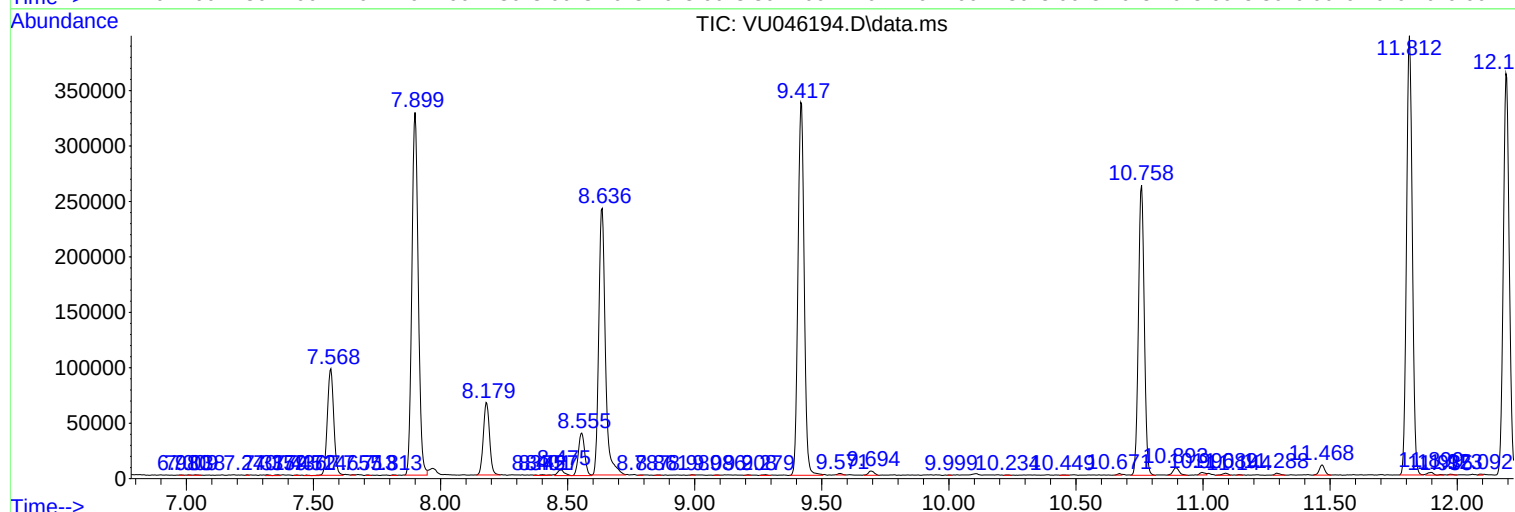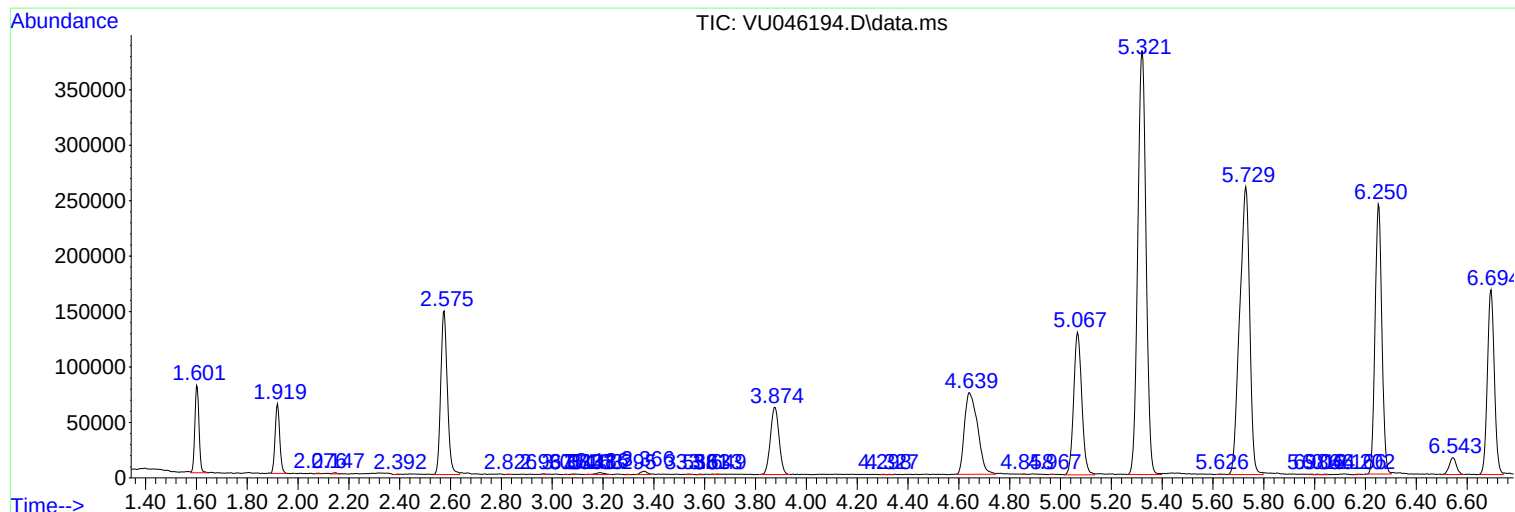

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046194.D
Acq On : 08 Dec 2021 22:35
Operator : SY/MD
Sample : M4983-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046194.D
Acq On : 08 Dec 2021 22:35
Operator : SY/MD
Sample : M4983-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5N6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc