

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046201.D
 Acq On : 09 Dec 2021 01:12
 Operator : SY/MD
 Sample : M4982-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	93	rBV	81231	89453	12.46%	1.456%
2	1.919	171	180	197	rVB	63166	80660	11.23%	1.313%
3	1.983	197	200	204	rBV4	835	551	0.08%	0.009%
4	2.228	273	276	281	rVB2	594	487	0.07%	0.008%
5	2.257	281	285	287	rBV2	537	521	0.07%	0.008%
6	2.398	326	329	334	rBV	597	537	0.07%	0.009%
7	2.427	334	338	342	rVB2	503	436	0.06%	0.007%
8	2.462	342	349	352	rBV	761	877	0.12%	0.014%
9	2.575	371	384	406	rBV2	148006	265516	36.97%	4.322%
10	2.784	445	449	451	rBV2	433	374	0.05%	0.006%
11	2.871	472	476	479	rBV2	350	354	0.05%	0.006%
12	2.961	501	504	510	rVB2	521	496	0.07%	0.008%
13	3.134	556	558	566	rVB	571	472	0.07%	0.008%
14	3.176	566	571	577	rBV2	1193	1852	0.26%	0.030%
15	3.449	652	656	659	rBV	424	357	0.05%	0.006%
16	3.649	713	718	721	rBV	431	476	0.07%	0.008%
17	3.861	780	784	786	rBV	659	572	0.08%	0.009%
18	4.199	886	889	892	rBV	472	413	0.06%	0.007%
19	4.475	971	975	979	rBV	391	454	0.06%	0.007%
20	4.504	980	984	986	rVV2	634	479	0.07%	0.008%
21	4.517	986	988	993	rVB2	571	472	0.07%	0.008%
22	4.639	1009	1026	1063	rVV2	74220	257267	35.82%	4.188%
23	4.996	1133	1137	1141	rBV2	333	371	0.05%	0.006%
24	5.067	1142	1159	1180	rVV	129080	289972	40.38%	4.720%
25	5.157	1183	1187	1190	rVV3	411	384	0.05%	0.006%
26	5.179	1190	1194	1197	rVV	621	548	0.08%	0.009%
27	5.199	1197	1200	1207	rVB2	638	602	0.08%	0.010%
28	5.324	1228	1239	1248	rVB5	3015	5801	0.81%	0.094%
29	5.446	1274	1277	1280	rBV2	518	453	0.06%	0.007%
30	5.729	1343	1365	1383	rBV2	266959	718145	100.00%	11.691%
31	5.999	1446	1449	1455	rVB2	485	423	0.06%	0.007%
32	6.063	1467	1469	1475	rBV2	458	369	0.05%	0.006%
33	6.137	1490	1492	1501	rBV2	327	382	0.05%	0.006%
34	6.250	1513	1527	1547	rBV	258006	483760	67.36%	7.875%
35	6.398	1570	1573	1579	rBV3	404	365	0.05%	0.006%
36	6.469	1592	1595	1599	rVB2	503	418	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046201.D
 Acq On : 09 Dec 2021 01:12
 Operator : SY/MD
 Sample : M4982-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.536	1606	1616	1630	rBV6	5329	11404	1.59%	0.186%
38	6.694	1651	1665	1681	rVV	168162	323536	45.05%	5.267%
39	6.851	1710	1714	1717	rBV	616	412	0.06%	0.007%
40	7.276	1843	1846	1849	rBV	598	387	0.05%	0.006%
41	7.417	1886	1890	1892	rBV	553	402	0.06%	0.007%
42	7.568	1924	1937	1956	rBV	94739	166164	23.14%	2.705%
43	7.758	1993	1996	2002	rVB	571	534	0.07%	0.009%
44	7.790	2002	2006	2013	rVB2	570	634	0.09%	0.010%
45	7.899	2027	2040	2057	rBV	330063	577656	80.44%	9.404%
46	8.179	2116	2127	2139	rBV	65588	107432	14.96%	1.749%
47	8.430	2194	2205	2207	rBV	513	835	0.12%	0.014%
48	8.475	2210	2219	2229	rVB	4107	7580	1.06%	0.123%
49	8.517	2229	2232	2237	rVB2	655	487	0.07%	0.008%
50	8.546	2237	2241	2244	rBV	626	505	0.07%	0.008%
51	8.565	2244	2247	2253	rVB2	550	487	0.07%	0.008%
52	8.636	2256	2269	2296	rBV	230023	423366	58.95%	6.892%
53	8.858	2334	2338	2343	rBV	456	416	0.06%	0.007%
54	8.928	2355	2360	2362	rBV	376	391	0.05%	0.006%
55	8.957	2366	2369	2376	rVB	583	694	0.10%	0.011%
56	8.993	2376	2380	2382	rBV	637	491	0.07%	0.008%
57	9.102	2408	2414	2417	rBV	391	394	0.05%	0.006%
58	9.131	2420	2423	2428	rVB2	547	461	0.06%	0.008%
59	9.417	2500	2512	2533	rBV	362083	606443	84.45%	9.872%
60	9.690	2594	2597	2610	rVB5	1832	2324	0.32%	0.038%
61	9.854	2642	2648	2651	rBV2	740	714	0.10%	0.012%
62	10.108	2720	2727	2732	rVB3	826	1048	0.15%	0.017%
63	10.192	2748	2753	2756	rBV	435	510	0.07%	0.008%
64	10.266	2772	2776	2780	rBV	384	391	0.05%	0.006%
65	10.398	2813	2817	2822	rVB	557	582	0.08%	0.009%
66	10.668	2895	2901	2902	rBV	1266	1015	0.14%	0.017%
67	10.758	2916	2929	2946	rVB	259574	415804	57.90%	6.769%
68	10.896	2961	2972	2984	rVB2	4976	8549	1.19%	0.139%
69	10.954	2985	2990	2992	rBV	379	389	0.05%	0.006%
70	11.095	3030	3034	3040	rVB3	801	893	0.12%	0.015%
71	11.224	3068	3074	3078	rBV	531	676	0.09%	0.011%
72	11.468	3142	3150	3157	rVB3	2568	3370	0.47%	0.055%
73	11.697	3217	3221	3225	rBV2	496	428	0.06%	0.007%
74	11.812	3245	3257	3277	rVB	418017	656628	91.43%	10.689%
75	11.899	3277	3284	3289	rBV3	739	891	0.12%	0.015%
76	11.944	3294	3298	3303	rBV3	646	717	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046201.D
 Acq On : 09 Dec 2021 01:12
 Operator : SY/MD
 Sample : M4982-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.195	3363	3376	3392	rVB	365329	593758	82.68%	9.666%
78	12.372	3427	3431	3434	rBV2	412	389	0.05%	0.006%
79	12.478	3459	3464	3466	rBV3	797	708	0.10%	0.012%
80	12.562	3487	3490	3494	rVB	589	391	0.05%	0.006%
81	12.690	3524	3530	3532	rBV2	387	451	0.06%	0.007%
82	12.722	3537	3540	3542	rBV	570	406	0.06%	0.007%
83	12.774	3546	3556	3564	rVB3	1325	2464	0.34%	0.040%
84	12.902	3593	3596	3601	rVB2	450	401	0.06%	0.007%
85	12.973	3613	3618	3620	rBV2	429	393	0.05%	0.006%
86	13.102	3655	3658	3663	rBV	349	374	0.05%	0.006%
87	13.195	3683	3687	3691	rBV2	452	373	0.05%	0.006%
88	13.349	3729	3735	3737	rBV	559	596	0.08%	0.010%
89	13.790	3867	3872	3879	rBV	824	1184	0.16%	0.019%
90	13.996	3931	3936	3938	rBV2	502	443	0.06%	0.007%
91	14.478	4083	4086	4090	rVB2	586	462	0.06%	0.008%
92	14.504	4090	4094	4101	rBV	504	649	0.09%	0.011%
93	14.574	4108	4116	4125	rVB3	1951	3203	0.45%	0.052%
94	15.565	4421	4424	4432	rVB2	803	834	0.12%	0.014%
95	15.661	4451	4454	4460	rVB2	483	480	0.07%	0.008%
96	15.774	4486	4489	4496	rVB2	649	756	0.11%	0.012%
97	16.188	4611	4618	4624	rBV3	833	1429	0.20%	0.023%
98	16.240	4631	4634	4638	rBV4	488	375	0.05%	0.006%
99	16.259	4638	4640	4645	rVB2	815	662	0.09%	0.011%
100	16.716	4780	4782	4787	rBV2	594	614	0.09%	0.010%




Sum of corrected areas: 6142904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046201.D
Acq On : 09 Dec 2021 01:12
Operator : SY/MD
Sample : M4982-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

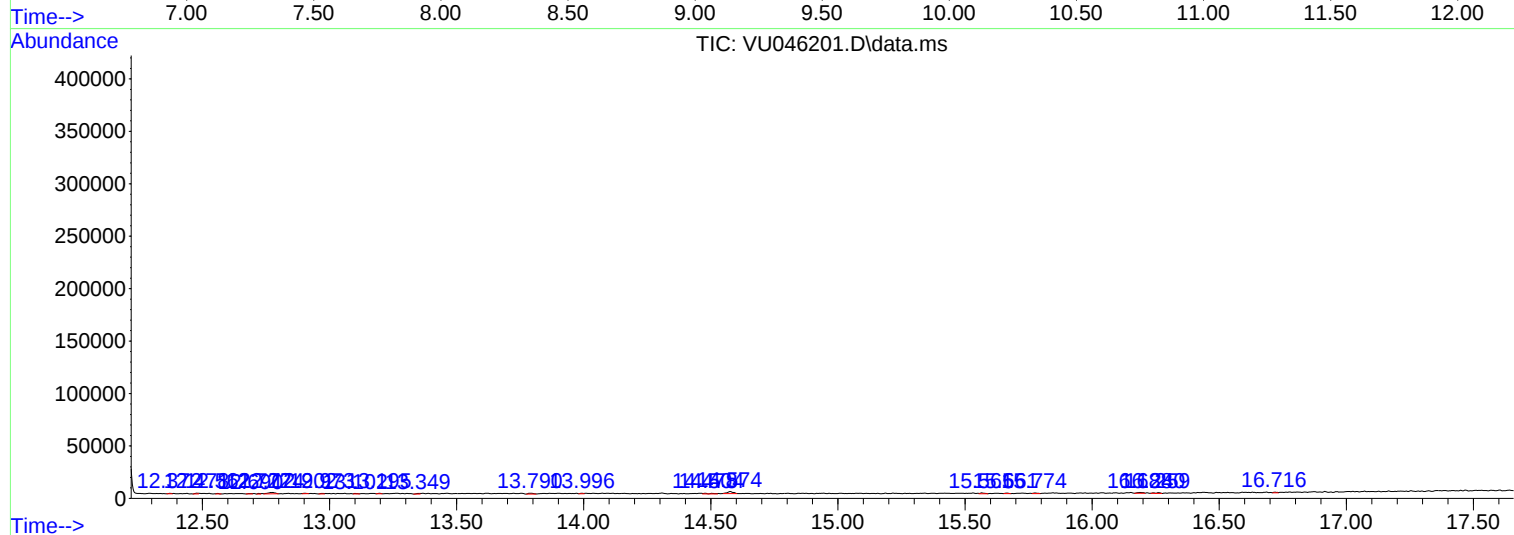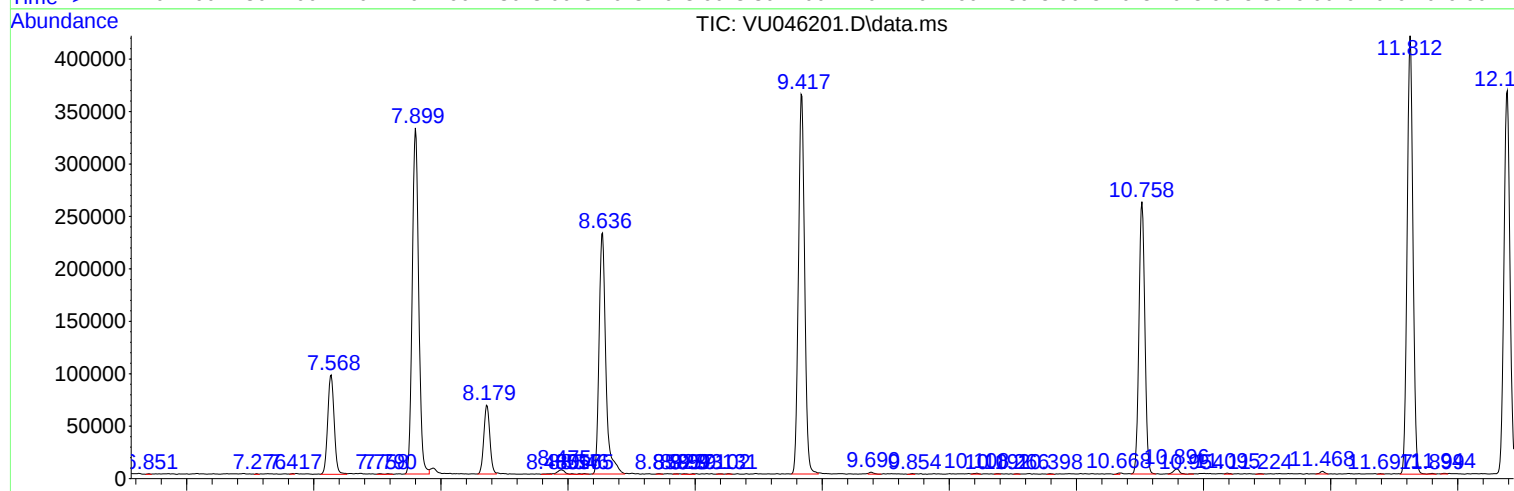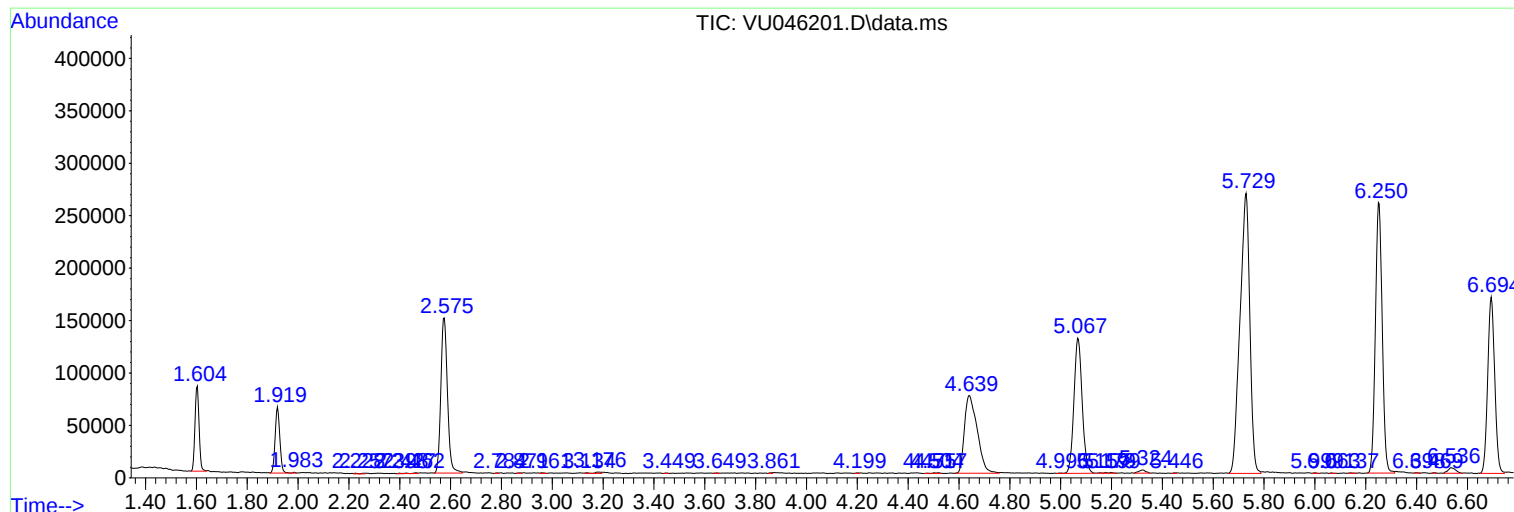

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046201.D
Acq On : 09 Dec 2021 01:12
Operator : SY/MD
Sample : M4982-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046201.D
Acq On : 09 Dec 2021 01:12
Operator : SY/MD
Sample : M4982-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------