

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046202.D
 Acq On : 09 Dec 2021 01:34
 Operator : SY/MD
 Sample : M4982-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	91	rVB	77101	85394	12.03%	1.426%
2	1.919	172	180	194	rVB	61540	78515	11.06%	1.311%
3	2.083	229	231	234	rBV	596	441	0.06%	0.007%
4	2.211	268	271	274	rVB2	267	147	0.02%	0.002%
5	2.231	274	277	280	rBV2	464	293	0.04%	0.005%
6	2.250	280	283	284	rBV	231	131	0.02%	0.002%
7	2.327	304	307	311	rBV2	578	556	0.08%	0.009%
8	2.379	318	323	326	rVB	362	293	0.04%	0.005%
9	2.398	326	329	335	rVB2	508	407	0.06%	0.007%
10	2.430	335	339	340	rBV	356	261	0.04%	0.004%
11	2.572	371	383	401	rBV	137550	232820	32.80%	3.889%
12	2.800	452	454	455	rBV	325	134	0.02%	0.002%
13	3.260	595	597	604	rVB2	475	379	0.05%	0.006%
14	3.379	631	634	637	rBV2	471	384	0.05%	0.006%
15	3.668	722	724	727	rBV	462	313	0.04%	0.005%
16	3.784	756	760	763	rBV	393	422	0.06%	0.007%
17	4.060	844	846	849	rBV	407	213	0.03%	0.004%
18	4.295	916	919	920	rBV	474	269	0.04%	0.004%
19	4.549	996	998	1005	rBB2	362	271	0.04%	0.005%
20	4.636	1006	1025	1064	rBV2	77606	238090	33.54%	3.977%
21	4.912	1109	1111	1114	rBV	530	430	0.06%	0.007%
22	5.067	1143	1159	1185	rBV	129833	292070	41.14%	4.878%
23	5.247	1211	1215	1216	rBV	492	334	0.05%	0.006%
24	5.430	1269	1272	1275	rBV	353	253	0.04%	0.004%
25	5.485	1286	1289	1297	rBV2	426	533	0.08%	0.009%
26	5.729	1344	1365	1384	rBV2	260338	709881	100.00%	11.857%
27	6.034	1458	1460	1461	rBV	241	90	0.01%	0.002%
28	6.086	1471	1476	1481	rBV2	504	703	0.10%	0.012%
29	6.115	1481	1485	1486	rBV	522	360	0.05%	0.006%
30	6.253	1513	1528	1548	rBV	251692	478234	67.37%	7.988%
31	6.533	1606	1615	1630	rBV4	4063	8319	1.17%	0.139%
32	6.620	1639	1642	1649	rBV	568	580	0.08%	0.010%
33	6.694	1652	1665	1684	rVV	165129	316563	44.59%	5.287%
34	6.951	1739	1745	1748	rBV	497	479	0.07%	0.008%
35	7.105	1791	1793	1794	rBV	205	94	0.01%	0.002%
36	7.173	1811	1814	1819	rBV2	684	743	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046202.D
 Acq On : 09 Dec 2021 01:34
 Operator : SY/MD
 Sample : M4982-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.292	1847	1851	1854	rBV	387	377	0.05%	0.006%
38	7.346	1866	1868	1871	rBV	233	137	0.02%	0.002%
39	7.404	1880	1886	1889	rBV2	604	587	0.08%	0.010%
40	7.465	1901	1905	1912	rVB2	516	755	0.11%	0.013%
41	7.504	1912	1917	1921	rBV2	642	632	0.09%	0.011%
42	7.568	1924	1937	1956	rBV	93678	163382	23.02%	2.729%
43	7.722	1982	1985	1987	rBV	305	156	0.02%	0.003%
44	7.742	1987	1991	1994	rBV	381	351	0.05%	0.006%
45	7.899	2027	2040	2056	rBV	328563	568916	80.14%	9.502%
46	8.179	2117	2127	2141	rBV	62730	104968	14.79%	1.753%
47	8.330	2171	2174	2175	rBV2	201	121	0.02%	0.002%
48	8.375	2185	2188	2193	rVB2	530	505	0.07%	0.008%
49	8.411	2195	2199	2202	rBV2	463	451	0.06%	0.008%
50	8.475	2209	2219	2229	rBV3	3882	7202	1.01%	0.120%
51	8.578	2247	2251	2252	rBV	469	357	0.05%	0.006%
52	8.636	2257	2269	2297	rVV	232178	424107	59.74%	7.084%
53	8.825	2325	2328	2337	rVB3	939	1310	0.18%	0.022%
54	8.928	2357	2360	2365	rBV	411	420	0.06%	0.007%
55	9.021	2385	2389	2394	rBV	681	601	0.08%	0.010%
56	9.050	2394	2398	2404	rVB2	465	518	0.07%	0.009%
57	9.083	2404	2408	2412	rBV2	498	373	0.05%	0.006%
58	9.134	2421	2424	2426	rBV	285	200	0.03%	0.003%
59	9.275	2465	2468	2471	rBV	585	395	0.06%	0.007%
60	9.417	2499	2512	2540	rBV	357137	599634	84.47%	10.015%
61	9.751	2612	2616	2619	rBV2	437	334	0.05%	0.006%
62	9.771	2619	2622	2624	rBV	375	210	0.03%	0.004%
63	10.092	2719	2722	2723	rBV	709	424	0.06%	0.007%
64	10.243	2766	2769	2773	rBB4	603	430	0.06%	0.007%
65	10.758	2916	2929	2946	rBV	256205	409723	57.72%	6.843%
66	10.893	2964	2971	2982	rVB2	5034	7485	1.05%	0.125%
67	10.983	2995	2999	3000	rBV	377	287	0.04%	0.005%
68	11.433	3136	3139	3140	rBV	262	140	0.02%	0.002%
69	11.472	3141	3151	3162	rVB5	4720	8509	1.20%	0.142%
70	11.529	3165	3169	3171	rBV	525	456	0.06%	0.008%
71	11.597	3187	3190	3193	rVB	548	346	0.05%	0.006%
72	11.661	3205	3210	3216	rBV	514	705	0.10%	0.012%
73	11.812	3245	3257	3275	rBV	409608	645017	90.86%	10.773%
74	12.192	3363	3375	3390	rBV	364461	585881	82.53%	9.786%
75	13.005	3625	3628	3632	rBV	435	337	0.05%	0.006%
76	13.574	3802	3805	3807	rBV	401	246	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046202.D
Acq On : 09 Dec 2021 01:34
Operator : SY/MD
Sample : M4982-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis

77	14.288	4024	4027	4028	rBV	484	278	0.04%	0.005%
78	15.346	4353	4356	4359	rBV	484	455	0.06%	0.008%




Sum of corrected areas: 5987117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046202.D
Acq On : 09 Dec 2021 01:34
Operator : SY/MD
Sample : M4982-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

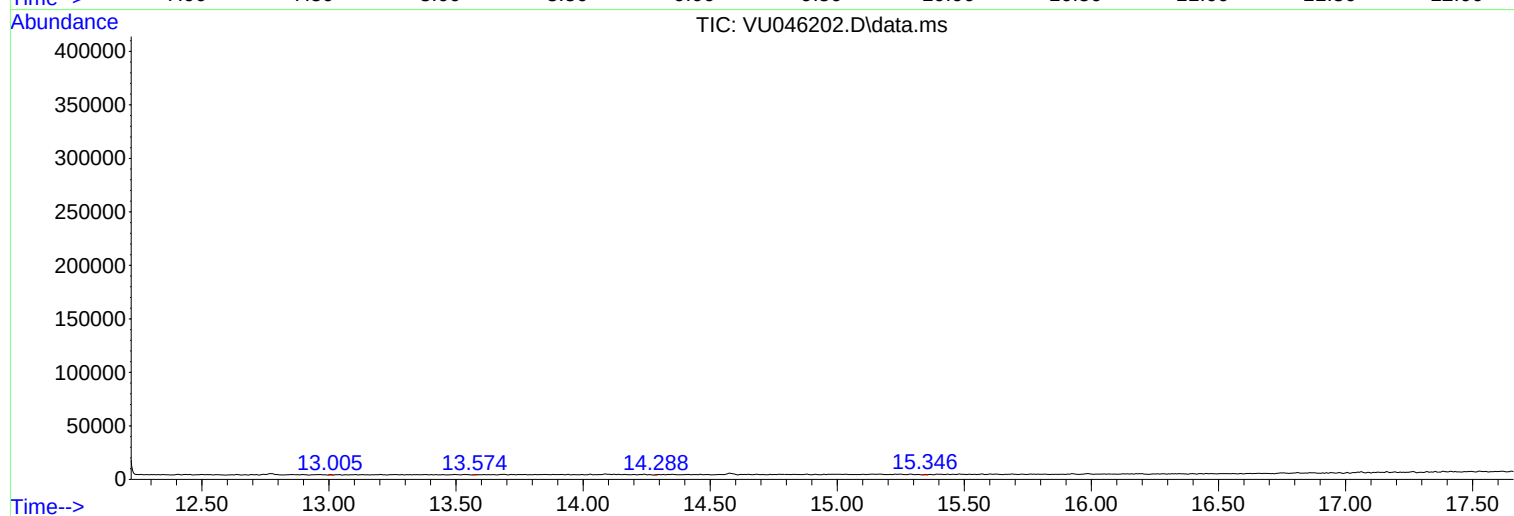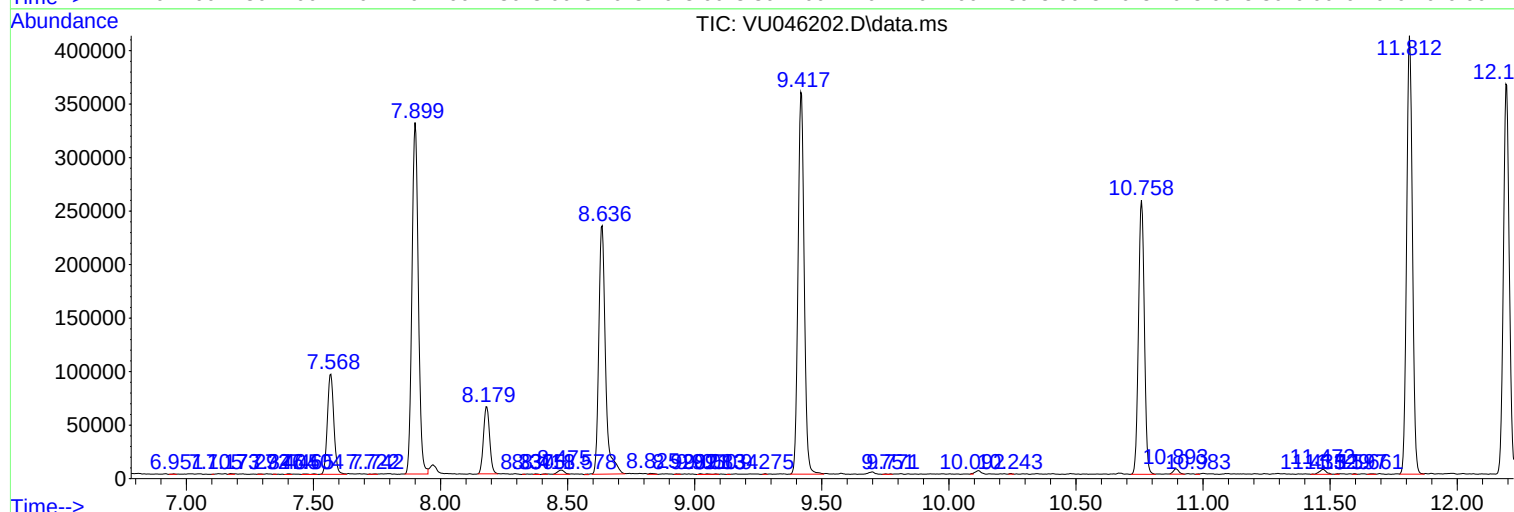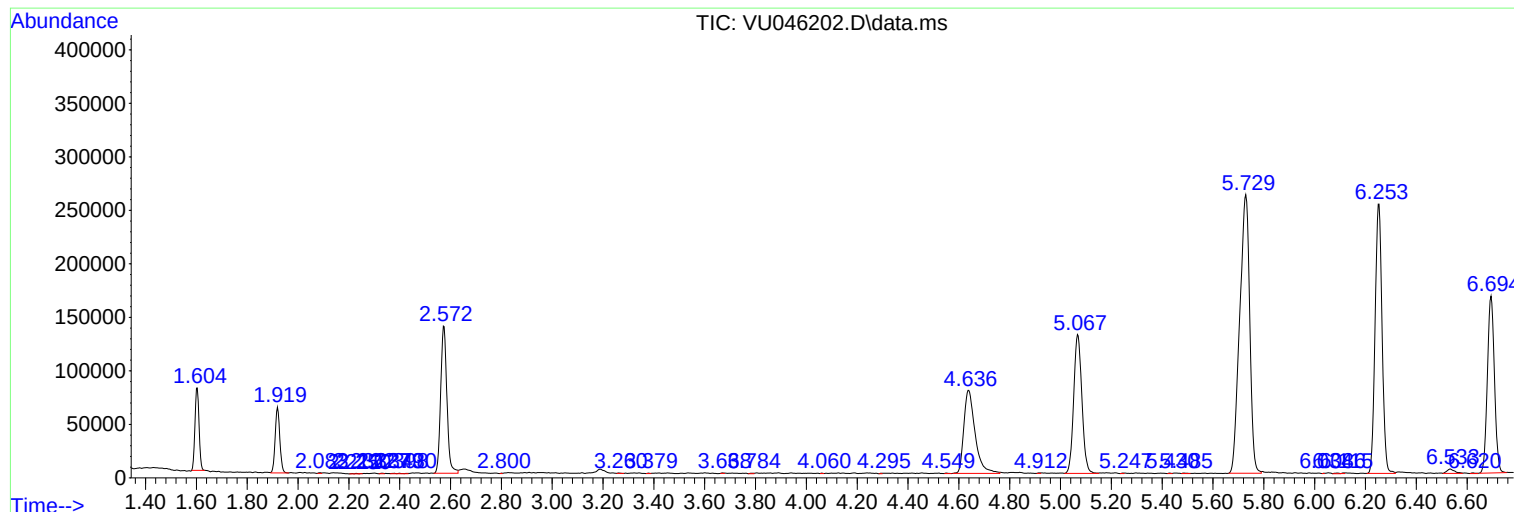

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046202.D
Acq On : 09 Dec 2021 01:34
Operator : SY/MD
Sample : M4982-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
Data File : VU046202.D
Acq On : 09 Dec 2021 01:34
Operator : SY/MD
Sample : M4982-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------