


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120821\
 Data File : VU046162.D
 Acq On : 08 Dec 2021 09:25
 Operator : SY/MD
 Sample : BFB026
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB026

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 03 05:08:36 2021

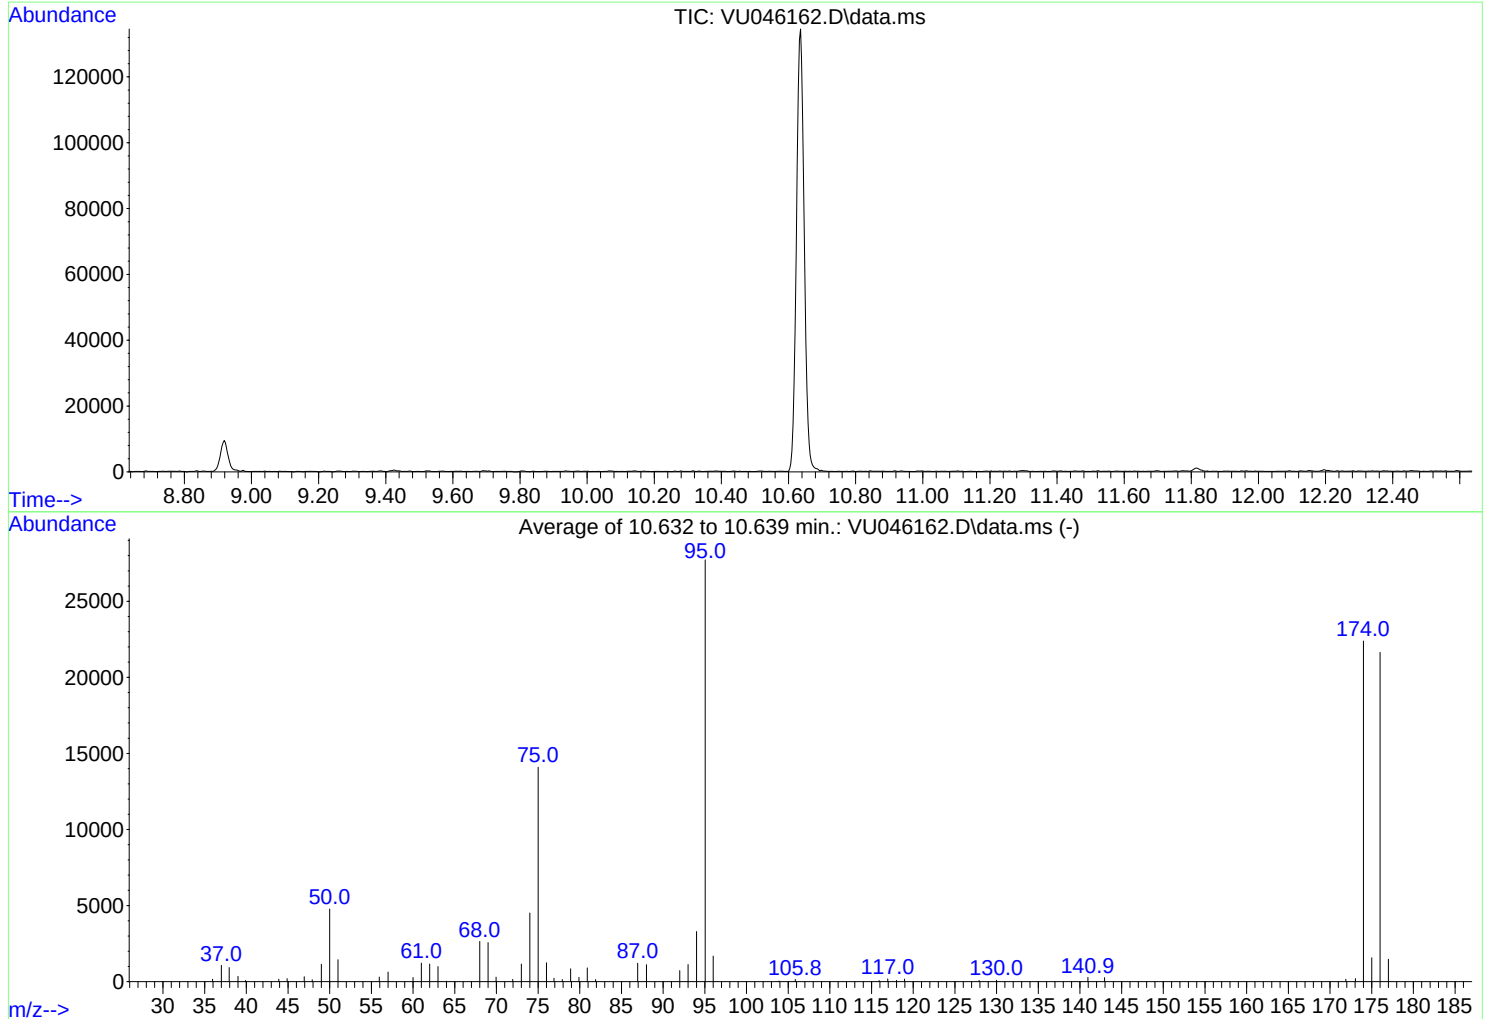

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4777	PASS
75	95	30	80	50.8	14088	PASS
95	95	100	100	100.0	27723	PASS
96	95	5	9	6.1	1680	PASS
173	174	0.00	2	0.9	199	PASS
174	95	50	120	80.8	22392	PASS
175	174	5	9	7.0	1572	PASS
176	174	95	101	96.7	21645	PASS
177	176	5	9	6.8	1471	PASS

m/z	Abundance
43.90	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	162.0
37.00	1125.0
38.00	944.0
39.00	372.0
43.90	352.0
44.90	176.0
46.90	313.0
47.90	150.0
49.00	1231.0
50.00	4961.0
51.00	1415.0
56.00	336.0
57.00	653.0
60.00	272.0
61.00	1240.0
62.00	1171.0
63.00	946.0
68.00	2743.0
69.00	2702.0
69.90	279.0
71.90	115.0
73.00	1123.0
74.00	4634.0
75.00	13867.0
76.00	1314.0
76.90	245.0
77.90	131.0
78.90	860.0
79.90	291.0
80.90	854.0
81.90	137.0
86.90	1197.0
88.00	1061.0
92.00	769.0
93.00	1086.0
94.00	3366.0
95.10	28248.0
96.00	1802.0
103.90	119.0
105.90	118.0
116.90	195.0
118.90	172.0
127.90	117.0
130.00	152.0
141.00	277.0
143.00	242.0
171.90	140.0
173.10	202.0
174.00	22240.0
175.00	1625.0
176.00	21456.0
177.00	1528.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	163.0
37.00	1112.0
37.90	948.0
39.00	351.0
39.90	110.0
43.90	336.0
44.90	209.0
46.90	332.0
47.90	128.0
49.00	1183.0
50.00	4904.0
51.00	1511.0
55.90	300.0
57.00	645.0
60.00	296.0
61.00	1260.0
62.00	1168.0
63.00	999.0
64.00	107.0
68.00	2728.0
69.00	2628.0
69.90	302.0
72.00	157.0
73.00	1209.0
74.00	4642.0
75.00	14565.0
76.00	1278.0
76.90	220.0
77.90	141.0
78.90	878.0
79.90	302.0
80.90	940.0
81.90	144.0
87.00	1273.0
88.00	1167.0
92.00	739.0
93.00	1165.0
94.00	3378.0
95.00	28536.0
96.00	1698.0
105.80	155.0
115.90	104.0
117.00	181.0
118.00	114.0
119.00	167.0
127.90	122.0
130.00	135.0
140.90	295.0
142.90	274.0
171.90	169.0
173.00	212.0
174.00	23064.0
175.00	1631.0
176.00	22192.0
177.00	1549.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.00	161.0
37.00	978.0
37.00	888.0
39.00	318.0
39.00	109.0
43.00	292.0
44.00	221.0
47.00	326.0
47.00	108.0
49.00	1019.0
50.00	4466.0
51.00	1405.0
55.00	291.0
57.00	584.0
60.00	261.0
61.00	1149.0
62.00	1129.0
63.00	1009.0
68.00	2433.0
69.00	2384.0
70.00	298.0
72.00	166.0
73.00	1129.0
74.00	4259.0
75.00	13832.0
76.00	1130.0
76.00	182.0
77.00	127.0
78.00	781.0
79.00	251.0
80.00	922.0
81.00	137.0
87.00	1148.0
88.00	1133.0
92.00	676.0
93.00	1121.0
94.00	3142.0
95.00	26384.0
96.00	1540.0
105.00	159.0
115.00	103.0
116.00	162.0
118.00	126.0
118.00	160.0
140.00	271.0
143.00	286.0
171.00	167.0
173.00	182.0
174.00	21872.0
175.00	1459.0
176.00	21288.0
177.00	1337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026