

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
 Data File : VU052256.D
 Acq On : 08 Dec 2022 18:10
 Operator : JC/MD
 Sample : N5930-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ84

Quant Time: Dec 08 22:33:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	1728	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	2048	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	2381	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	119	0.708	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	14.200%#
7) Chloroethane-d5	1.919	69	49	0.375	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	7.600%#
11) 1,1-Dichloroethene-d2	0.000	65	0	0.000	ug/L	
Spiked Amount	5.000	Range	60 - 125	Recovery	=	0.000%#
20) 2-Butanone-d5	4.661	46	64	2.101	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	4.200%#
24) Chloroform-d	5.086	84	14369	58.181	ug/L	0.03
Spiked Amount	5.000	Range	70 - 125	Recovery	=	1163.600%#
26) 1,2-Dichloroethane-d4	5.706	65	555	4.449	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
32) Benzene-d6	5.722	84	731	1.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	24.000%#
36) 1,2-Dichloropropane-d6	6.693	67	136	0.723	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	14.400%#
41) Toluene-d8	7.899	98	1634	2.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	59.400%#
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	5.000	Range	55 - 130	Recovery	=	0.000%#
46) 2-Hexanone-d5	8.632	63	247	8.500	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	17.000%#
56) 1,1,2,2-Tetrachloroeth...	10.758	84	686	4.205	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.000%
66) 1,2-Dichlorobenzene-d4	12.188	152	1820	3.992	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.800%#
Target Compounds						
					Qvalue	
3) Chloromethane	1.523	50	1680	8.589	ug/L	86
5) Vinyl chloride	1.604	62	40	0.213	ug/L #	1
6) Bromomethane	1.713	94	21	0.218	ug/L #	3
8) Chloroethane	1.941	64	196	1.677	ug/L #	45
12) 1,1-Dichloroethene	2.552	96	46	0.367	ug/L #	1
13) Acetone	2.655	43	35370	1709.604	ug/L	95
14) Carbon disulfide	2.797	76	2638	6.079	ug/L #	88
15) Methyl Acetate	3.044	43	318	5.926	ug/L #	48
16) Methylene chloride	3.047	84	116548	687.248	ug/L	98
17) Methyl tert-butyl Ether	3.362	73	91	0.324	ug/L #	67
18) trans-1,2-Dichloroethene	3.147	96	80	0.595	ug/L #	1
19) 1,1-Dichloroethane	3.661	63	57	0.235	ug/L #	50
21) 2-Butanone	4.748	43	866	26.116	ug/L #	48
22) cis-1,2-Dichloroethene	4.668	96	41	0.291	ug/L #	1
23) Bromochloromethane	4.980	128	62	0.919	ug/L #	1
25) Chloroform	5.086	83	352987	1438.401	ug/L	98
27) 1,2-Dichloroethane	5.793	62	1007	6.700	ug/L #	72
30) Cyclohexane	5.391	56	50	0.227	ug/L #	14
33) Benzene	5.777	78	1589	2.384	ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
 Data File : VU052256.D
 Acq On : 08 Dec 2022 18:10
 Operator : JC/MD
 Sample : N5930-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ84

Quant Time: Dec 08 22:33:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

34) Trichloroethene	6.542	95	10406	62.595	ug/L	95
38) Bromodichloromethane	7.102	83	7709	36.640	ug/L #	94
40) 4-Methyl-2-pentanone	7.800	43	520	5.769	ug/L #	40
42) Toluene	7.970	91	11558	16.858	ug/L	96
48) 2-Hexanone	8.687	43	1729	26.163	ug/L #	79
49) Dibromochloromethane	8.812	129	1134	7.808	ug/L	80
51) Chlorobenzene	9.443	112	977	2.235	ug/L #	77
52) Ethylbenzene	9.568	91	1641	2.462	ug/L	95
53) m,p-Xylene	9.690	106	2518	9.756	ug/L	91
54) o-Xylene	10.102	106	583	2.357	ug/L	82
60) Isopropylbenzene	10.095	105	192	0.128	ug/L #	49
61) 1,2,3-Trichloropropane	11.812	75	184	0.675	ug/L #	41
64) 1,3-Dichlorobenzene	11.825	146	256	0.335	ug/L #	71
65) 1,4-Dichlorobenzene	11.825	146	256	0.336	ug/L #	72
67) 1,2-Dichlorobenzene	12.211	146	1538	2.091	ug/L	88
71) Naphthalene	14.095	128	230	0.297	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_U
ClientSampleId :
EXZ84

Instrument :
MSVOA_U
ClientSampleId :
EXZ84

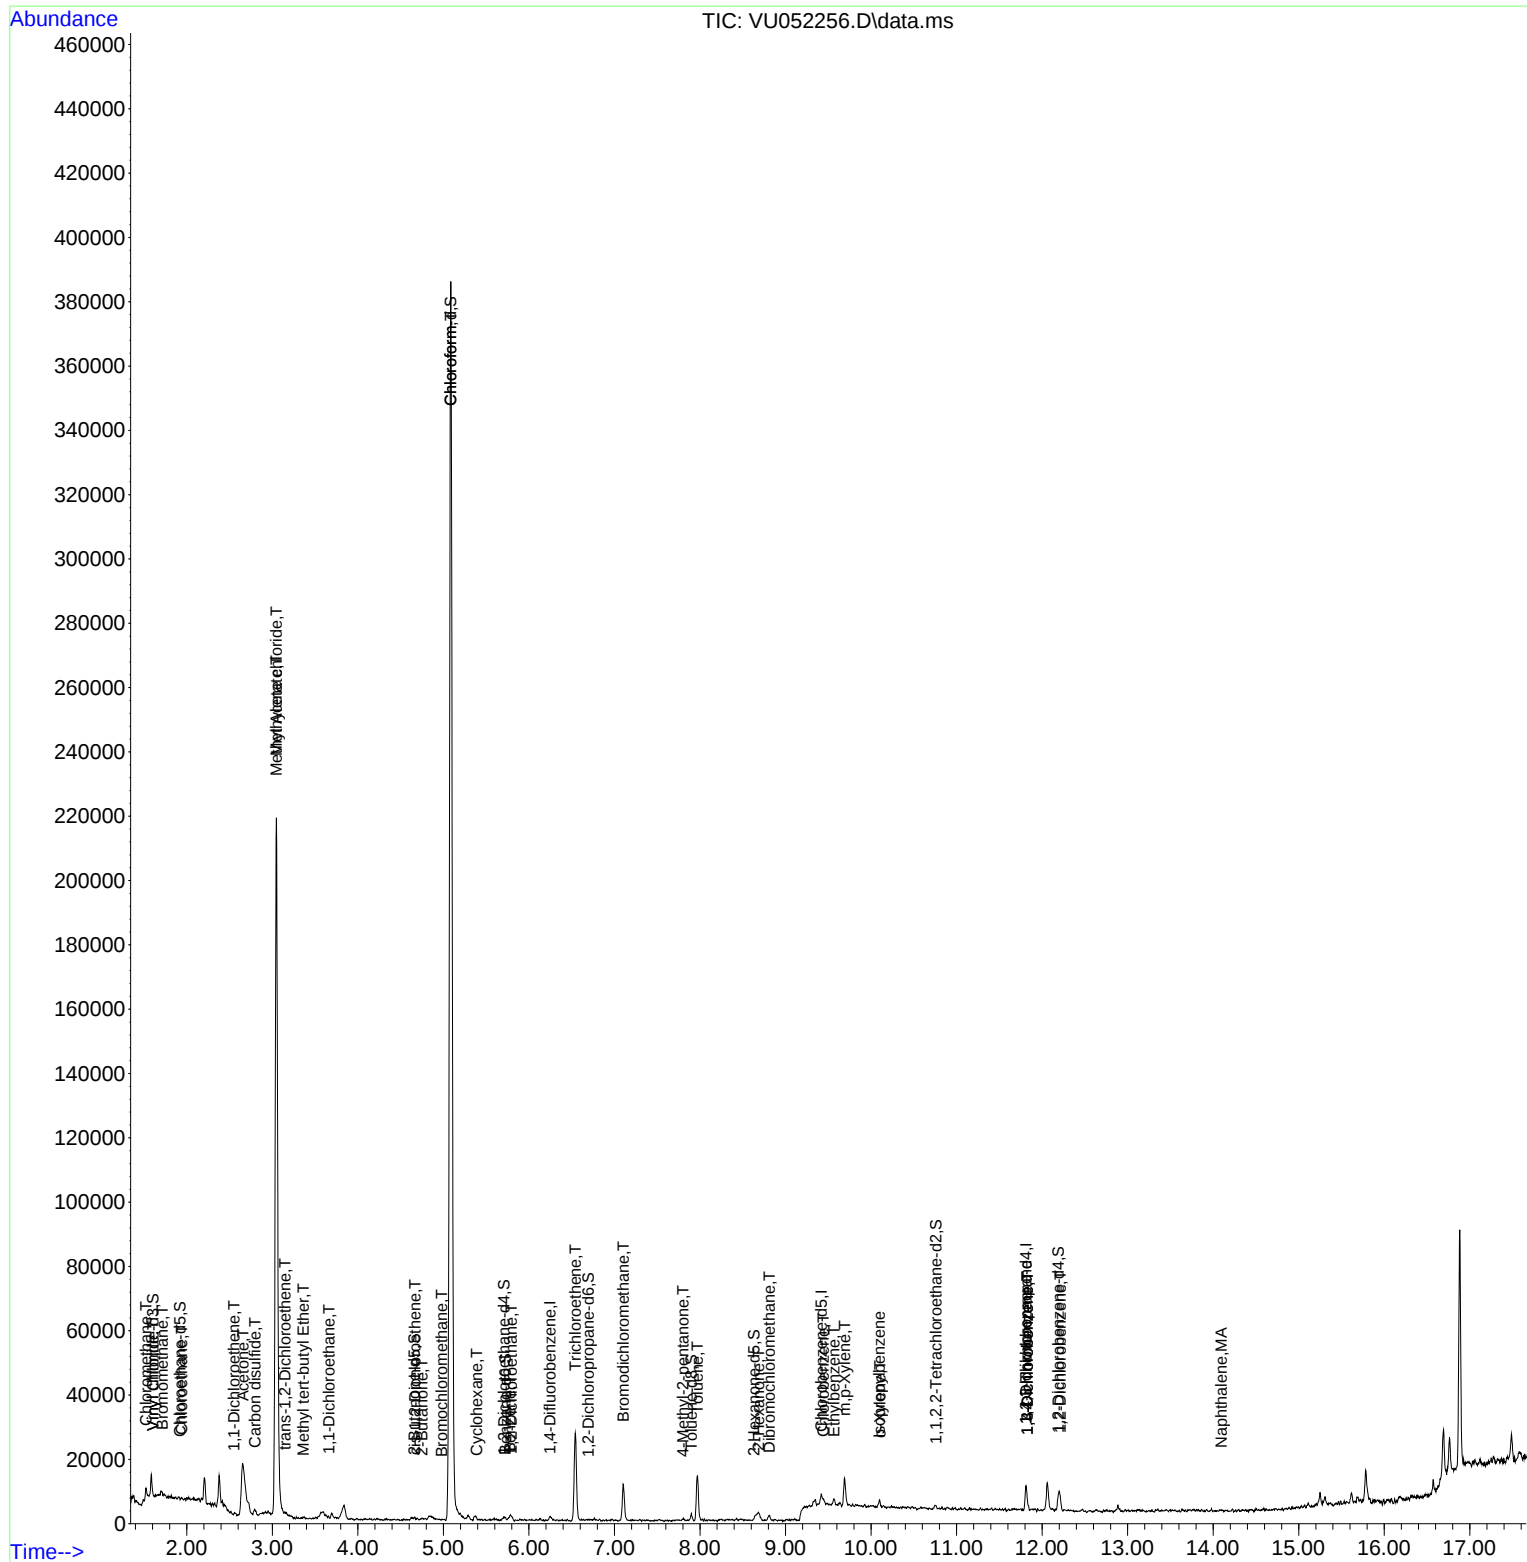





Abundance Scan 57 (1.523 min): VU052237.D\data.ms (-46)

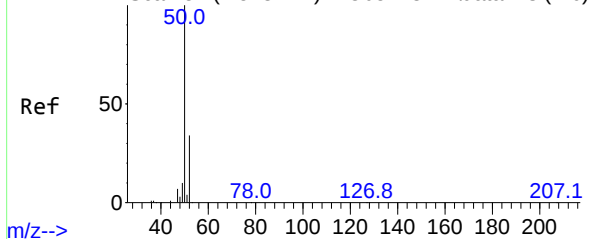

#3
Chloromethane
Concen: 8.589 ug/L
RT: 1.523 min Scan# 51
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 50 Resp: 1680
Ion Ratio Lower Upper
50 100
52 41.6 23.4 43.4

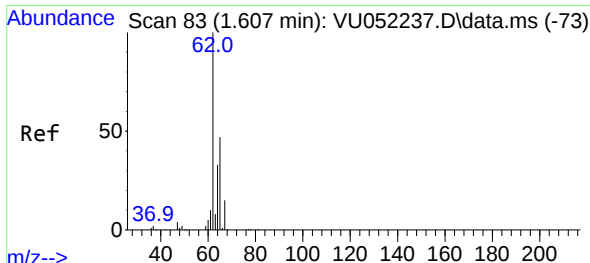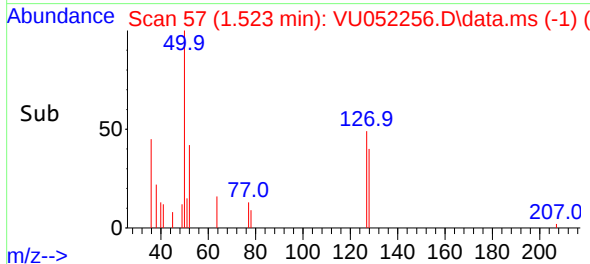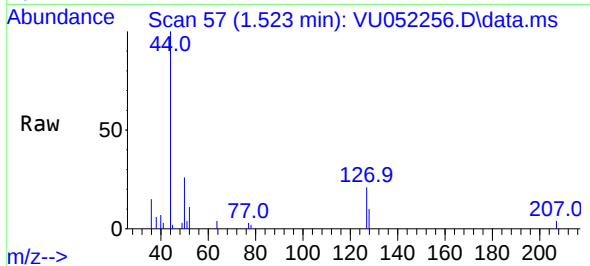

#5
Vinyl chloride
Concen: 0.213 ug/L
RT: 1.604 min Scan# 82
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 62 Resp: 40
Ion Ratio Lower Upper
62 100
64 140.2 23.5 43.7#


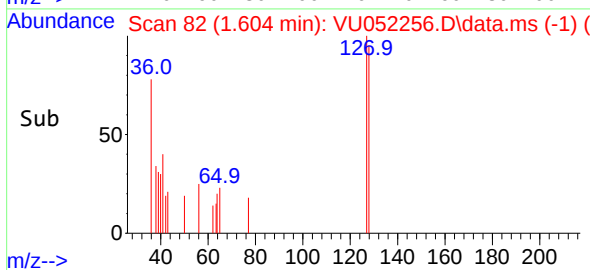

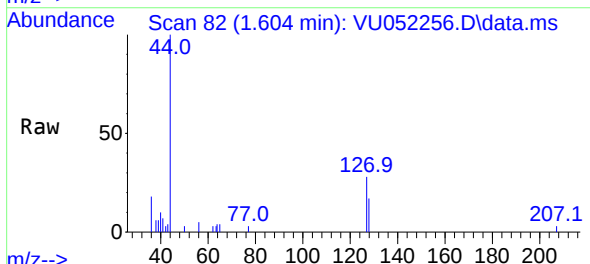




#6
Bromomethane
Concen: 0.218 ug/L
RT: 1.713 min Scan# 11
Delta R.T. -0.145 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 94 Resp: 21
Ion Ratio Lower Upper
94 100
96 0.0 65.7 122.1#

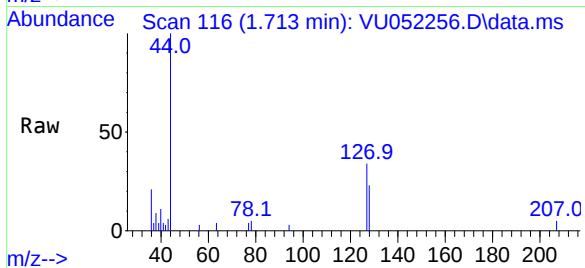

#8
Chloroethane
Concen: 1.677 ug/L
RT: 1.941 min Scan# 187
Delta R.T. 0.006 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 64 Resp: 196
Ion Ratio Lower Upper
64 100
66 0.0 21.1 39.1#


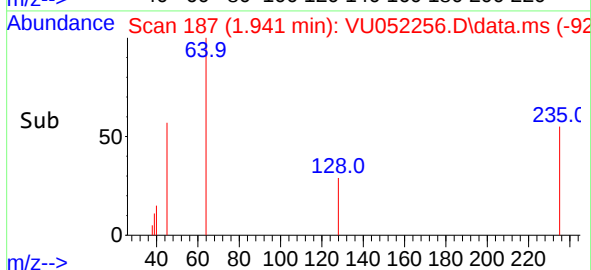

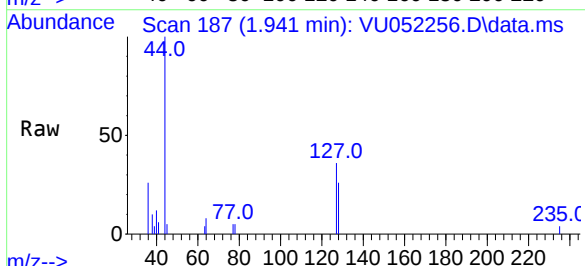




#12
1,1-Dichloroethene
Concen: 0.367 ug/L
RT: 2.552 min Scan# 31
Delta R.T. -0.029 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 96 Resp: 46
Ion Ratio Lower Upper
96 100
61 0.0 114.8 213.2#
63 0.0 93.7 174.1#

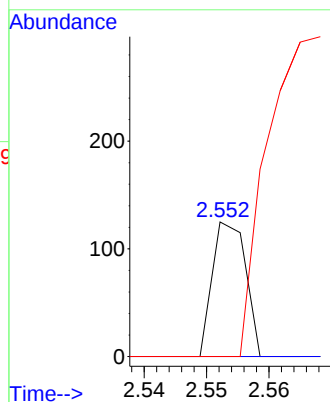

#13
Acetone
Concen: 1709.604 ug/L
RT: 2.655 min Scan# 409
Delta R.T. 0.010 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 43 Resp: 35370
Ion Ratio Lower Upper
43 100
58 35.2 0.0 76.0

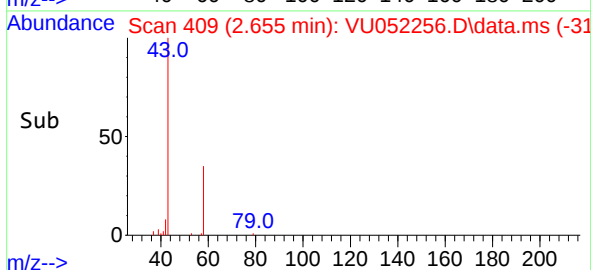



#14

Carbon disulfide

Concen: 6.079 ug/L

RT: 2.797 min Scan# 4

Delta R.T. 0.003 min

Lab File: VU052256.D

Acq: 08 Dec 2022 18:10

Instrument :

MSVOA_U

ClientSampleId :





EXZ84

Tgt Ion: 76 Resp: 2638

Ion Ratio Lower Upper

76 100

78 12.9 7.0 10.4#

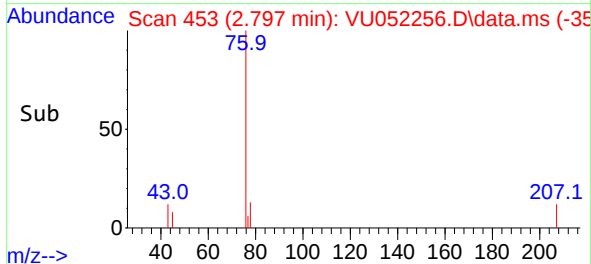

#15

Methyl Acetate

Concen: 5.926 ug/L

RT: 3.044 min Scan# 530

Delta R.T. 0.087 min

Lab File: VU052256.D




Acq: 08 Dec 2022 18:10


Tgt Ion: 43 Resp: 318

Ion Ratio Lower Upper

43 100

74 0.0 21.3 31.9#



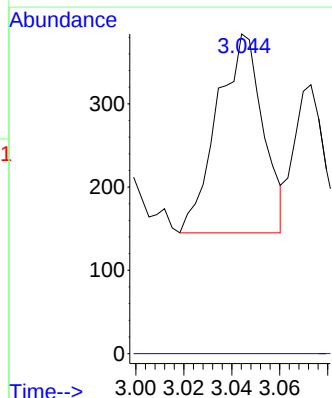
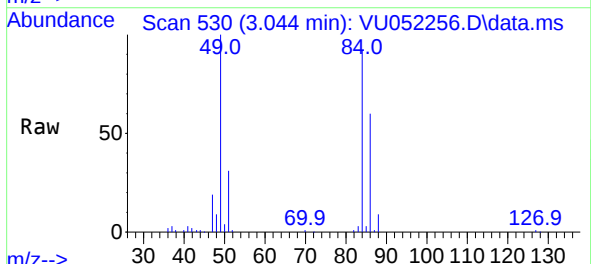


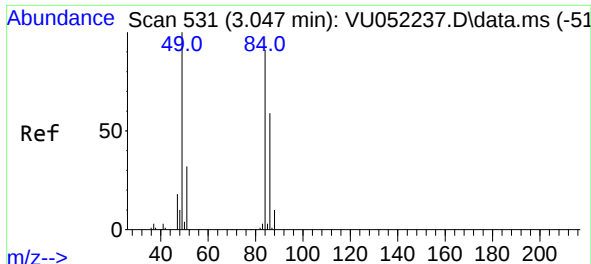

#16
Methylene chloride
Concen: 687.248 ug/L
RT: 3.047 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 84 Resp: 116548
Ion Ratio Lower Upper
84 100
86 65.0 43.8 81.4
49 109.7 75.9 141.1

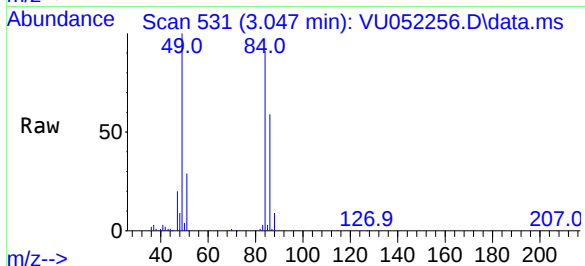

#17
Methyl tert-butyl Ether
Concen: 0.324 ug/L
RT: 3.362 min Scan# 629
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10


Tgt Ion: 73 Resp: 91
Ion Ratio Lower Upper
73 100
43 23.1 13.2 19.8#
57 0.0 17.8 26.8#

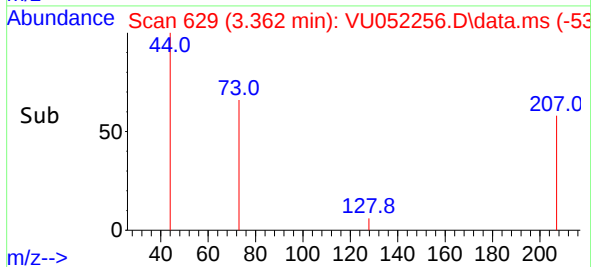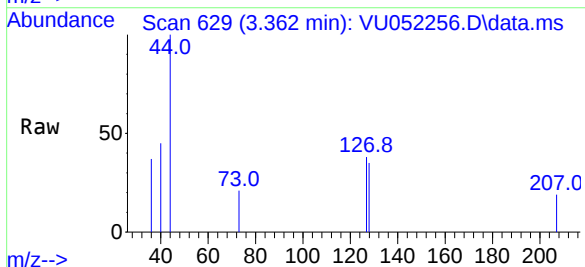



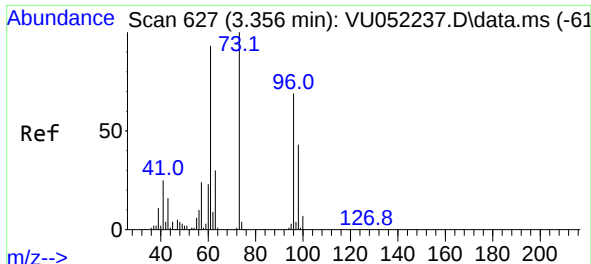


#18
trans-1,2-Dichloroethene
Concen: 0.595 ug/L
RT: 3.147 min Scan# 501
Delta R.T. -0.206 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Instrument :
MSVOA_U
ClientSampleId :
EXZ84







Tgt Ion: 96 Resp: 80
Ion Ratio Lower Upper
96 100
61 0.0 97.9 181.7#
98 0.0 43.8 81.3#

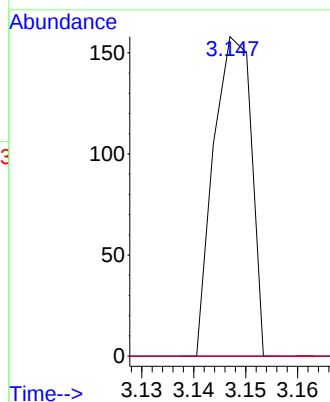

#19
1,1-Dichloroethane
Concen: 0.235 ug/L
RT: 3.661 min Scan# 722
Delta R.T. -0.206 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 63 Resp: 57
Ion Ratio Lower Upper
63 100
65 0.0 22.2 41.2#
83 0.0 9.2 17.0#




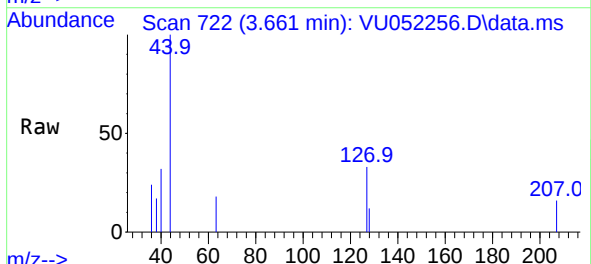




#21
2-Butanone
Concen: 26.116 ug/L
RT: 4.748 min Scan# 1060
Delta R.T. 0.035 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 43 Resp: 866
Ion Ratio Lower Upper
43 100
72 2.3 15.6 46.8#

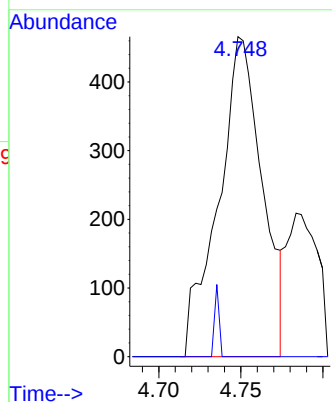

#22
cis-1,2-Dichloroethene
Concen: 0.291 ug/L
RT: 4.668 min Scan# 1035
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 96 Resp: 41
Ion Ratio Lower Upper
96 100
61 0.0 85.1 158.1#
98 0.0 42.8 79.6#


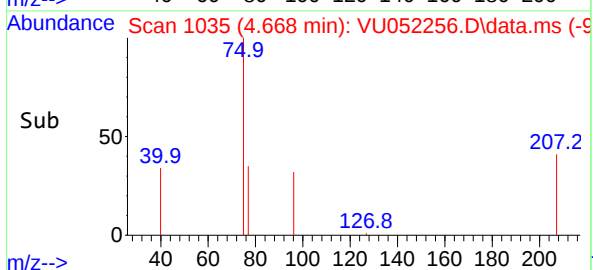






#23
Bromochloromethane
Concen: 0.919 ug/L
RT: 4.980 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion:	128	Resp:	62
Ion	Ratio	Lower	Upper
128	100		
49	0.0	104.0	193.2#
130	0.0	84.6	157.2#
51	0.0	38.1	57.1#

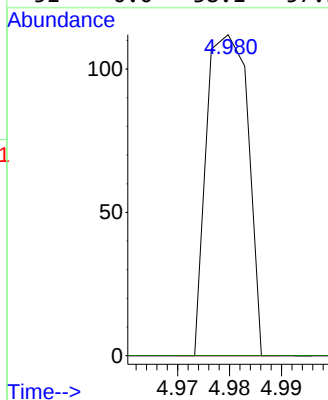

#25
Chloroform
Concen: 1438.401 ug/L
RT: 5.086 min Scan# 1165
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion:	83	Resp:	352987
Ion	Ratio	Lower	Upper
83	100		
85	63.8	43.8	81.4


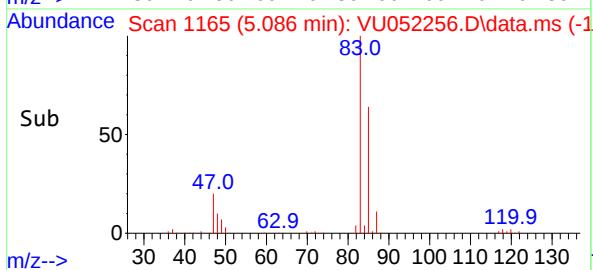
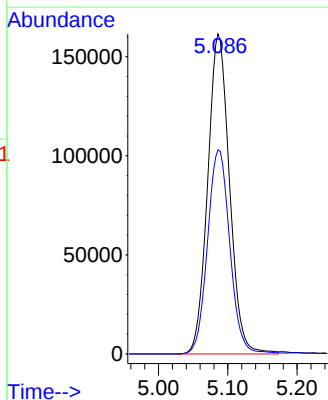





#27
1,2-Dichloroethane
Concen: 6.700 ug/L
RT: 5.793 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 62 Resp: 1007
Ion Ratio Lower Upper
62 100
98 0.0 8.4 12.6#



#30
Cyclohexane
Concen: 0.227 ug/L
RT: 5.391 min Scan# 1260
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 56 Resp: 50
Ion Ratio Lower Upper
56 100
69 0.0 25.6 38.4#
84 0.0 72.0 108.0#









#33
Benzene
Concen: 2.384 ug/L
RT: 5.777 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Instrument :
MSVOA_U
ClientSampleId :
EXZ84




Tgt Ion: 78 Resp: 1589




#34
Trichloroethene
Concen: 62.595 ug/L
RT: 6.542 min Scan# 1618
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 95 Resp: 10406

Ion	Ratio	Lower	Upper
95	100		
97	62.1	43.7	81.1
132	81.2	64.3	119.3
130	98.7	67.3	124.9


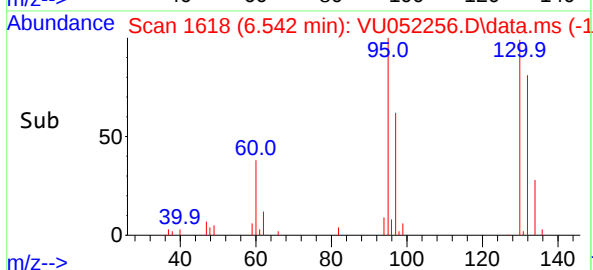
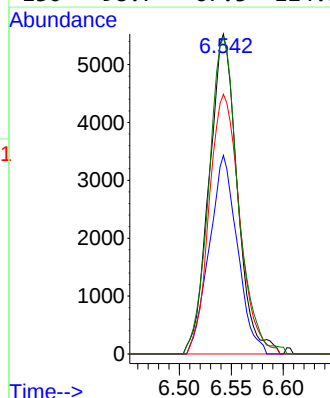





#38
Bromodichloromethane
Concen: 36.640 ug/L
RT: 7.102 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 83 Resp: 7709
Ion Ratio Lower Upper
83 100
85 65.5 43.5 80.9
127 14.0 6.8 10.2#



#40
4-Methyl-2-pentanone
Concen: 5.769 ug/L
RT: 7.800 min Scan# 2009
Delta R.T. 0.010 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 43 Resp: 520
Ion Ratio Lower Upper
43 100
58 0.0 35.3 52.9#
100 0.0 13.6 20.4#

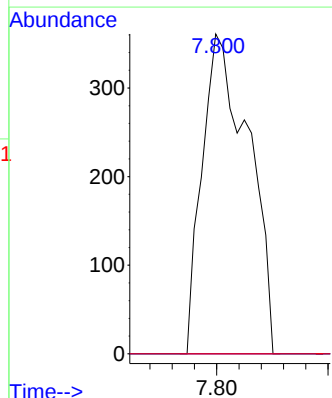



#42

Toluene

Concen: 16.858 ug/L

RT: 7.970 min Scan# 2061

Delta R.T. 0.003 min

Lab File: VU052256.D

Acq: 08 Dec 2022 18:10

Instrument :

MSVOA_U

ClientSampleId :





EXZ84

Tgt Ion: 91 Resp: 11558

Ion Ratio Lower Upper

91 100

92 55.4 40.7 75.5

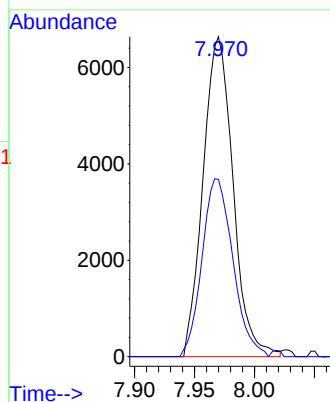

#48

2-Hexanone

Concen: 26.163 ug/L

RT: 8.687 min Scan# 2285

Delta R.T. 0.003 min

Lab File: VU052256.D

Acq: 08 Dec 2022 18:10

Tgt Ion: 43 Resp: 1729




Ion Ratio Lower Upper


43 100

58 47.6 49.4 74.0#

57 10.2 16.3 24.5#

100 0.0 10.4 15.6#

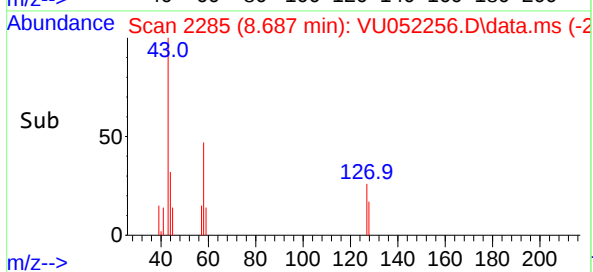



#49

Dibromochloromethane

Concen: 7.808 ug/L

RT: 8.812 min Scan# 21

Delta R.T. 0.006 min

Lab File: VU052256.D

Acq: 08 Dec 2022 18:10

Instrument :

MSVOA_U

ClientSampleId :





EXZ84

Tgt Ion:129 Resp: 1134

Ion Ratio Lower Upper

129 100

127 92.6 52.8 98.2

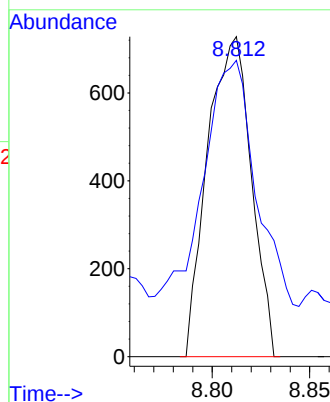

#51

Chlorobenzene

Concen: 2.235 ug/L

RT: 9.443 min Scan# 2520

Delta R.T. -0.003 min

Lab File: VU052256.D

Acq: 08 Dec 2022 18:10




Tgt Ion:112 Resp: 977


Ion Ratio Lower Upper

112 100

114 32.0 22.2 41.2

77 85.0 46.6 70.0#


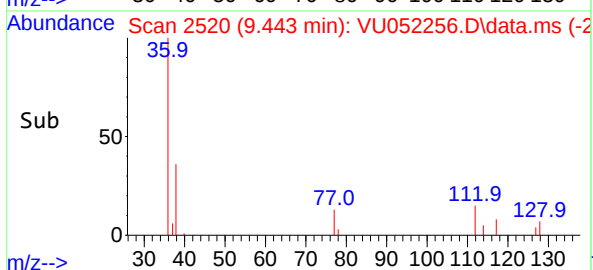






#52
Ethylbenzene
Concen: 2.462 ug/L
RT: 9.568 min Scan# 2559
Delta R.T. -0.000 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument : MSVOA_U
ClientSampleId : EXZ84


Tgt Ion: 91 Resp: 1641
Ion Ratio Lower Upper
91 100
106 34.7 22.3 41.3



#53
m,p-Xylene
Concen: 9.756 ug/L
RT: 9.690 min Scan# 2597
Delta R.T. -0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion: 106 Resp: 2518
Ion Ratio Lower Upper
106 100
91 182.5 137.7 255.7



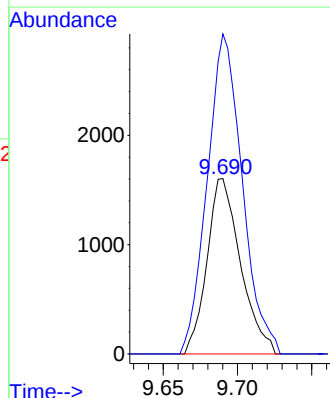





#54
o-Xylene
Concen: 2.357 ug/L
RT: 10.102 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion:106 Resp: 583
Ion Ratio Lower Upper
106 100
91 187.6 151.5 281.5

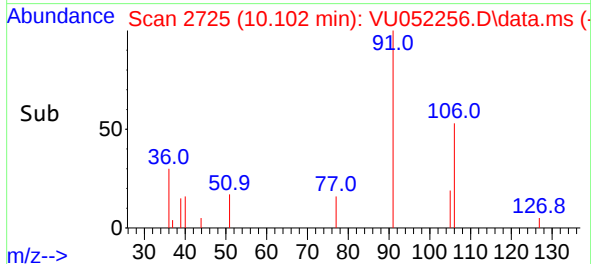

#60
Isopropylbenzene
Concen: 0.128 ug/L
RT: 10.095 min Scan# 2723
Delta R.T. -0.386 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion:105 Resp: 192
Ion Ratio Lower Upper
105 100
120 0.0 21.0 31.6#
77 36.5 12.5 18.7#


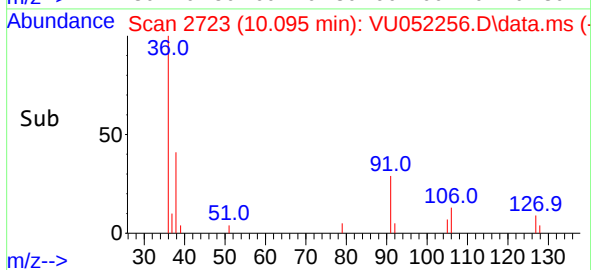

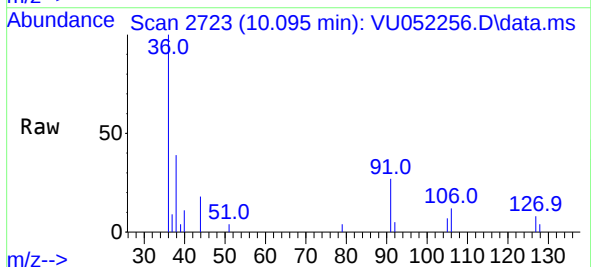




#61
1,2,3-Trichloropropane
Concen: 0.675 ug/L
RT: 11.812 min Scan# 31
Delta R.T. 0.993 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion: 75 Resp: 184
Ion Ratio Lower Upper
75 100
110 0.0 28.3 42.5#
77 0.0 26.2 39.2#

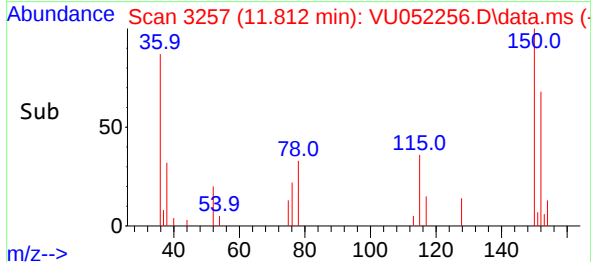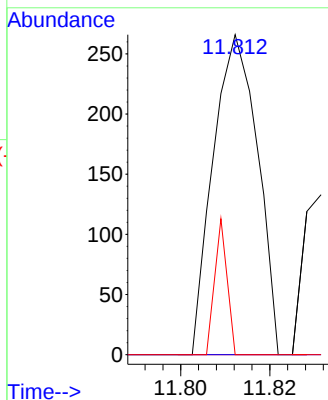

#64
1,3-Dichlorobenzene
Concen: 0.335 ug/L
RT: 11.825 min Scan# 3261
Delta R.T. 0.083 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Tgt Ion:146 Resp: 256
Ion Ratio Lower Upper
146 100
111 0.0 28.6 53.2#
148 59.5 45.4 84.2


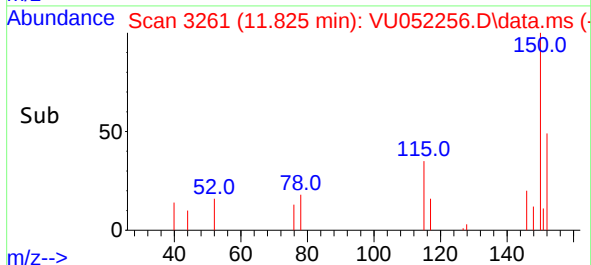
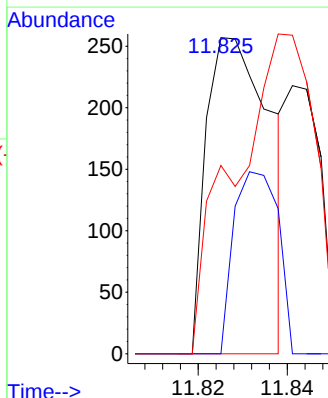
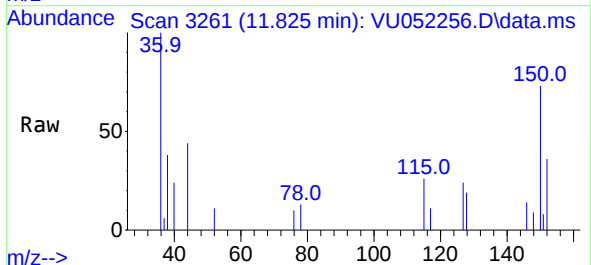


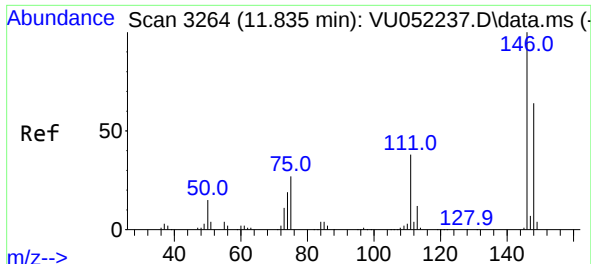

#65
1,4-Dichlorobenzene
Concen: 0.336 ug/L
RT: 11.825 min Scan# 31
Delta R.T. -0.007 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10




Instrument :
MSVOA_U
ClientSampleId :
EXZ84


Tgt Ion:146 Resp: 256
Ion Ratio Lower Upper
146 100
111 0.0 26.9 50.1#
148 59.5 45.1 83.7

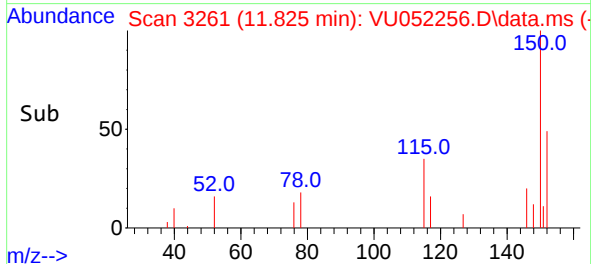

#67
1,2-Dichlorobenzene
Concen: 2.091 ug/L
RT: 12.211 min Scan# 3381
Delta R.T. 0.003 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10


Tgt Ion:146 Resp: 1538
Ion Ratio Lower Upper
146 100
111 35.5 32.7 49.1
148 74.0 50.6 75.8

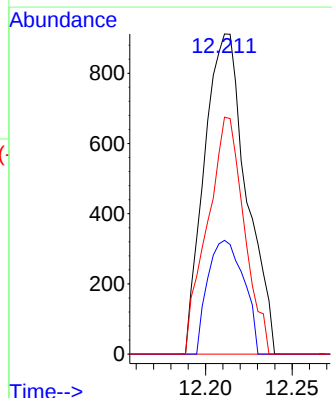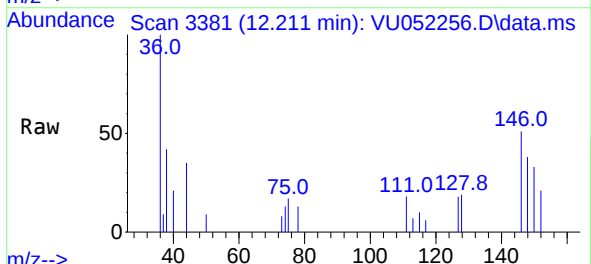



#71
Naphthalene
Concen: 0.297 ug/L
RT: 14.095 min Scan# 3967
Delta R.T. 0.013 min
Lab File: VU052256.D
Acq: 08 Dec 2022 18:10

Instrument :
MSVOA_U
ClientSampleId :
EXZ84



Tgt Ion:128 Resp: 230
Ion Ratio Lower Upper
128 100
129 0.0 8.3 12.5#
127 198.3 10.2 15.4#

