


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052270.D
Acq On : 09 Dec 2022 00:15
Operator : JC/MD
Sample : N5958-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EL7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/09/2022
Supervised By :Mahesh Dadoda 12/09/2022

Quant Time: Dec 09 01:23:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

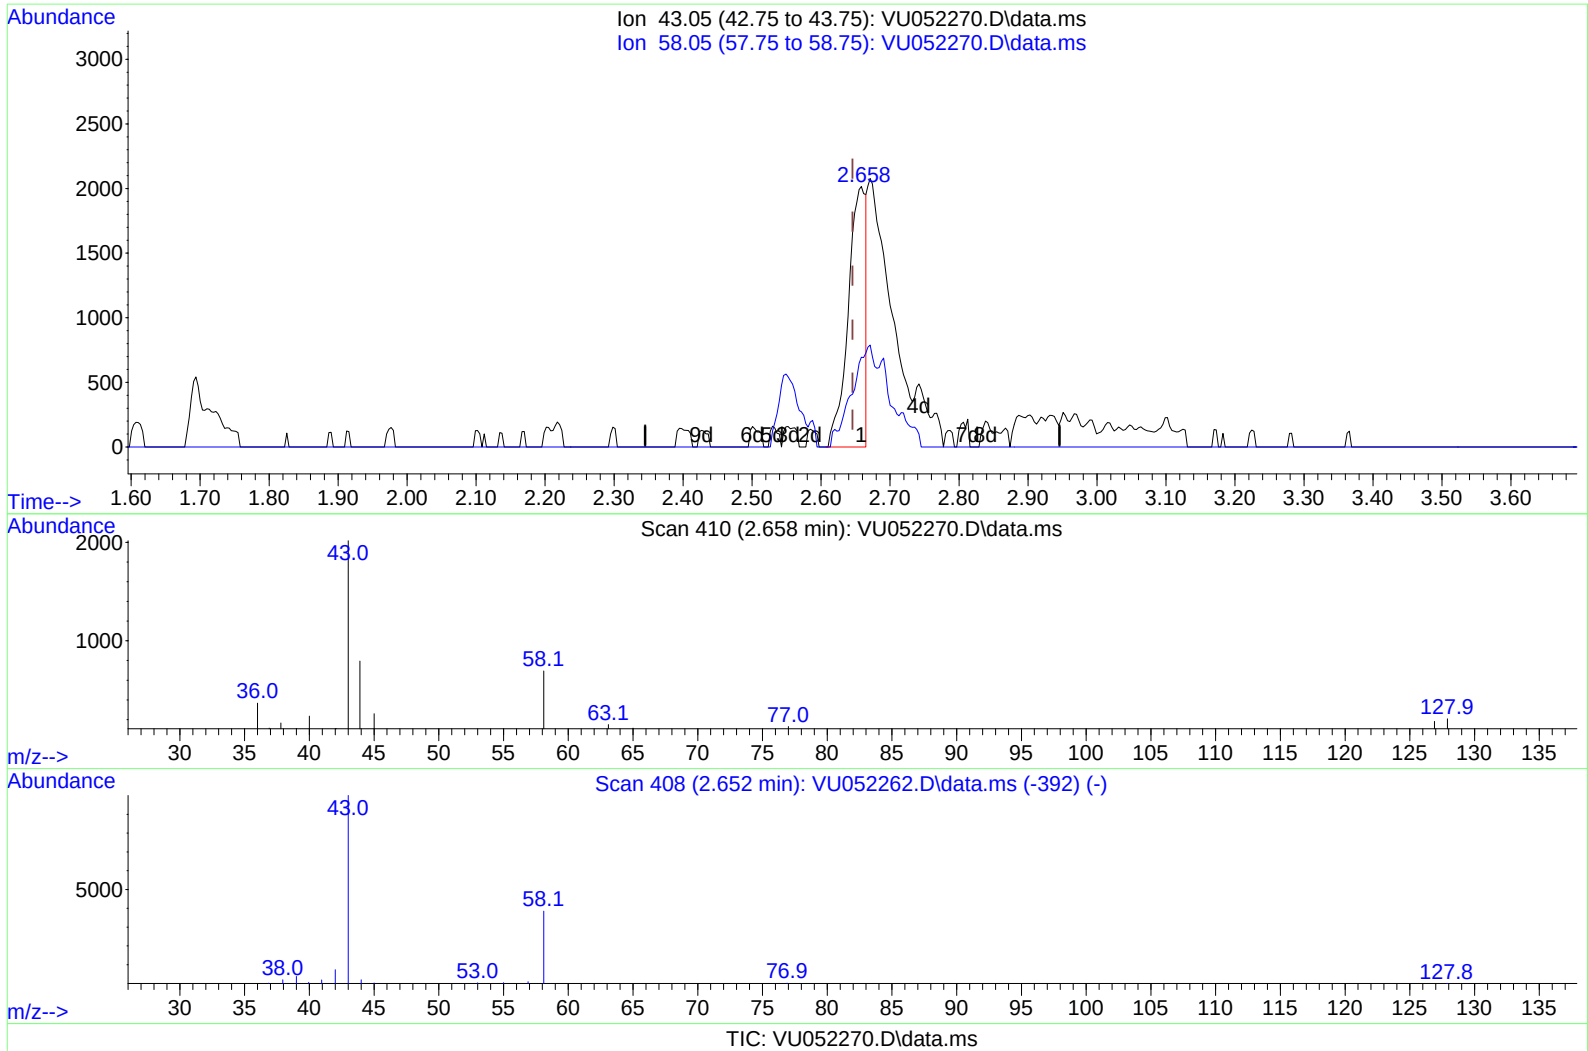

(13) Acetone (T)

2.658min (+ 0.013) 1.45 ug/L

response	3561	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	52.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
 Data File : VU052270.D
 Acq On : 09 Dec 2022 00:15
 Operator : JC/MD
 Sample : N5958-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EL7

Manual IntegrationsAPPROVED

Quant Time: Dec 09 01:23:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/09/2022
 Supervised By :Mahesh Dadoda 12/09/2022

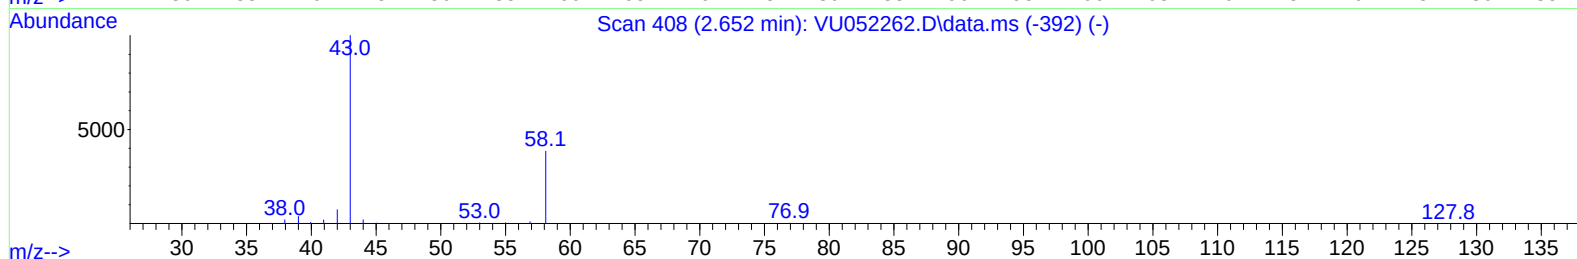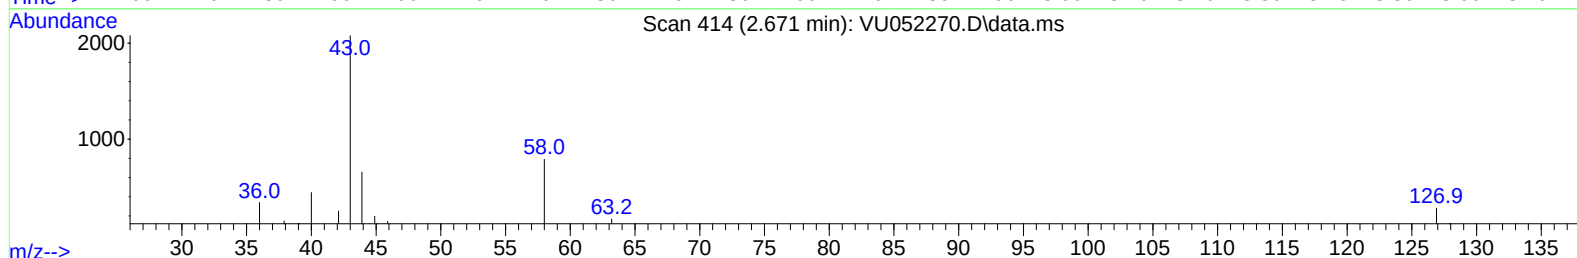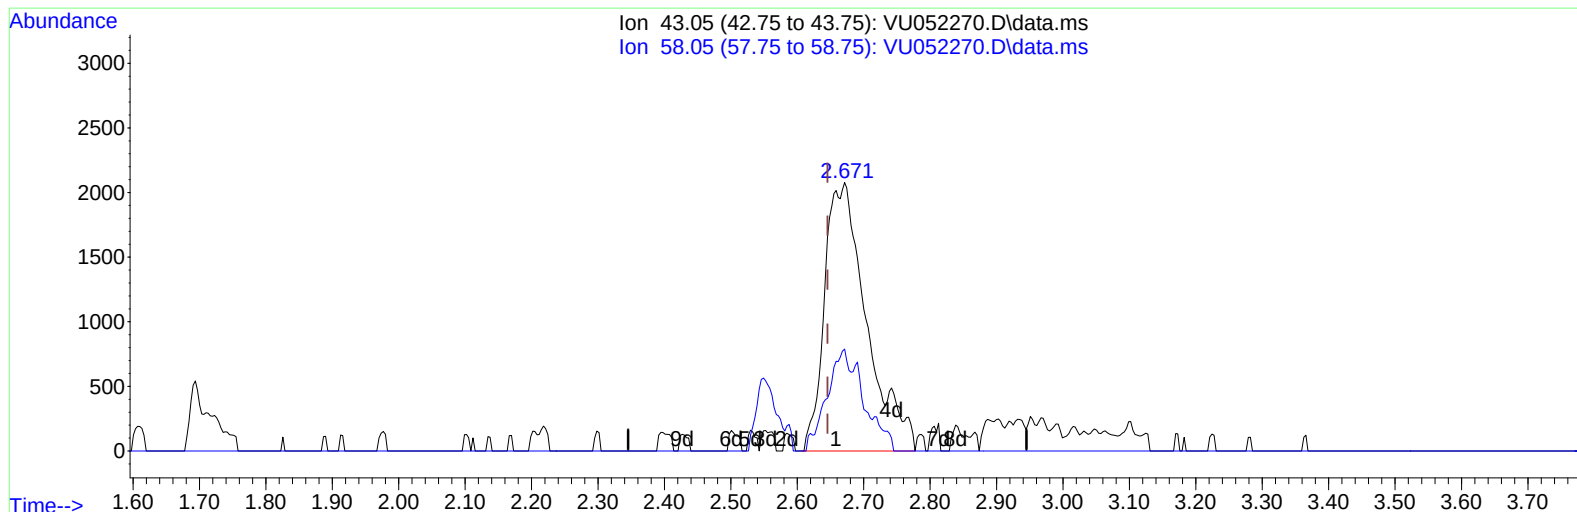

TIC: VU052270.D\data.ms

(13) Acetone (T)

2.671min (+ 0.026) 3.72 ug/L m

response 9100

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	20.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
 Data File : VU052270.D
 Acq On : 09 Dec 2022 00:15
 Operator : JC/MD
 Sample : N5958-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EL7

Manual IntegrationsAPPROVED

Quant Time: Dec 09 01:23:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/09/2022
 Supervised By :Mahesh Dadoda 12/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	204433	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	214449	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	92176	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	65962	3.317	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	66.400%	
7) Chloroethane-d5	1.916	69	64093	4.150	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.000%	
11) 1,1-Dichloroethene-d2	2.568	65	27619	3.875	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.400%	
20) 2-Butanone-d5	4.642	46	235783	65.414	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	130.820%#	
24) Chloroform-d	5.063	84	143994	4.928	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.700	65	76917	5.212	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.200%	
32) Benzene-d6	5.726	84	277026	4.351	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	6.687	67	97134	4.930	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.600%	
41) Toluene-d8	7.896	98	210672	3.657	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...	8.176	79	28453	3.963	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.200%	
46) 2-Hexanone-d5	8.632	63	161142	52.959	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.920%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	92498	5.415	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	108.200%	
66) 1,2-Dichlorobenzene-d4	12.189	152	86580	4.906	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.200%	
Target Compounds						
13) Acetone	2.671	43	9100m	3.718	ug/L	
25) Chloroform	5.086	83	52482	1.808	ug/L	93
34) Trichloroethene	6.542	95	10103	0.580	ug/L	98
38) Bromodichloromethane	7.105	83	8083	0.367	ug/L #	97
49) Dibromochloromethane	8.806	129	7738	0.509	ug/L	99
59) Bromoform	10.288	173	6452	0.850	ug/L #	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052270.D
Acq On : 09 Dec 2022 00:15
Operator : JC/MD
Sample : N5958-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EL7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 12/09/2022
Supervised By :Mahesh Dadoda 12/09/2022

Quant Time: Dec 09 01:23:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

