

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
 Data File : VU052247.D
 Acq On : 08 Dec 2022 14:34
 Operator : JC/MD
 Sample : N5918-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	52	57	66	rBV	6273	8641	1.01%	0.125%
2	1.600	73	81	95	rVB	114645	133954	15.66%	1.940%
3	1.916	171	179	194	rBV	94035	131216	15.34%	1.900%
4	2.568	368	382	396	rVB	177317	290806	34.01%	4.211%
5	4.665	1014	1034	1074	rBV2	85127	397478	46.48%	5.755%
6	5.063	1141	1158	1186	rBV	171230	392422	45.89%	5.682%
7	5.726	1342	1364	1387	rBV2	319376	855119	100.00%	12.382%
8	6.247	1513	1526	1554	rBV	240084	473286	55.35%	6.853%
9	6.533	1590	1615	1617	rBV2	37849	151429	17.71%	2.193%
10	6.690	1653	1664	1680	rBV	208074	401654	46.97%	5.816%
11	7.565	1927	1936	1953	rVB	86360	156094	18.25%	2.260%
12	7.896	2028	2039	2062	rVB	355419	612871	71.67%	8.874%
13	8.179	2118	2127	2138	rVB2	52427	91556	10.71%	1.326%
14	8.645	2260	2272	2312	rBV2	272902	801917	93.78%	11.612%
15	9.414	2500	2511	2529	rVB	362653	602403	70.45%	8.723%
16	10.754	2911	2928	2942	rBV	192023	317209	37.10%	4.593%
17	11.809	3244	3256	3280	rBV	319922	522106	61.06%	7.560%
18	12.066	3330	3336	3346	rVB6	5432	8769	1.03%	0.127%
19	12.188	3362	3374	3392	rBV	335074	557281	65.17%	8.069%




Sum of corrected areas: 6906211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052247.D
Acq On : 08 Dec 2022 14:34
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

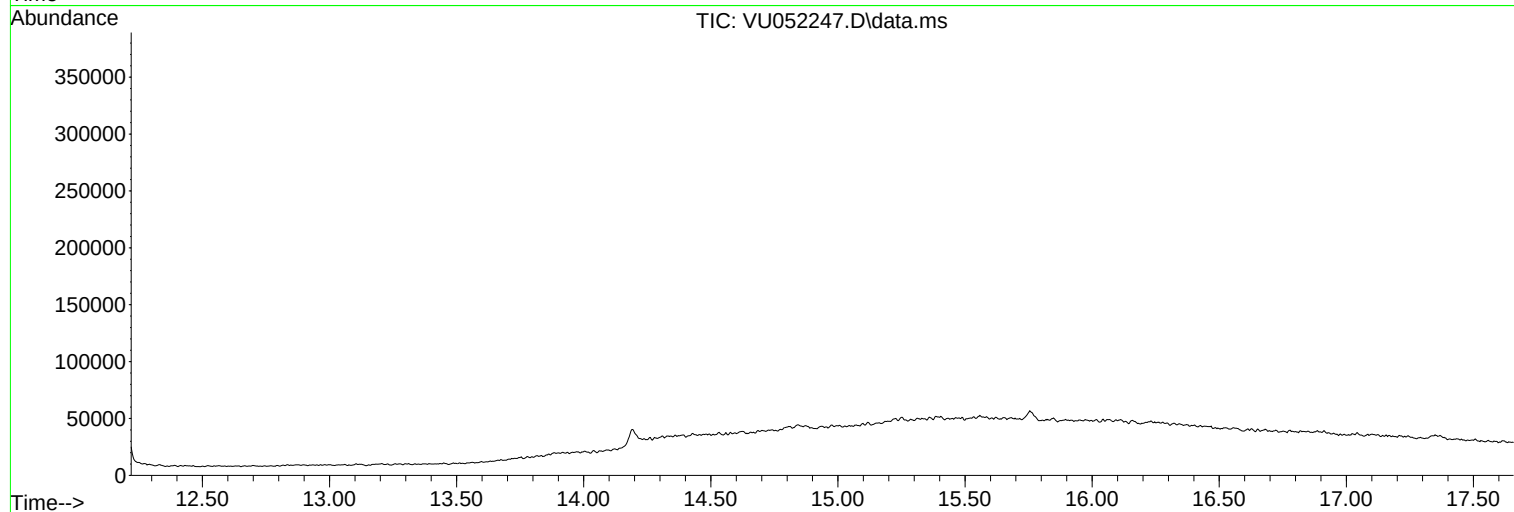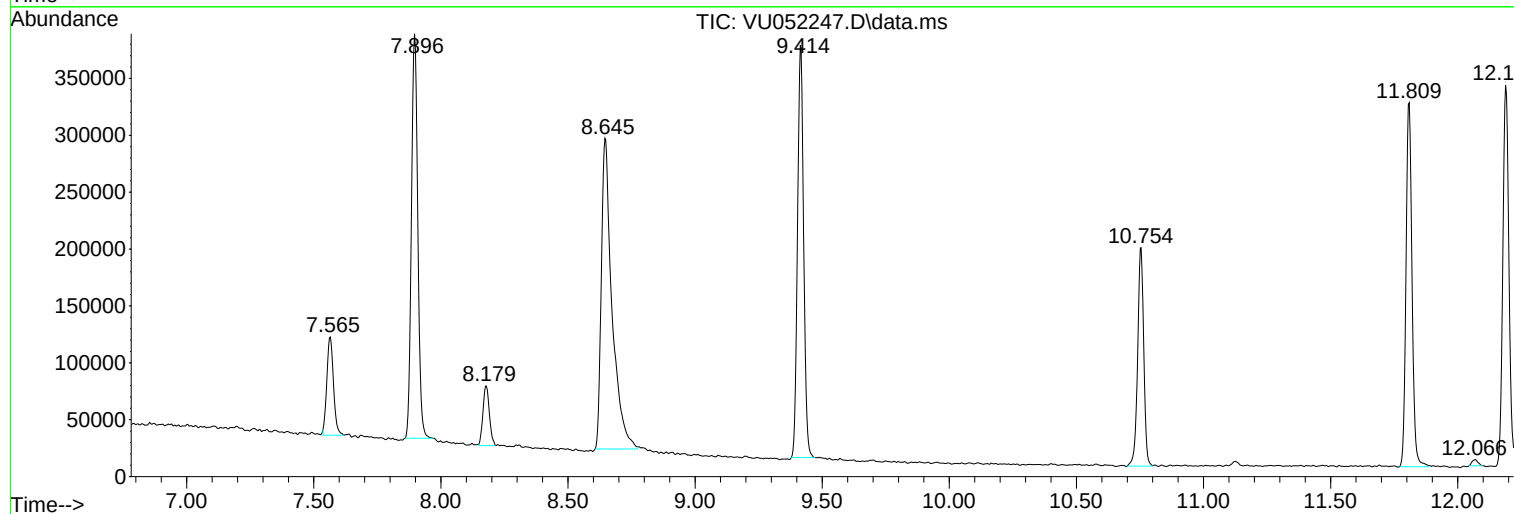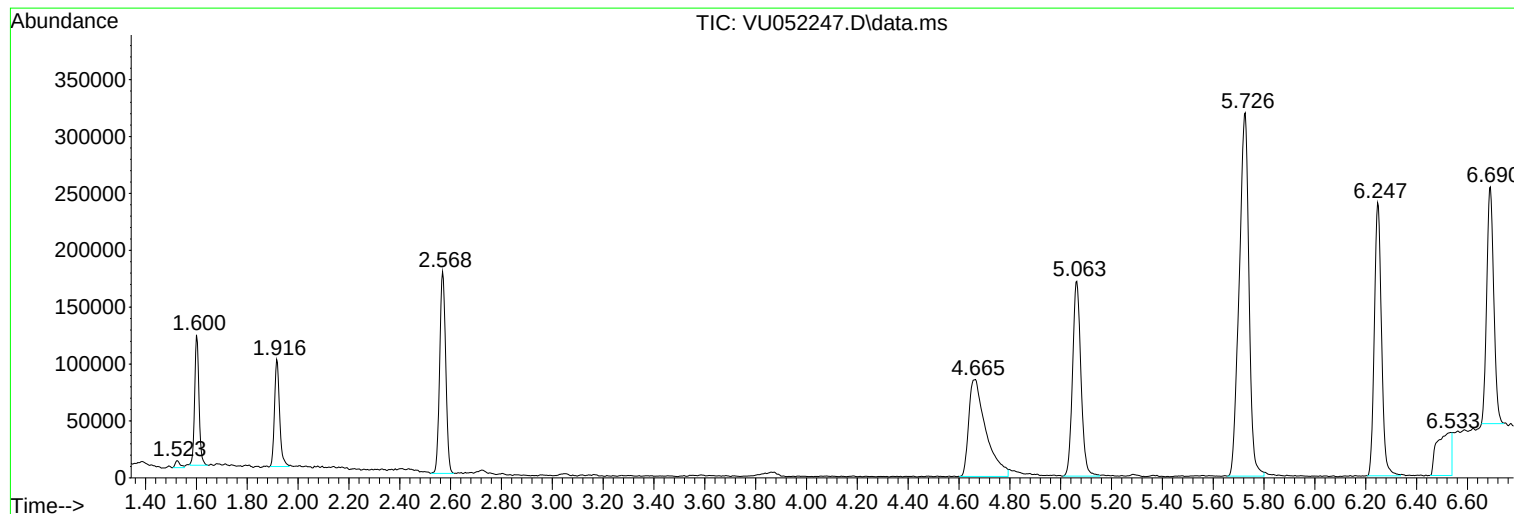

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052247.D
Acq On : 08 Dec 2022 14:34
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.533	1.60 ug/L	151429	1,4-Difluorobenzene	6.247

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hydrogen chloride	36	ClH	007647-01-0	9
2			Hydrogen chloride	36	ClH	007647-01-0	9
3			Ammonium Chloride	53	ClH4N	012125-02-9	4
4			Methanol-D4	36	CD4O	000811-98-3	2
5			1H-Imidazole-1-ethanol, .alpha.-...	126	C6H10N2O	037788-55-9	2

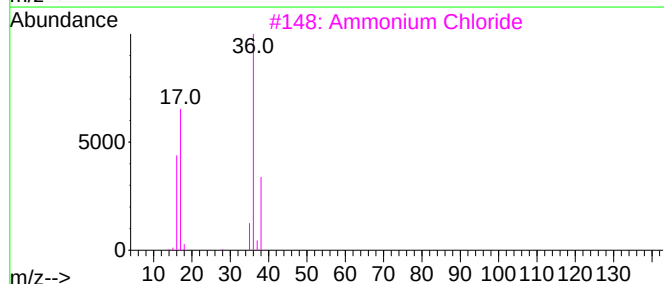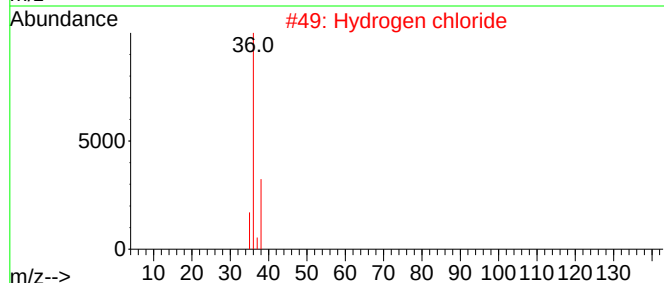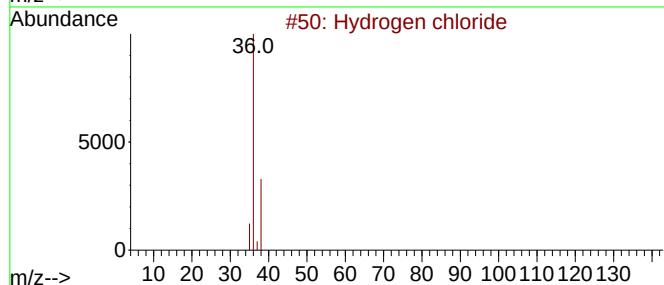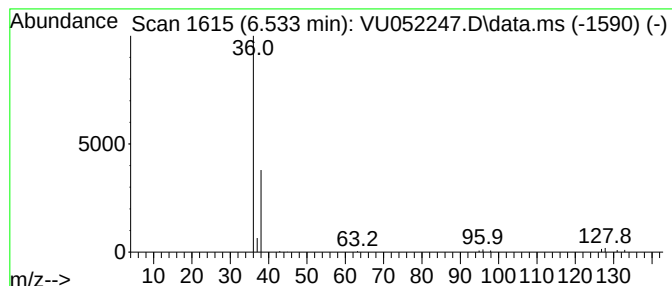

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052247.D
Acq On : 08 Dec 2022 14:34
Operator : JC/MD
Sample : N5918-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.533	1.6	ug/L	151429	1	6.247	473286	5.0