
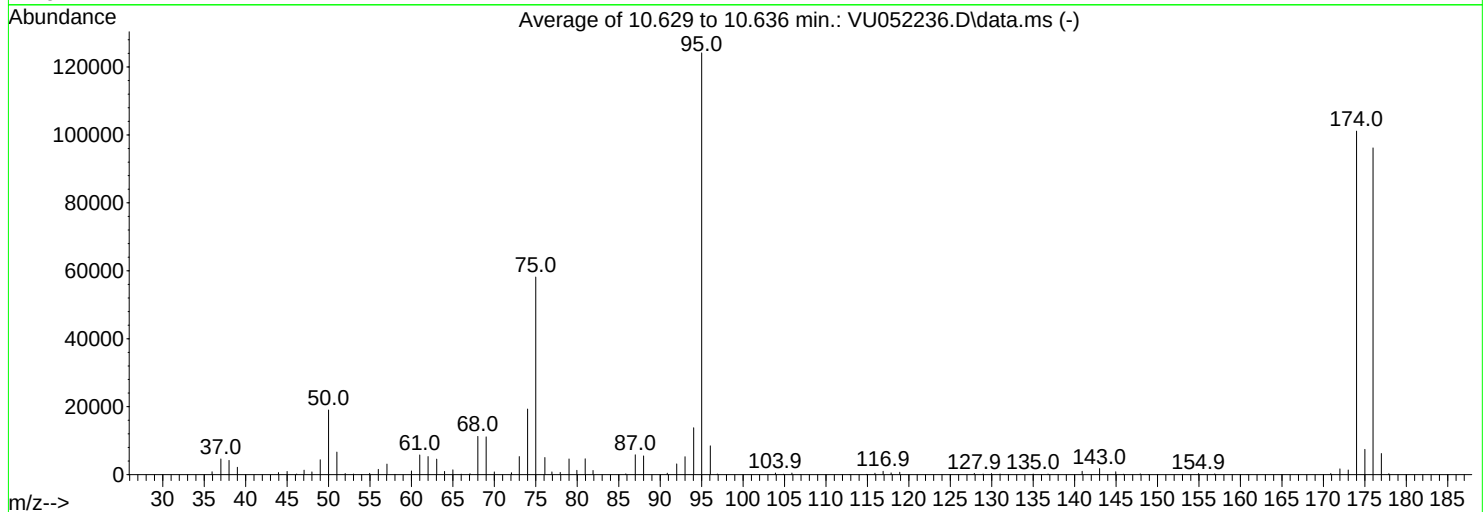


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120822\
Data File : VU052236.D
Acq On : 08 Dec 2022 09:36
Operator : JC/MD
Sample : BFB175
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB175

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 08 04:19:43 2022

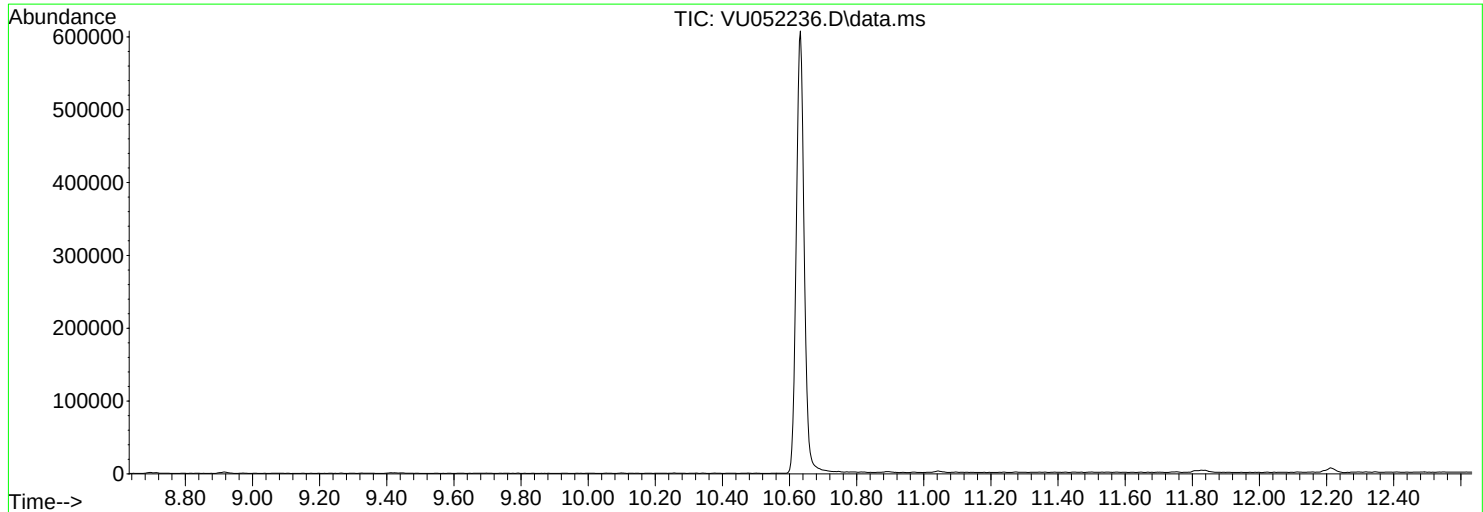

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	19040	PASS
75	95	30	80	46.9	58171	PASS
95	95	100	100	100.0	124155	PASS
96	95	5	9	6.8	8457	PASS
173	174	0.00	2	1.3	1356	PASS
174	95	50	120	81.4	101104	PASS
175	174	5	9	7.4	7434	PASS
176	174	95	101	95.1	96160	PASS
177	176	5	9	6.5	6233	PASS

Scan 2875 (10.584 min): VU052236.D\data.ms
BFB175

m/z	Abundance
40.00	348.0
43.90	478.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
36.00	849.0
37.00	4570.0
38.00	4503.0
39.00	2042.0
39.90	283.0
44.00	1100.0
45.00	978.0
46.10	178.0
47.10	1326.0
48.00	898.0
49.00	4381.0
50.00	19312.0
51.00	6663.0
52.00	285.0
53.00	178.0
54.00	111.0
55.00	415.0
56.00	1671.0
57.00	3353.0
60.00	1146.0
61.00	5834.0
62.00	5429.0
63.00	4854.0
64.00	1047.0
65.00	1345.0
66.00	154.0
67.00	263.0
68.00	11707.0
69.00	11464.0
70.00	867.0
72.10	570.0
73.00	5546.0
74.00	19704.0
75.00	59440.0
76.10	5339.0
76.90	783.0
78.00	711.0
79.00	4615.0
79.90	1188.0
81.00	4898.0
81.90	1233.0
85.90	243.0
87.00	5870.0
88.00	5411.0
90.90	454.0
92.00	3312.0
93.00	5286.0
94.00	13690.0
95.00	125696.0
96.00	8881.0
96.90	230.0
103.90	469.0
104.90	114.0
105.90	488.0
112.90	135.0
115.90	451.0
116.90	1107.0
117.90	482.0
118.90	649.0
127.90	347.0
128.90	178.0
129.90	360.0
131.00	159.0
135.00	163.0
136.80	181.0
140.90	1114.0
143.00	1867.0
144.90	875.0
145.90	160.0
147.90	229.0
148.90	100.0
150.00	109.0
155.00	308.0
156.90	195.0
160.80	111.0
170.90	346.0
172.00	1596.0
173.00	1320.0
174.00	99968.0
175.00	7316.0
176.00	96496.0
177.00	6465.0
177.90	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
36.00	855.0
37.00	4763.0
38.00	4328.0
39.00	2268.0
39.90	271.0
44.00	1142.0
45.00	990.0
46.20	189.0
47.10	1355.0
48.00	835.0
49.00	4489.0
50.00	19664.0
51.00	6923.0
52.00	320.0
53.00	209.0
54.00	113.0
54.90	372.0
56.00	1619.0
57.00	3198.0
58.00	117.0
60.00	1100.0
61.00	6032.0
62.00	5467.0
63.00	4629.0
64.00	1003.0
65.00	1438.0
66.00	160.0
67.10	267.0
68.00	11650.0
69.00	11378.0
70.00	852.0
72.00	560.0
73.00	5575.0
74.00	19840.0
75.00	60216.0
76.10	5290.0
76.90	791.0
77.90	682.0
79.00	4821.0
79.90	1272.0
81.00	4820.0
81.90	1252.0
85.80	256.0
87.00	6135.0
88.00	5676.0
90.90	436.0
92.00	3176.0
93.00	5419.0
94.00	14310.0
95.00	128672.0
96.10	8654.0
96.90	201.0
103.90	499.0
104.90	149.0
105.90	466.0
114.90	155.0
115.90	451.0
116.90	1050.0
117.90	509.0
118.90	695.0
127.90	387.0
129.00	191.0
130.00	346.0
131.00	207.0
135.00	181.0
136.80	201.0
140.90	994.0
143.00	1836.0
145.00	862.0
145.90	157.0
147.90	236.0
150.00	103.0
153.00	122.0
155.00	316.0
156.90	246.0
160.80	102.0
170.90	334.0
172.00	1771.0
173.00	1453.0
174.00	104320.0
175.00	7652.0
176.00	99328.0
177.00	6413.0
177.90	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175

m/z	Abundance
35.90	806.0
37.00	4503.0
38.00	3824.0
39.00	2194.0
40.00	288.0
44.00	1088.0
45.00	929.0
46.20	146.0
47.00	1258.0
48.00	653.0
49.00	4212.0
50.00	18144.0
51.00	6412.0
52.00	353.0
53.00	215.0
55.00	328.0
56.00	1332.0
57.10	2726.0
58.00	121.0
60.00	1031.0
61.00	5585.0
62.00	5136.0
63.10	4254.0
64.00	813.0
65.00	1447.0
66.00	156.0
67.10	261.0
68.00	10423.0
69.00	10495.0
70.00	761.0
72.00	549.0
73.00	4899.0
74.00	18408.0
75.00	54856.0
76.10	4503.0
77.00	768.0
77.90	613.0
79.00	4388.0
80.00	1306.0
80.90	4284.0
81.90	1207.0
85.80	204.0
87.00	5567.0
88.00	5408.0
90.80	364.0
92.00	2973.0
93.00	5142.0
94.10	13452.0
95.00	118096.0
96.10	7837.0
96.90	172.0
103.90	481.0
104.90	194.0
105.90	431.0
106.90	106.0
114.90	179.0
115.90	376.0
116.90	888.0
117.80	529.0
118.90	725.0
127.90	393.0
129.00	191.0
130.00	305.0
131.00	250.0
135.00	161.0
136.80	130.0
140.90	908.0
143.00	1713.0
145.00	845.0
145.90	142.0
147.90	200.0
153.00	118.0
154.90	302.0
156.90	273.0
170.90	299.0
172.00	1778.0
173.00	1296.0
174.00	99024.0
175.00	7334.0
176.00	92656.0
177.00	5820.0
177.90	283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB175